
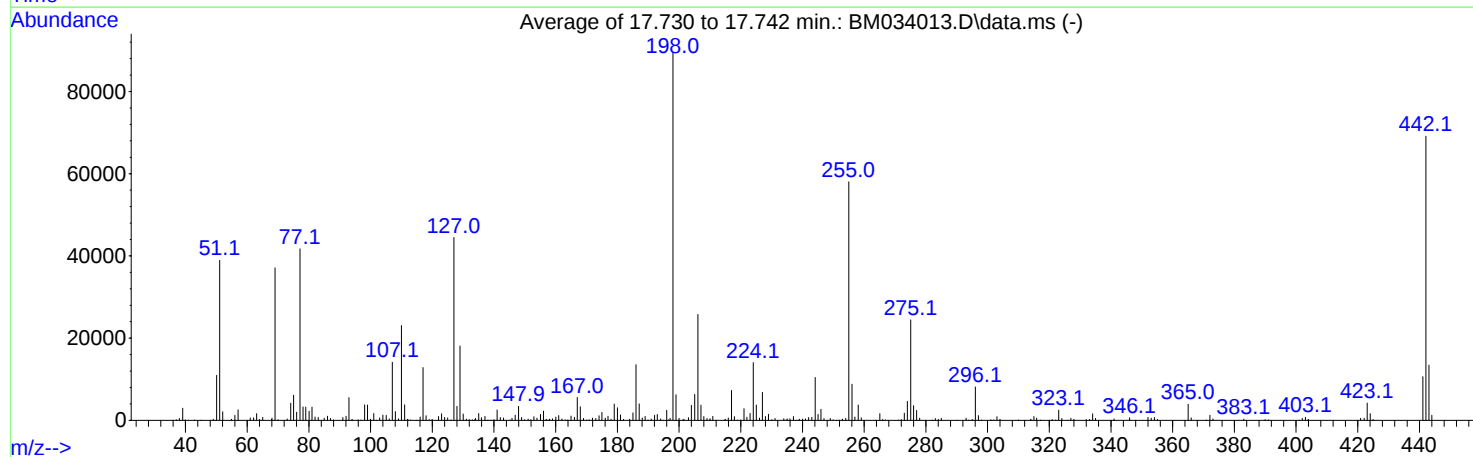


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020422\
 Data File : BM034013.D
 Acq On : 04 Feb 2022 11:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 04 17:33:01 2022

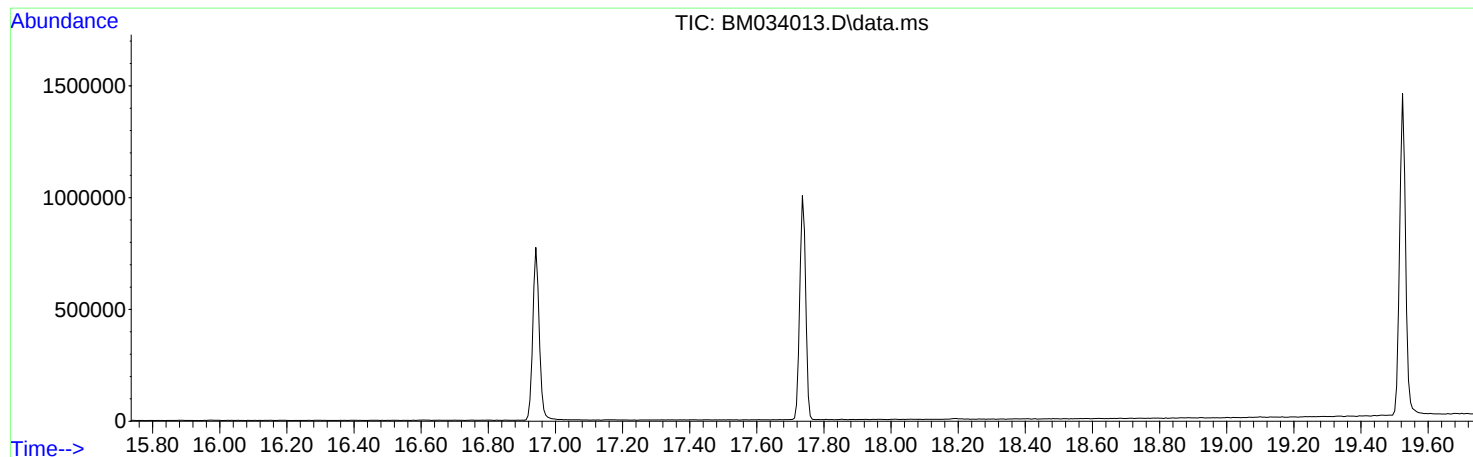




AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.5	38939	PASS
68	69	0.00	2	1.4	530	PASS
69	198	0.00	100	41.4	37091	PASS
70	69	0.00	2	0.4	138	PASS
127	198	10	80	49.7	44491	PASS
197	198	0.00	2	0.5	463	PASS
198	198	100	100	100.0	89491	PASS
199	198	5	9	6.9	6217	PASS
275	198	10	60	27.3	24451	PASS
365	198	1	100	4.4	3947	PASS
441	198	0.01	100	11.9	10643	PASS
442	442	50	100	100.0	69123	PASS
443	442	15	24	19.4	13424	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020422\
 Data File : BM034013.D
 Acq On : 04 Feb 2022 11:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Feb 04 16:34:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 04 16:34:01 2022
 Response via : Initial Calibration

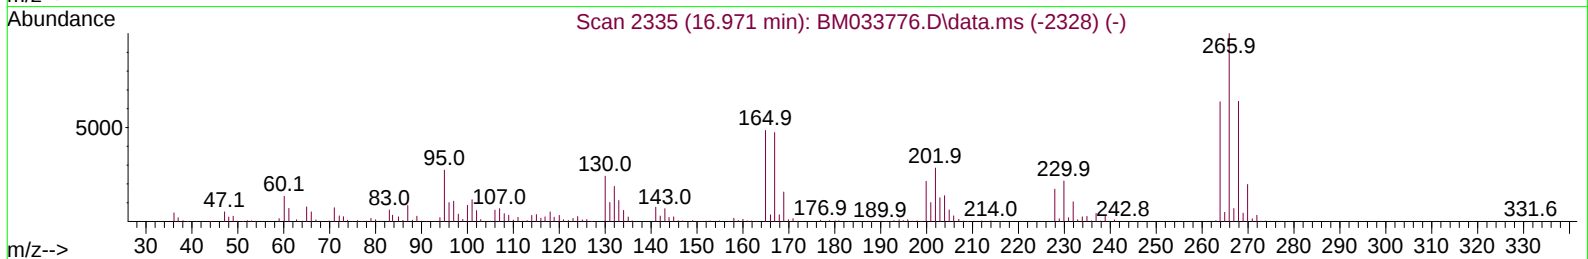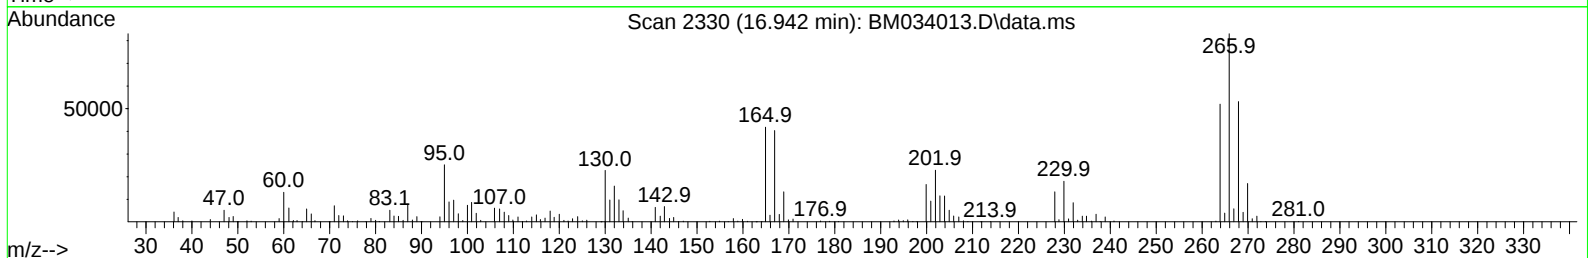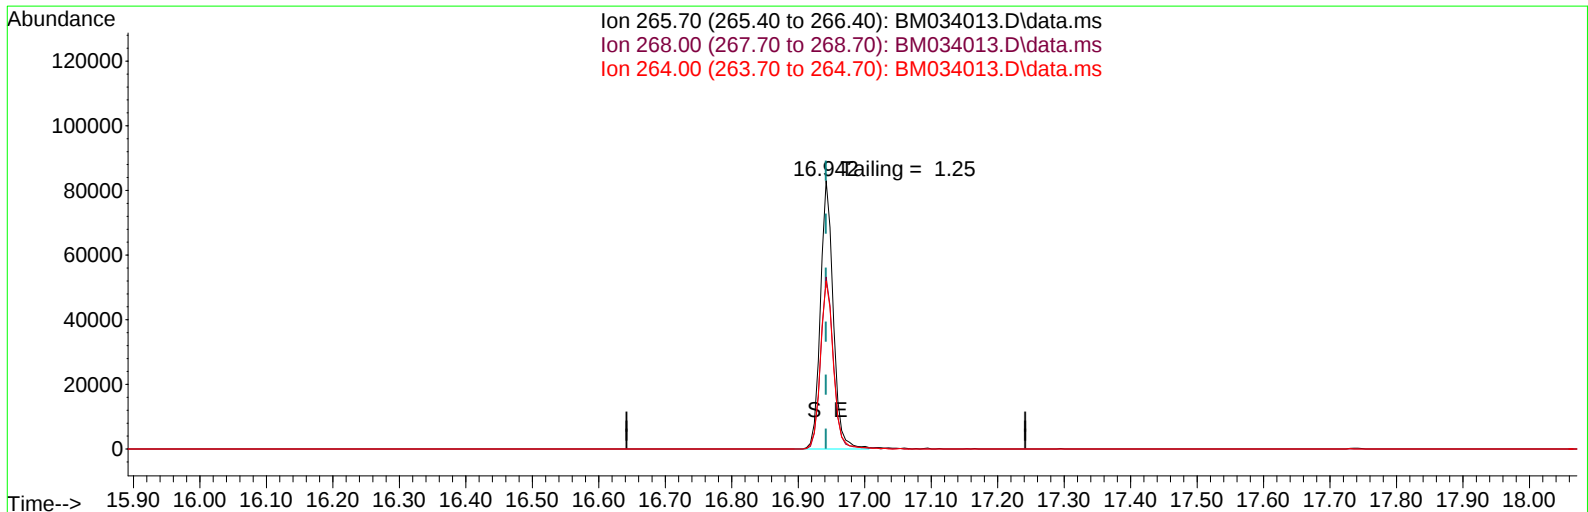

TIC: BM034013.D\data.ms

(70) Pentachlorophenol (C)

16.942min (0.000) 0.00 ng




response 112699

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.02
264.00	61.40	62.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020422\
 Data File : BM034013.D
 Acq On : 04 Feb 2022 11:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Feb 04 16:34:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 04 16:34:01 2022
 Response via : Initial Calibration

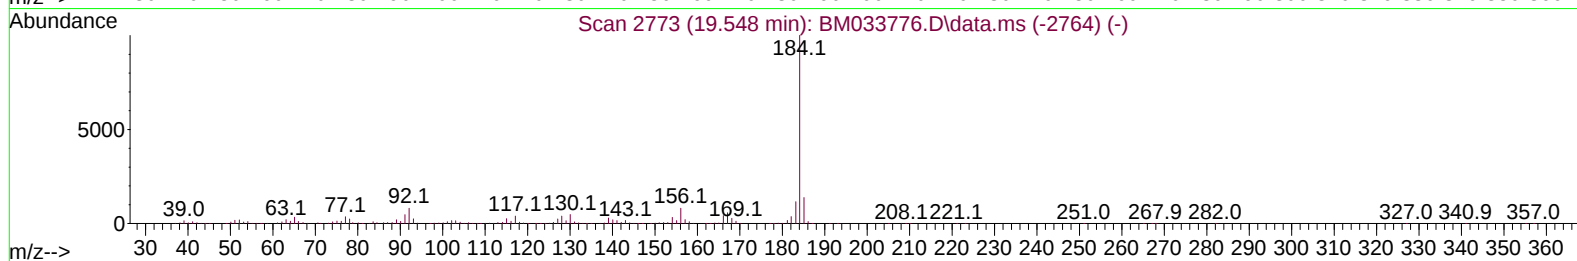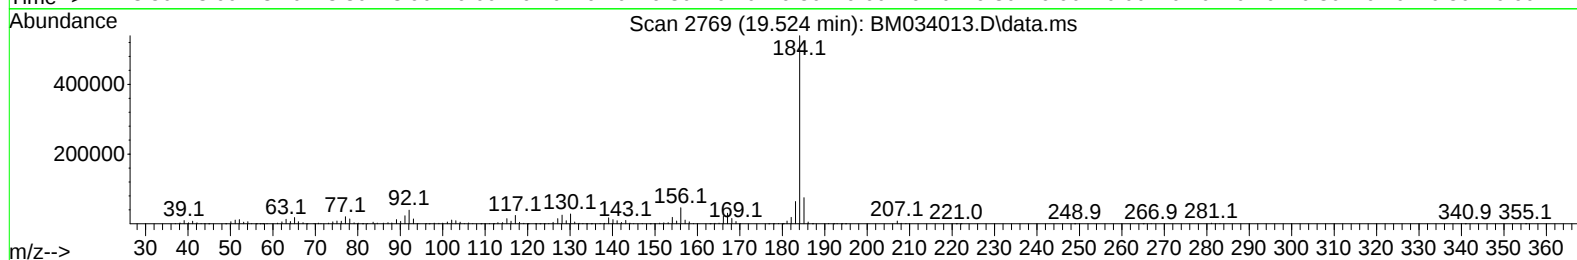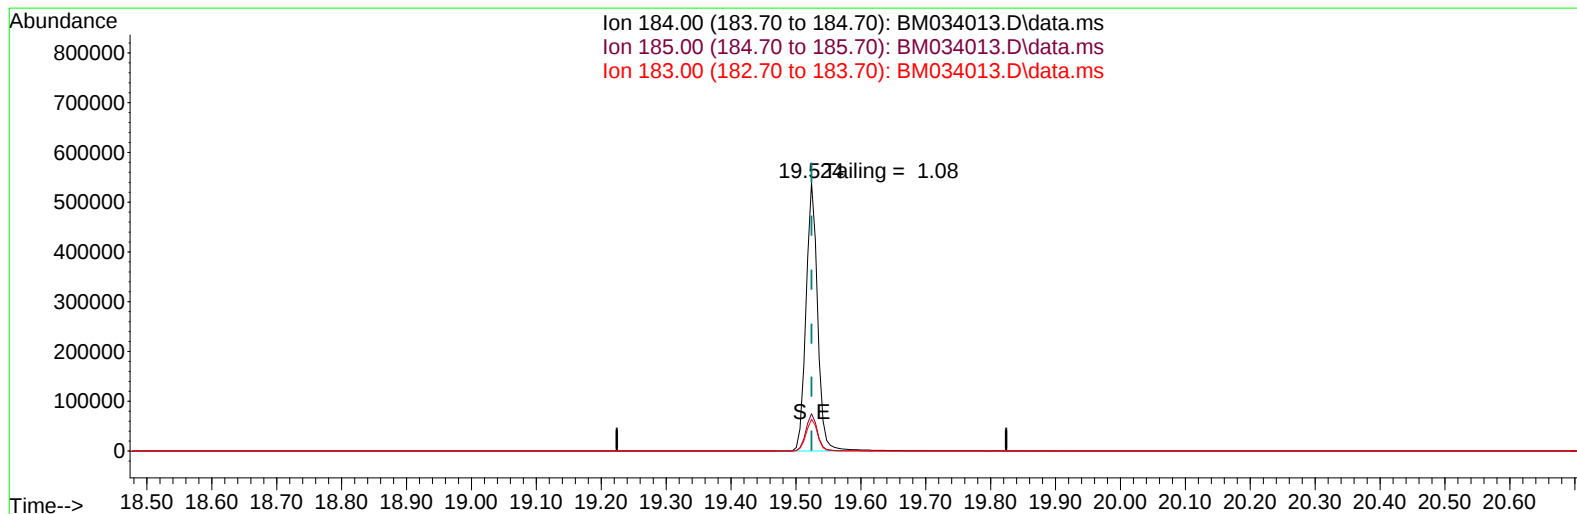

TIC: BM034013.D\data.ms

(77) Benzidine

19.524min (0.000) 0.00 ng

response 672230

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.89
183.00	12.10	11.85
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/4/2022	BNA_M	<u>BM034013.D</u>
Compound Name	Response	Retention Time
DDT	326084	20.75
DDD	256	20.31
DDE	0	19.9
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
256	326340	0.08

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP