

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020515\
 Data File : BM000428.D
 Acq On : 05 Feb 2015 13:28
 Operator : TP/IZ
 Sample : SSTD3.279
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Feb 05 14:08:52 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM020515.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 05 13:55:34 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	2304	0.40	ng/ul	0.00
2) Naphthalene-d8	10.51	136	7636	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.38	164	4716	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.12	188	9136	0.40	ng/ul	0.00
16) Chrysene-d12	21.31	240	8558	0.40	ng/ul	0.00
20) Perylene-d12	23.55	264	7268	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	0.00	152	0d	0.00	ng/ul	
14) Fluoranthene-d10	0.00	212	0d	0.00	ng/ul	
Target Compounds						
11) Pentachlorophenol	16.78	266	7407	3.57	ng/ul	Qvalue 98




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020515\
Data File : BM000428.D
Acq On : 05 Feb 2015 13:28
Operator : TP/IZ
Sample : SST3.279
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Feb 05 14:08:52 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM020515.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 05 13:55:34 2015
Response via : Initial Calibration

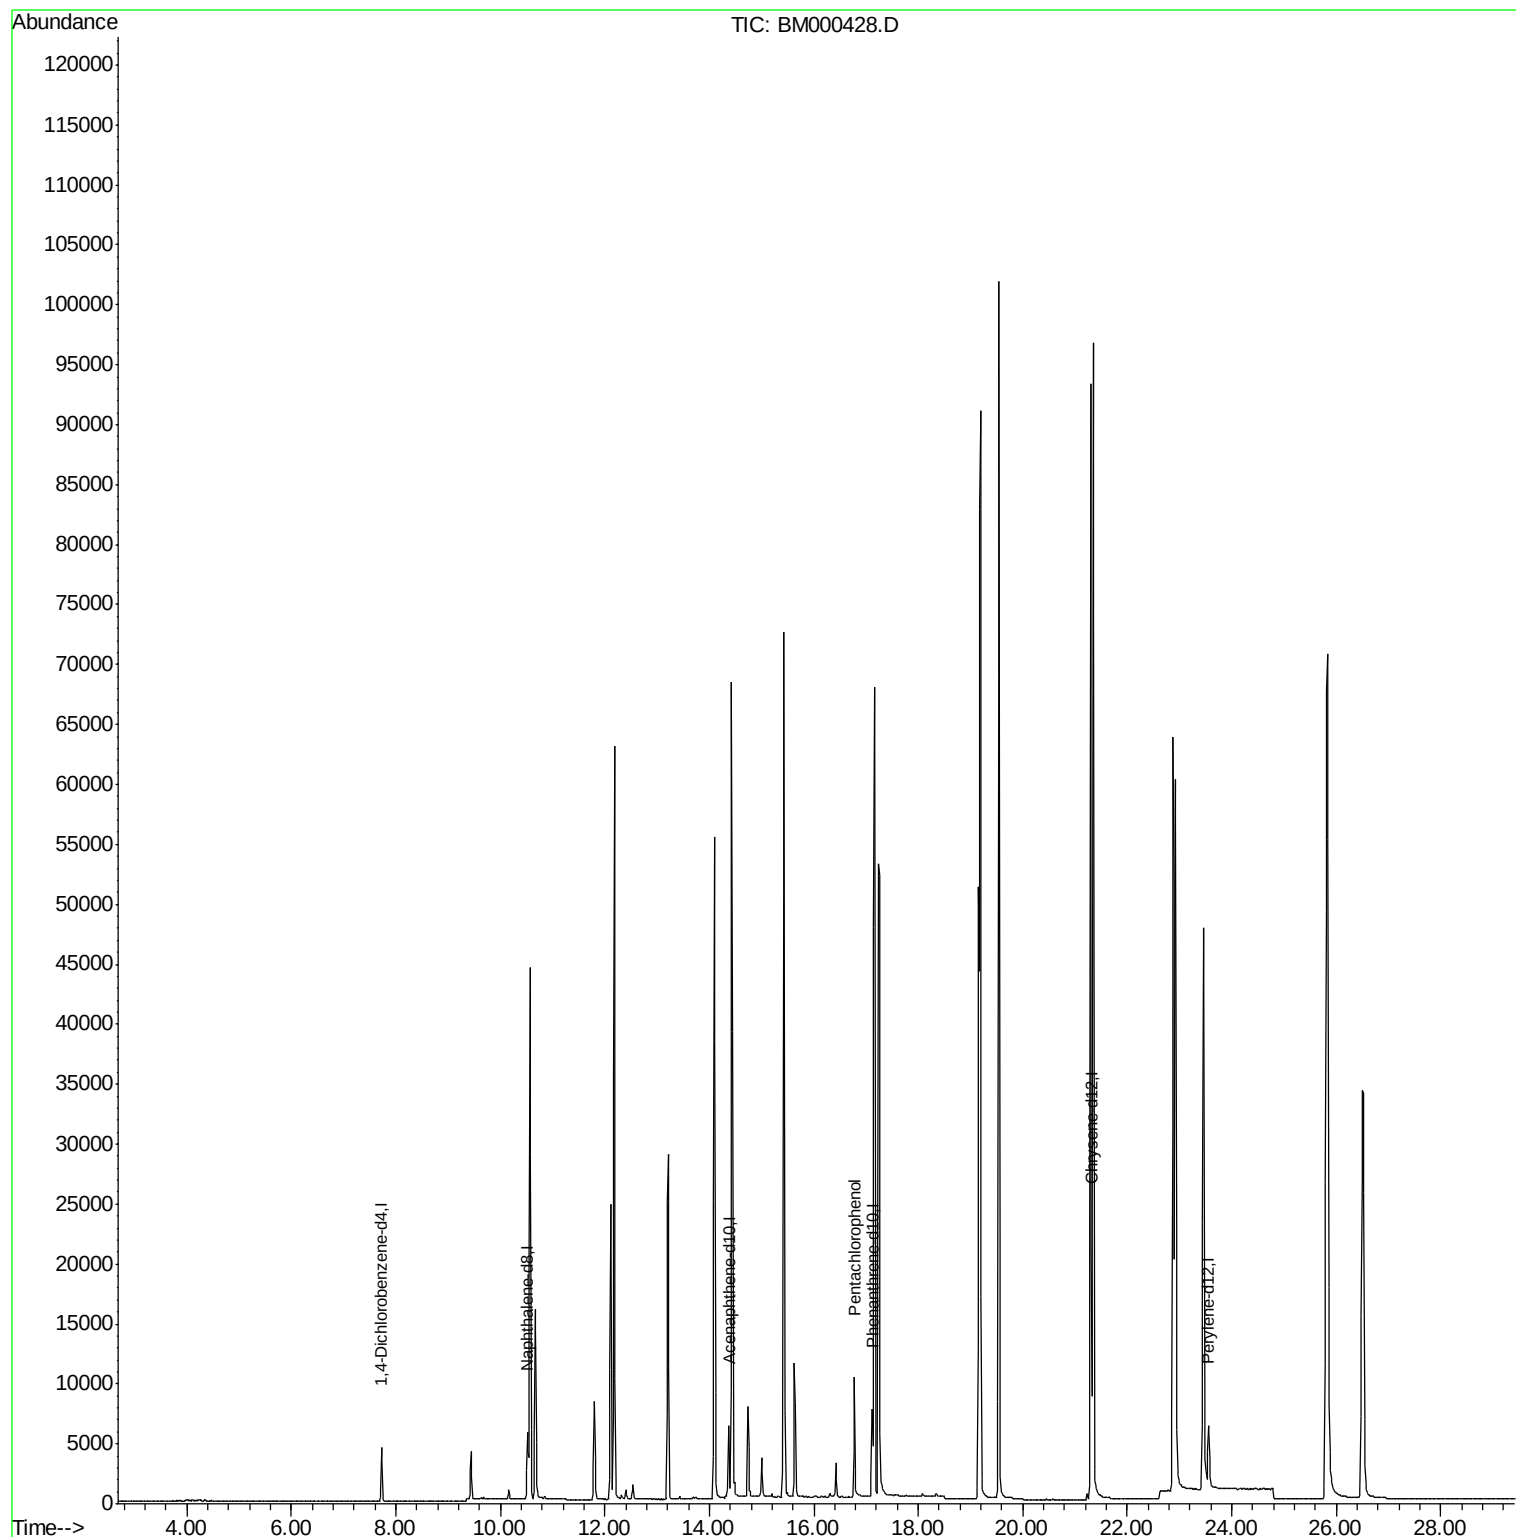

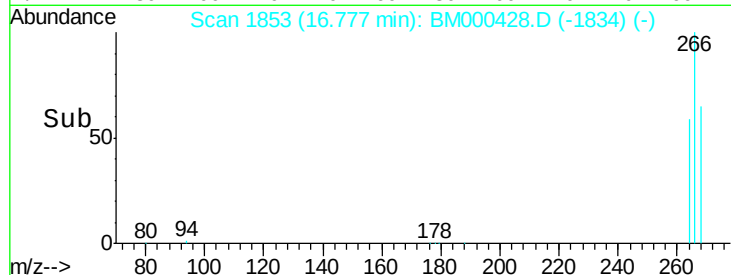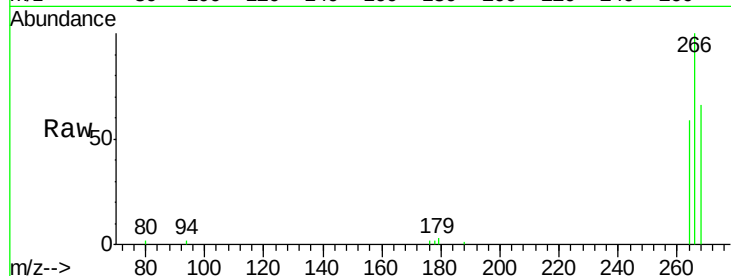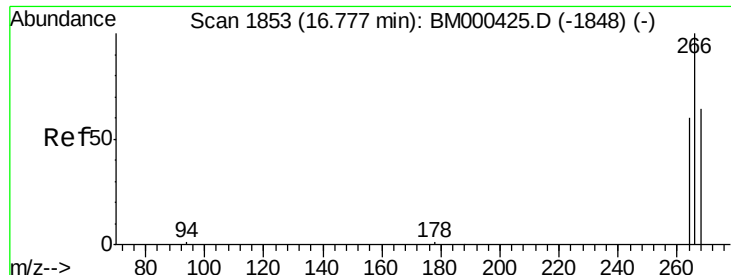

#11

Pentachlorophenol

Concen: 3.57 ng/ul

RT: 16.78 min Scan# 1853

Delta R.T. -0.00 min

Lab File: BM000428.D

Acq: 05 Feb 2015 13:28

Instrument :

BNA_M

ClientSampleId :

Tgt Ion: 266 Resp: 7407

Ion Ratio Lower Upper

266 100

264 62.3 49.8 74.8

268 64.1 49.4 74.0

Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

