


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM020521\
 Data File : BM028661.D
 Acq On : 05 Feb 2021 12:37
 Operator : CG/JU
 Sample : DFTPP23
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP23

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM020521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 05 17:33:51 2021

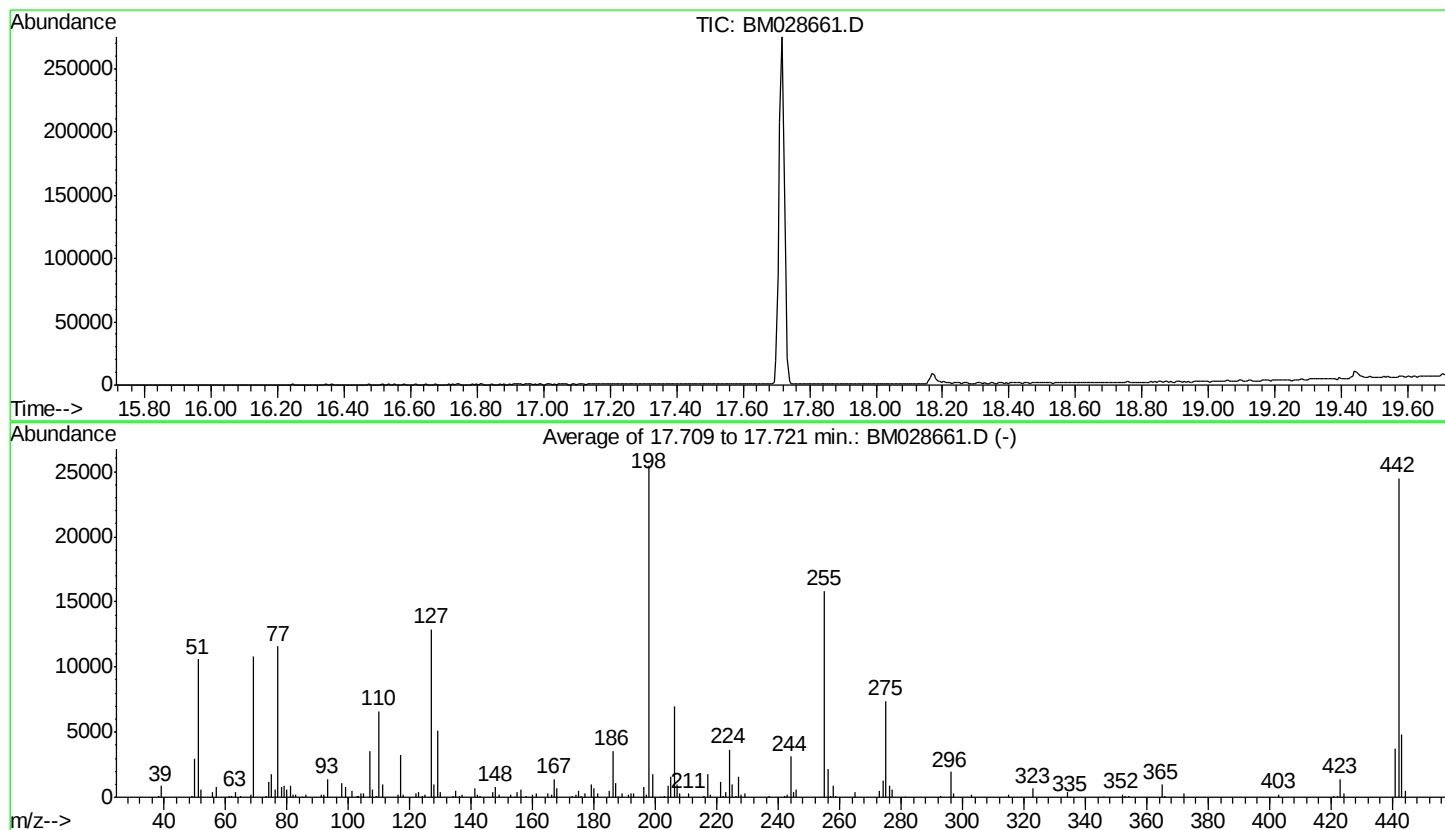

AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.7	10605	PASS
68	69	0.00	2	1.8	200	PASS
69	198	0.00	100	42.6	10843	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.7	12912	PASS
197	198	0.00	2	0.7	186	PASS
198	198	100	100	100.0	25458	PASS
199	198	5	9	6.9	1760	PASS
275	198	10	60	29.0	7384	PASS
365	198	1	100	3.8	976	PASS
441	198	0.01	100	14.9	3783	PASS
442	198	50	100	96.3	24509	PASS
443	442	15	24	19.7	4835	PASS

Scan 2463 (17.674 min): BM028661.D
DFTPP23

m/z	Abundance
44.00	323.0
73.00	202.0
207.00	376.0

Instrument :
BNA_M
ClientSampleId :
DFTPP23

m/z	Abundance
38.00	153.0
39.00	934.0
43.90	285.0
50.00	2987.0
51.10	11400.0
52.00	562.0
55.90	397.0
57.00	820.0
62.00	167.0
63.00	437.0
65.00	203.0
67.90	162.0
69.00	11340.0
73.00	278.0
74.00	1235.0
75.00	1842.0
76.10	574.0
77.00	11691.0
78.00	835.0
79.00	925.0
80.00	673.0
81.00	799.0
82.00	210.0
83.00	226.0
85.90	281.0
91.00	200.0
92.00	202.0
93.00	1347.0
98.00	1047.0
99.00	894.0
100.90	521.0
102.90	183.0
103.90	345.0
105.00	344.0
107.00	3795.0
108.00	579.0
109.10	187.0
110.00	6484.0
111.00	1011.0
115.90	202.0
117.00	3270.0
118.00	228.0
121.90	289.0
123.00	365.0
123.90	175.0
124.90	183.0
127.00	12638.0
128.00	1104.0
129.00	4825.0
129.90	451.0
135.00	452.0
136.00	164.0
136.90	224.0
141.00	671.0
142.00	199.0
147.00	375.0
148.00	749.0
148.90	193.0
153.00	194.0
155.00	347.0
155.90	532.0
159.90	189.0
161.00	224.0
164.90	262.0
166.00	216.0
167.00	1199.0
168.00	697.0
174.00	201.0
175.00	471.0
176.90	251.0
179.00	957.0
179.90	585.0
180.90	259.0
185.00	464.0
186.00	3290.0
187.00	948.0
188.90	252.0
190.90	157.0
191.90	271.0
192.90	319.0
196.00	840.0
198.00	22648.0
198.90	1582.0
204.00	708.0
205.00	1380.0
206.00	6221.0
207.00	1306.0
208.00	335.0
210.90	194.0
217.00	1543.0
218.00	225.0
221.00	1103.0

Instrument :
BNA_M
ClientSampleId :
DFTPP23

223.00	309.0
224.00	3178.0
225.10	778.0
227.00	1397.0
228.00	201.0
228.90	225.0
243.00	192.0
244.00	2686.0
244.90	317.0
246.00	501.0
255.00	13261.0
256.00	1953.0
257.00	192.0
258.00	842.0
265.00	334.0
273.00	381.0
274.00	1049.0
275.00	6145.0
276.00	798.0
276.90	491.0
296.00	1562.0
296.90	212.0
314.90	189.0
323.00	522.0
334.00	256.0
352.00	155.0
365.00	728.0
372.00	176.0
403.00	166.0
423.00	901.0
423.90	283.0
441.00	2655.0
442.00	16616.0
443.00	3365.0
444.00	365.0

Instrument :
BNA_M
ClientSampleId :
DFTPP23

m/z	Abundance
38.00	162.0
39.00	953.0
43.90	247.0
49.00	161.0
50.00	3522.0
51.00	12023.0
52.00	663.0
55.90	456.0
57.00	885.0
61.00	174.0
62.00	182.0
63.00	498.0
65.00	220.0
68.00	251.0
69.00	12638.0
73.00	295.0
74.00	1437.0
75.00	2097.0
76.00	724.0
77.10	13728.0
78.00	977.0
79.00	981.0
79.90	692.0
81.00	1043.0
82.00	279.0
82.90	230.0
85.00	158.0
86.00	286.0
91.00	236.0
92.00	262.0
93.00	1751.0
98.00	1274.0
99.00	938.0
101.00	490.0
102.90	215.0
104.00	303.0
105.00	375.0
107.00	3877.0
108.00	616.0
110.00	7823.0
111.00	1142.0
115.90	232.0
117.00	3815.0
117.90	229.0
122.00	260.0
123.00	461.0
124.00	215.0
125.00	168.0
127.00	15201.0
128.00	1120.0
129.00	6066.0
130.00	463.0
133.90	199.0
135.00	544.0
136.00	238.0
137.00	229.0
141.00	901.0
141.90	235.0
147.00	444.0
147.90	880.0
148.90	223.0
152.90	251.0
153.90	158.0
154.90	462.0
156.00	668.0
158.00	197.0
160.00	162.0
161.00	370.0
164.90	295.0
166.00	272.0
167.00	1645.0
168.00	867.0
172.90	178.0
174.00	308.0
175.00	617.0
175.90	177.0
177.00	276.0
179.00	1165.0
180.00	827.0
181.00	432.0
185.00	568.0
186.00	4317.0
187.00	1345.0
188.00	158.0
188.90	286.0
191.00	177.0
192.00	362.0
193.00	401.0
195.90	872.0
197.10	326.0
198.00	30296.0
199.00	2167.0

Instrument :
BNA_M
ClientSampleId :
DFTPP23

201.40	154.0
203.00	213.0
204.00	1143.0
205.00	1906.0
206.00	8084.0
207.00	1477.0
208.00	319.0
210.80	387.0
215.90	164.0
217.00	2179.0
217.90	253.0
221.00	1305.0
222.90	489.0
224.00	4403.0
225.00	1221.0
226.00	174.0
227.00	1916.0
227.90	216.0
229.00	350.0
237.00	205.0
242.00	201.0
243.00	271.0
244.00	3625.0
245.00	474.0
246.00	729.0
255.00	18480.0
256.00	2709.0
258.00	978.0
258.80	179.0
265.00	480.0
273.00	495.0
274.00	1354.0
275.00	8647.0
276.00	1094.0
276.90	586.0
293.00	204.0
296.00	2422.0
296.90	316.0
303.00	339.0
315.00	257.0
323.10	784.0
334.00	504.0
335.00	151.0
351.90	241.0
353.00	162.0
354.00	246.0
364.90	1069.0
365.90	163.0
372.10	283.0
403.00	250.0
421.00	158.0
422.00	151.0
423.00	1525.0
424.00	326.0
441.00	4619.0
442.00	29536.0
443.00	5687.0
444.00	480.0

Instrument :
BNA_M
ClientSampleId :
DFTPP23

m/z	Abundance
39.00	748.0
43.90	295.0
50.00	2456.0
51.10	8392.0
52.00	420.0
56.00	231.0
57.00	627.0
63.00	355.0
68.10	189.0
69.00	8551.0
73.00	237.0
74.00	943.0
75.00	1483.0
76.10	464.0
77.10	9316.0
78.00	669.0
79.00	679.0
80.00	459.0
81.00	713.0
82.00	194.0
82.90	187.0
86.00	179.0
91.00	192.0
91.90	228.0
93.00	1100.0
98.00	889.0
99.00	615.0
101.00	369.0
103.10	179.0
103.90	272.0
104.90	229.0
107.00	3083.0
108.00	445.0
110.00	5504.0
111.00	773.0
116.00	175.0
117.00	2625.0
117.90	239.0
121.90	213.0
123.00	260.0
124.90	168.0
127.00	10899.0
128.00	812.0
129.00	4378.0
129.90	407.0
133.90	170.0
134.90	402.0
136.90	182.0
140.90	600.0
141.90	170.0
143.00	162.0
147.00	316.0
148.00	766.0
149.00	173.0
152.90	216.0
154.90	354.0
156.10	469.0
159.90	202.0
160.90	208.0
164.90	247.0
167.00	1304.0
168.00	589.0
173.90	198.0
174.90	433.0
177.00	256.0
178.90	825.0
179.90	569.0
181.00	250.0
185.00	350.0
186.00	3092.0
187.00	1054.0
188.90	216.0
190.90	156.0
192.00	284.0
193.00	313.0
196.00	721.0
197.10	232.0
198.00	23432.0
198.90	1533.0
202.90	155.0
204.00	849.0
205.00	1390.0
206.00	6493.0
207.00	1412.0
208.00	335.0
210.90	271.0
216.90	1633.0
217.90	214.0
221.00	1045.0
221.90	258.0
223.00	405.0
224.00	3348.0

Instrument :
BNA_M
ClientSampleId :
DFTPP23

225.00	835.0
227.00	1423.0
228.00	211.0
228.90	327.0
241.90	188.0
242.90	176.0
244.00	3000.0
245.00	390.0
245.90	576.0
255.00	15754.0
256.00	1923.0
257.00	163.0
258.00	811.0
265.00	346.0
273.00	477.0
274.00	1371.0
275.00	7360.0
276.00	869.0
277.00	567.0
281.00	155.0
296.00	1871.0
297.00	219.0
302.90	260.0
314.90	224.0
323.00	696.0
333.90	407.0
345.90	156.0
352.00	200.0
353.00	171.0
354.10	196.0
364.90	1132.0
372.00	363.0
402.90	251.0
421.00	218.0
422.00	188.0
423.00	1712.0
423.90	404.0
441.00	4075.0
442.00	27376.0
443.00	5455.0
444.00	536.0

Instrument :
BNA_M
ClientSampleId :
DFTPP23