
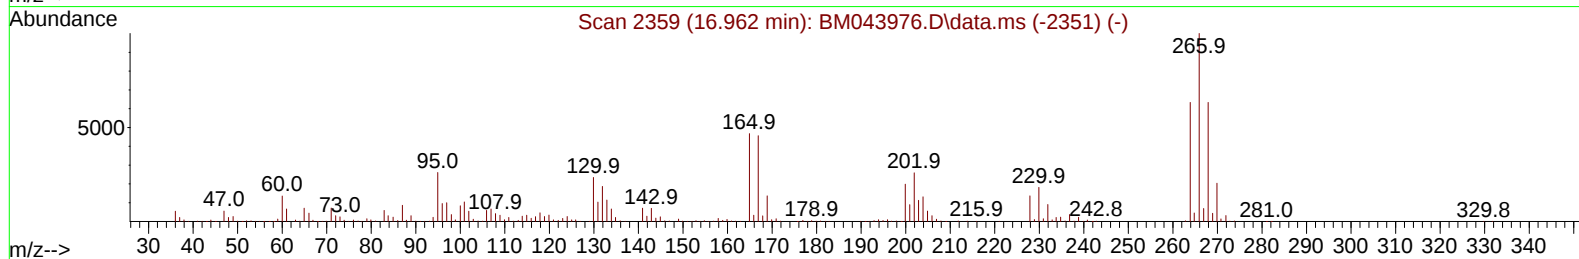
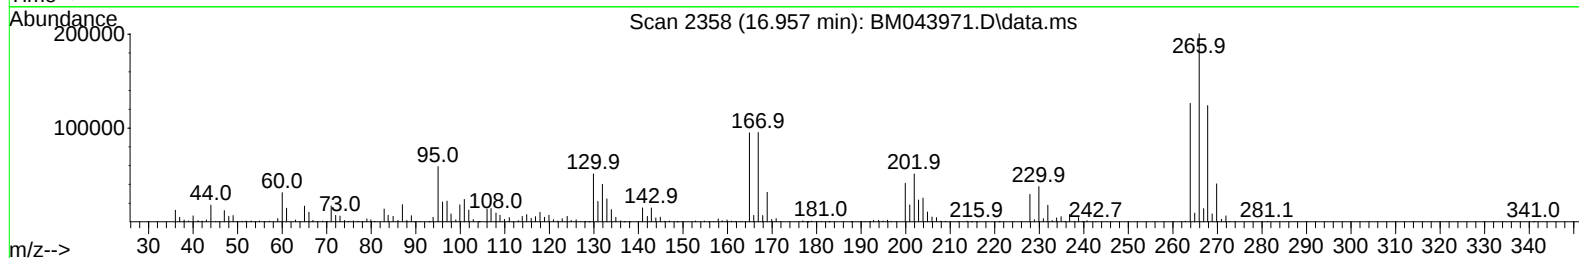


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020524\
Data File : BM043971.D
Acq On : 05 Feb 2024 10:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 07:24:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 07:03:31 2024
Response via : Initial Calibration

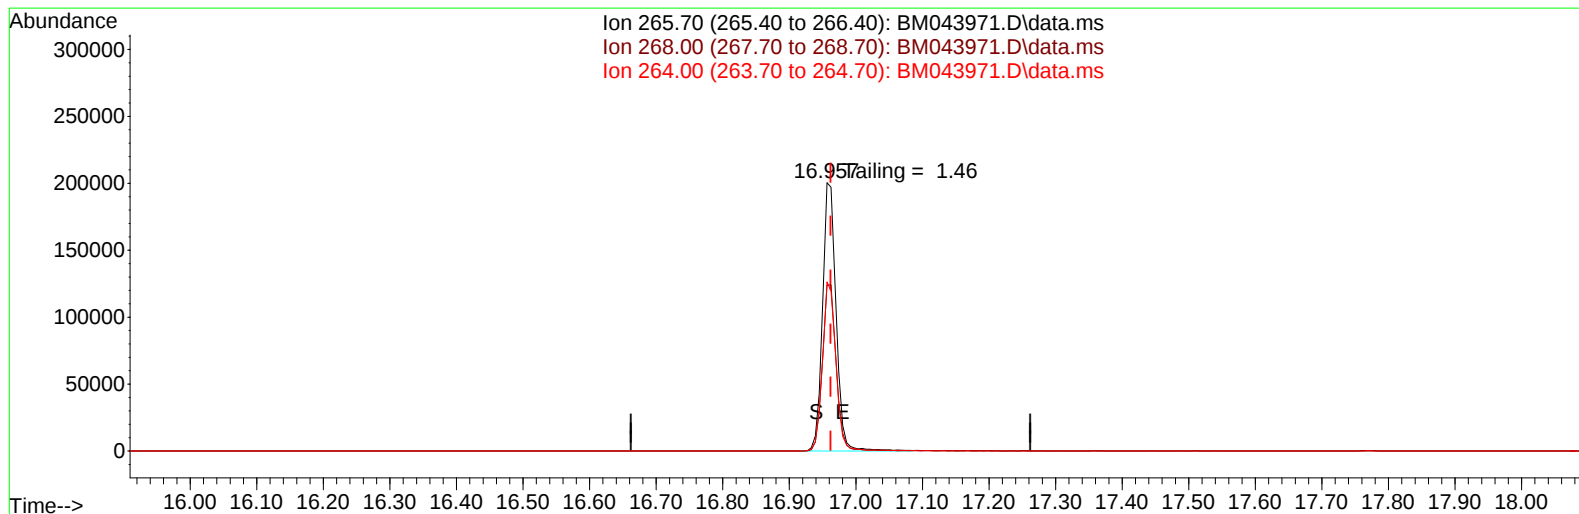

TIC: BM043971.D\data.ms

(70) Pentachlorophenol (C)




16.957min (-0.005) 0.00 ng m

response 284328

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	61.85
264.00	63.30	63.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020524\
Data File : BM043971.D
Acq On : 05 Feb 2024 10:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 07:24:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 07:03:31 2024
Response via : Initial Calibration

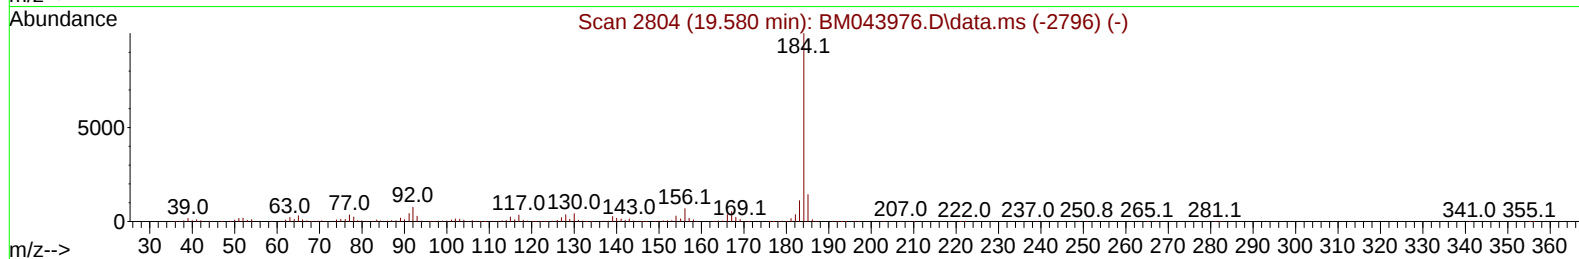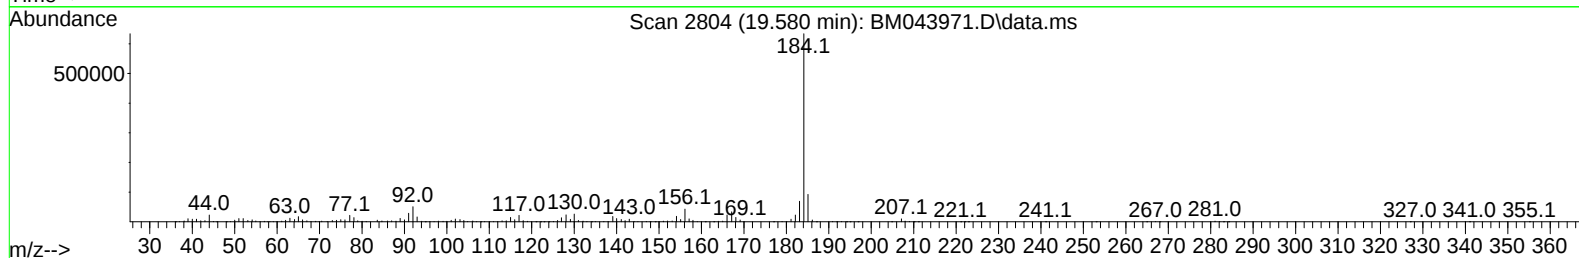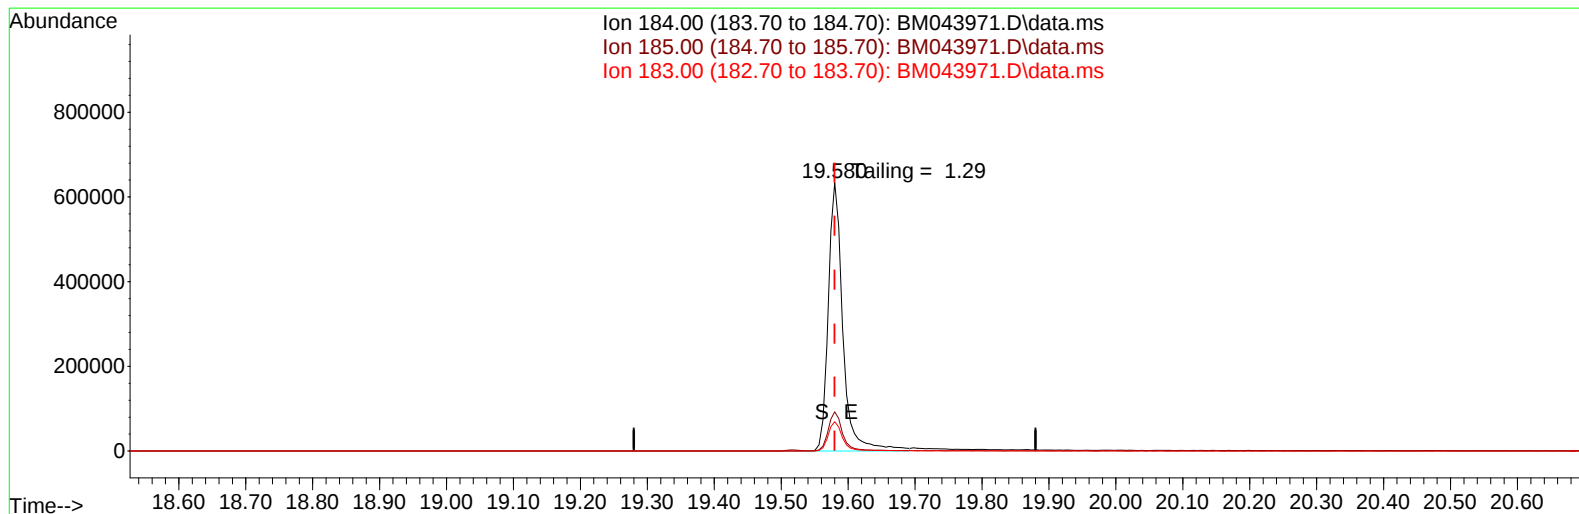

TIC: BM043971.D\data.ms

(77) Benzidine

19.580min (+ 0.000) 398685.66 ng

response 966154

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.61
183.00	11.10	10.93
0.00	0.00	0.00