
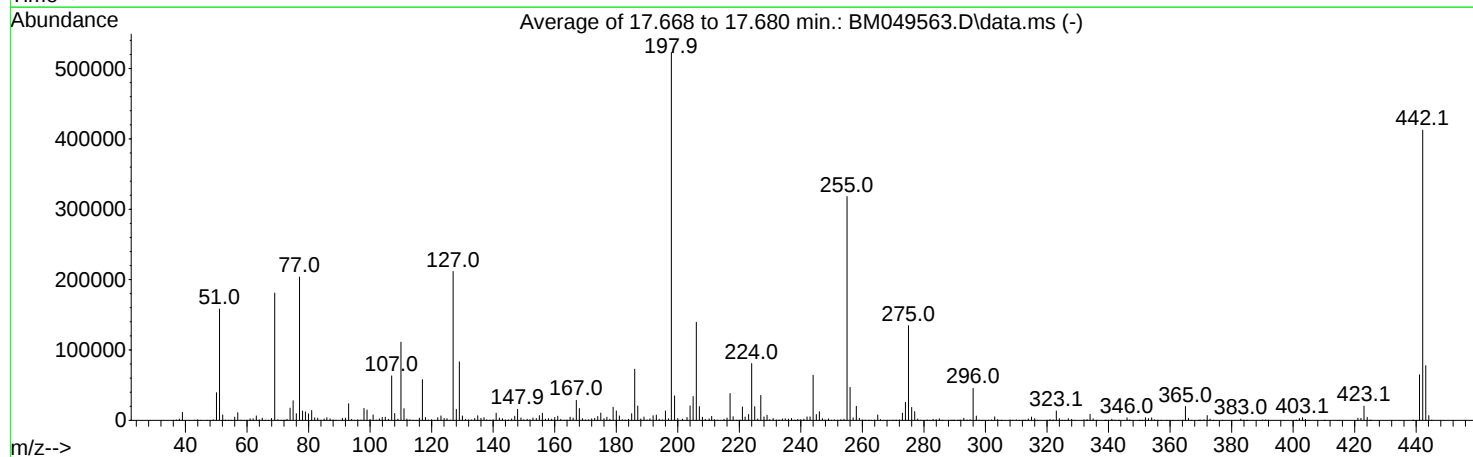


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020525\
Data File : BM049563.D
Acq On : 05 Feb 2025 10:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 06 04:55:28 2025

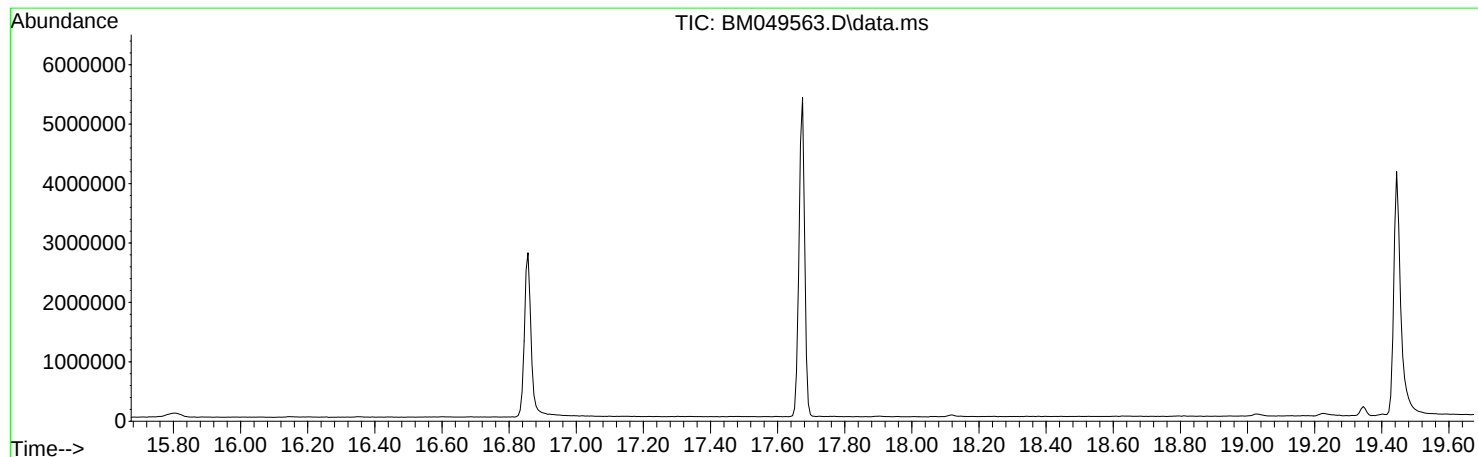




AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.3	158210	PASS
68	69	0.00	2	1.6	2839	PASS
69	198	0.00	100	34.6	181117	PASS
70	69	0.00	2	0.6	1001	PASS
127	198	10	80	40.5	211627	PASS
197	198	0.00	2	0.4	2343	PASS
198	198	100	100	100.0	522795	PASS
199	198	5	9	6.6	34765	PASS
275	198	10	60	25.7	134616	PASS
365	198	1	100	3.8	19722	PASS
441	198	0.01	100	12.4	64755	PASS
442	442	50	100	100.0	412437	PASS
443	442	15	24	18.8	77672	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020525\
Data File : BM049563.D
Acq On : 05 Feb 2025 10:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 06 06:35:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 04:55:28 2025
Response via : Initial Calibration

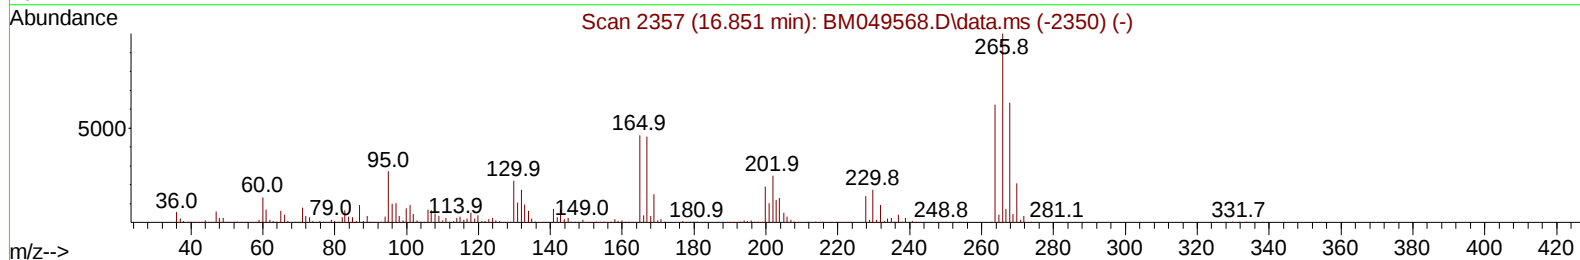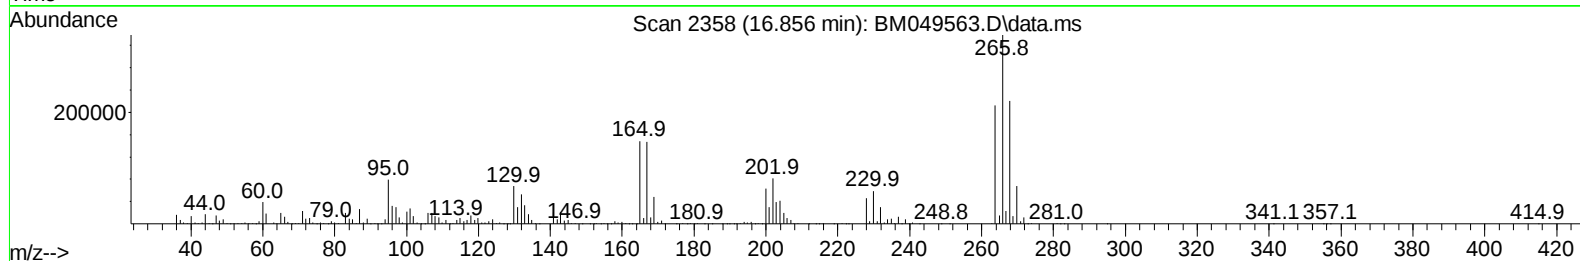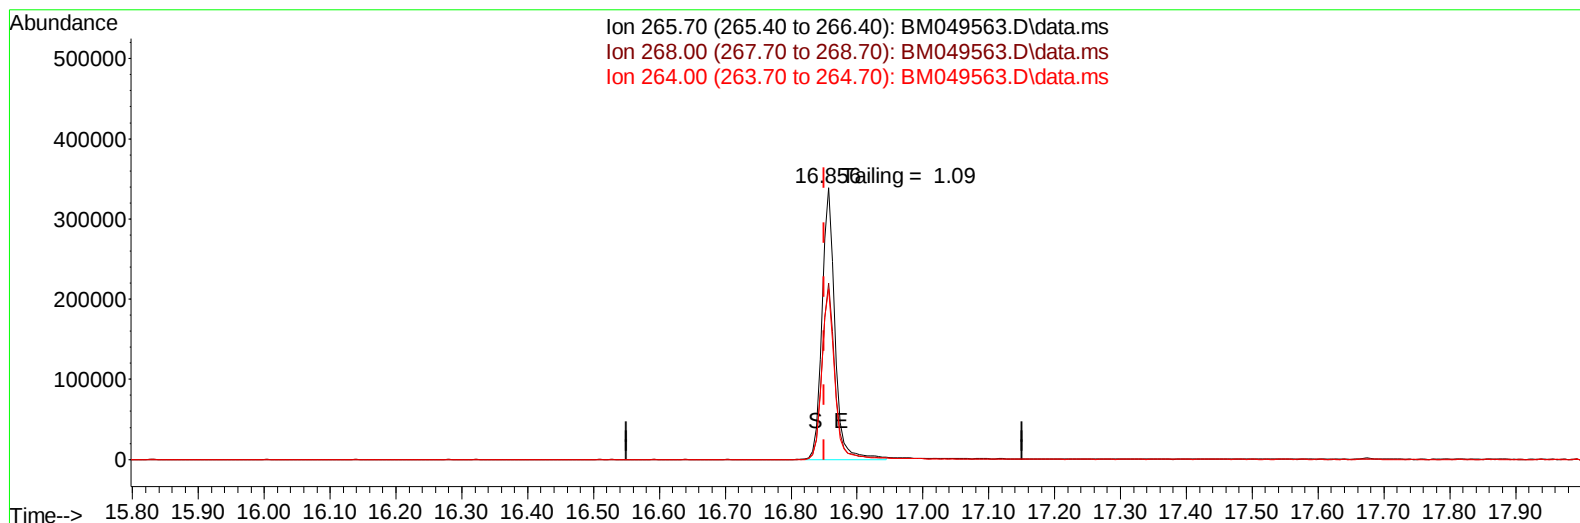

TIC: BM049563.D\data.ms

(70) Pentachlorophenol (C)

16.856min (+ 0.006) 56928.85 ng




response 460911

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	64.98
264.00	62.50	62.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020525\
Data File : BM049563.D
Acq On : 05 Feb 2025 10:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 06 06:38:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 04:55:28 2025
Response via : Initial Calibration

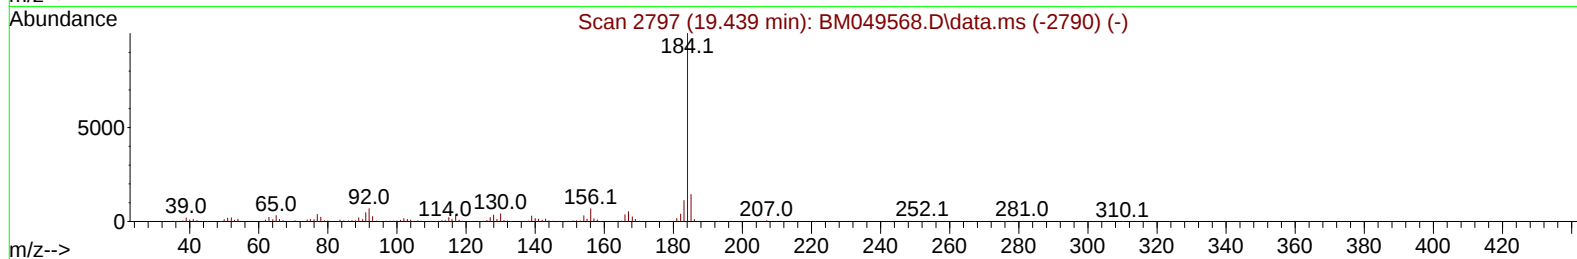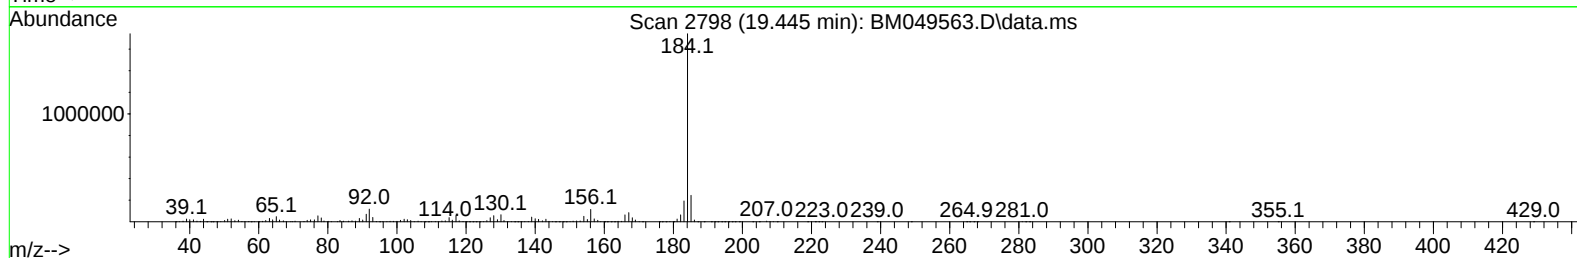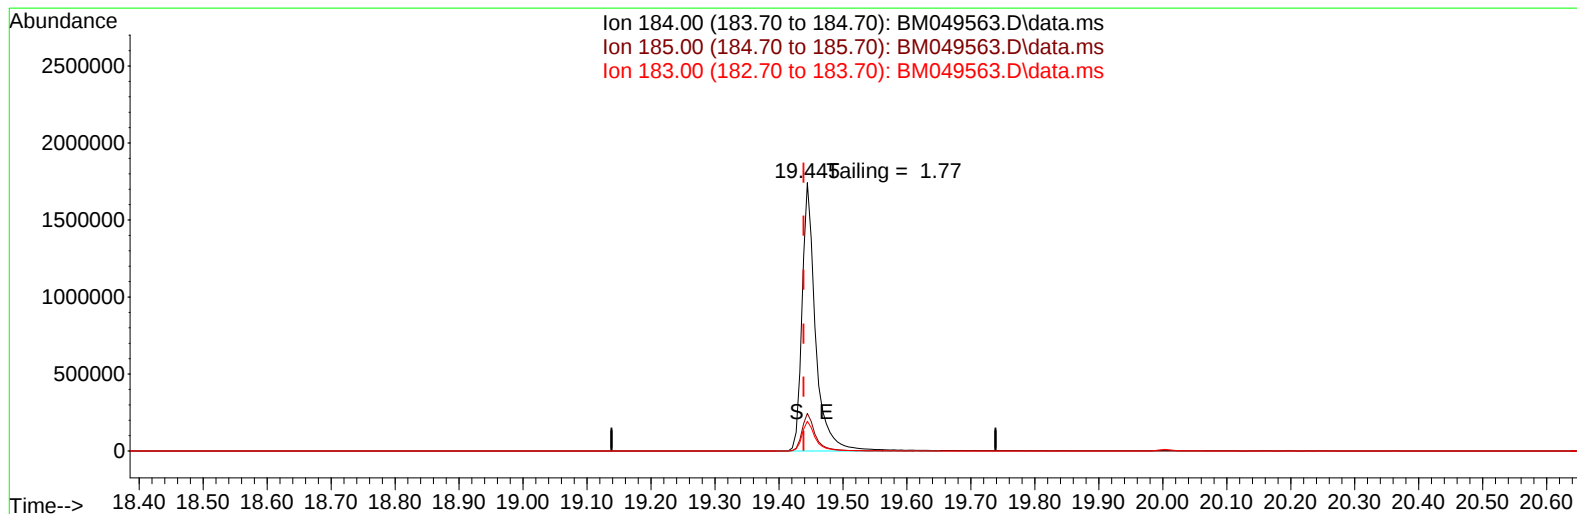

TIC: BM049563.D\data.ms

(77) Benzidine

19.445min (+ 0.006) 1424537.65 ng

response 2573477

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.05
183.00	11.10	11.12
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/5/2025	BNA_M	<u>BM049563.D</u>
Compound Name	Response	Retention Time
DDT	1163468	20.691
DDD	33835	20.25
DDE	3736	19.75
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
37571	1201039	3.13

Instrument :
BNA_M
ClientSampleId :
DFTPP