


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020615\
 Data File : BM000435.D
 Acq On : 06 Feb 2015 15:57
 Operator : TP/IZ
 Sample : DFTPP18
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP18

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-SIM-BM020615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Feb 07 01:08:20 2015

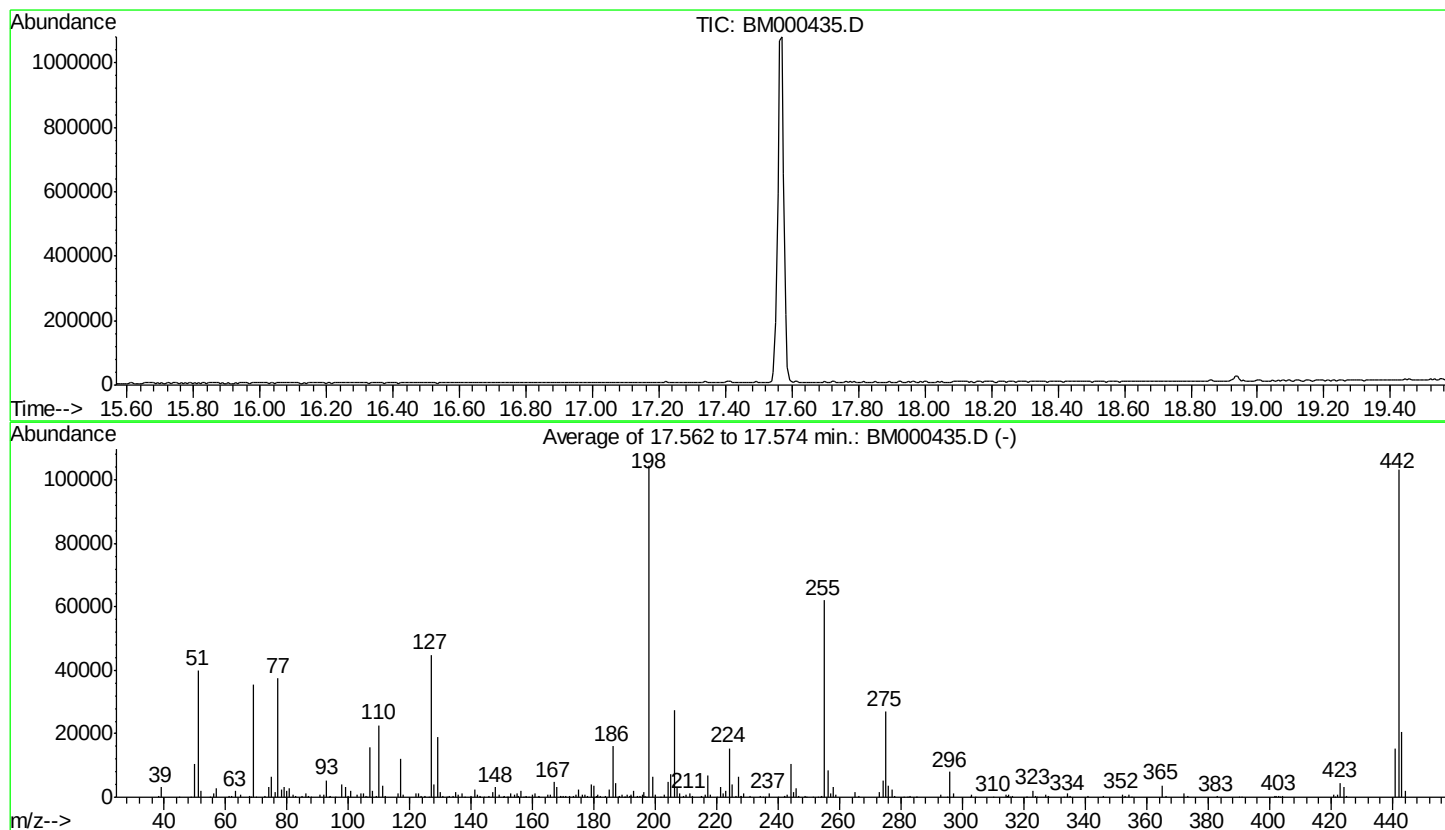

AutoFind: Scans 2529, 2530, 2531; Background Corrected with Scan 2522

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	39848	PASS
68	69	0.00	2	1.7	604	PASS
69	198	0.00	100	34.1	35624	PASS
70	69	0.00	2	0.3	106	PASS
127	198	10	80	43.0	44978	PASS
197	198	0.00	2	0.3	314	PASS
198	198	100	100	100.0	104536	PASS
199	198	5	9	6.1	6349	PASS
275	198	10	60	25.7	26874	PASS
365	198	1	100	3.6	3779	PASS
441	443	0.01	100	75.3	15386	PASS
442	198	50	100	98.9	103381	PASS
443	442	15	24	19.8	20432	PASS