


Data Path : Z:\HPCHEM1\BNA_M\Data\BM020615\SOM01.2\
Data File : BM000441.D
Acq On : 06 Feb 2015 19:30
Operator : TP/IZ
Sample : DFTPP19
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP19

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM020615.M
Title : SVOA CALIBRATION
Last Update : Mon Feb 09 13:47:04 2015

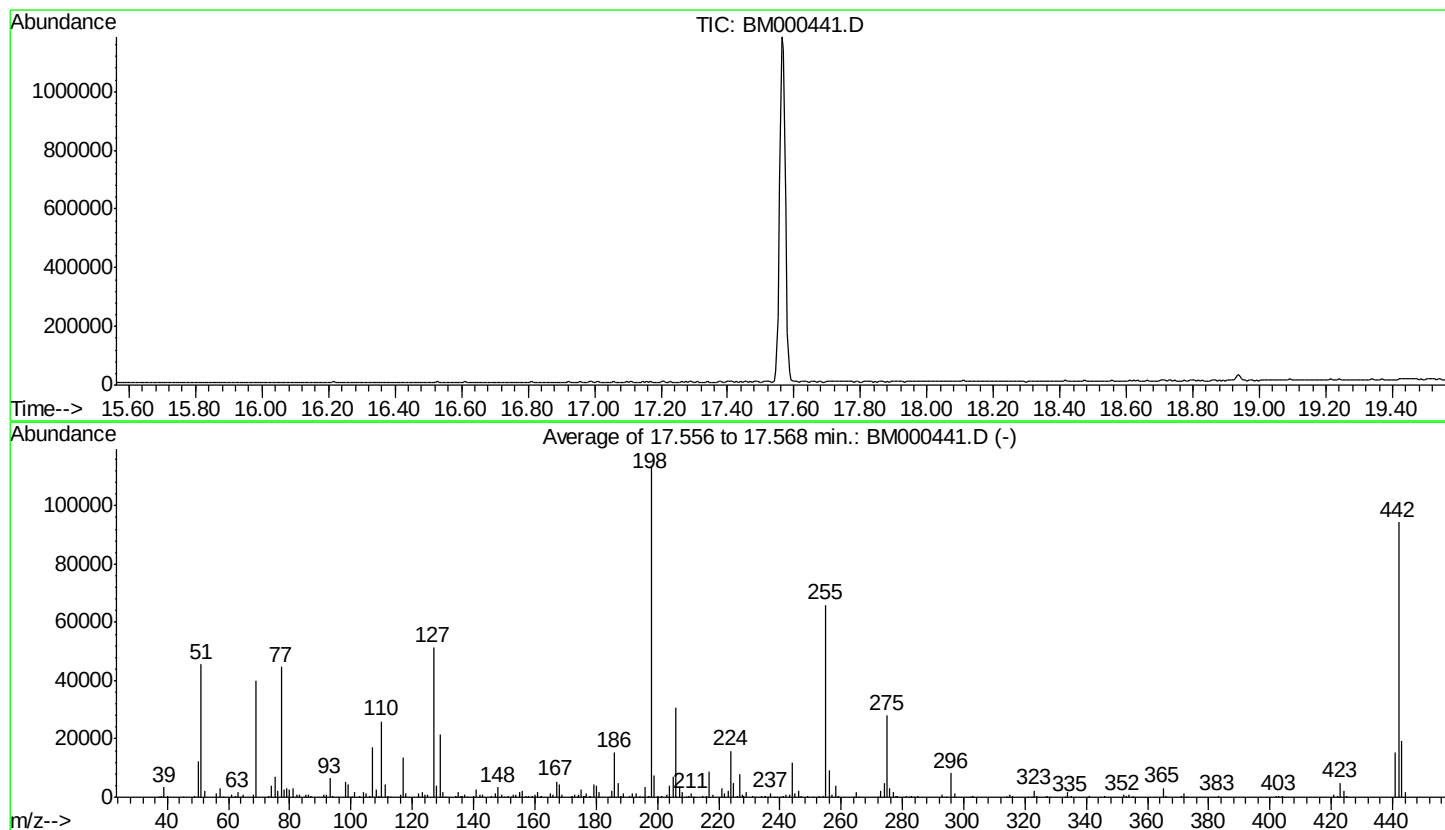

AutoFind: Scans 2528, 2529, 2530; Background Corrected with Scan 2523

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	45488	PASS
68	69	0.00	2	1.9	751	PASS
69	198	0.00	100	35.0	39850	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.0	51184	PASS
197	198	0.00	2	0.5	530	PASS
198	198	100	100	100.0	113765	PASS
199	198	5	9	6.7	7603	PASS
275	198	10	60	24.6	28018	PASS
365	198	1	100	2.8	3216	PASS
441	443	0.01	100	78.5	15259	PASS
442	198	50	100	82.9	94269	PASS
443	442	15	24	20.6	19442	PASS

m/z	Abundance
38.10	360.0
39.00	2421.0
40.00	3321.0
44.00	3777.0
49.10	416.0
50.00	9836.0
51.10	35288.0
52.10	2079.0
56.00	1088.0
57.00	2459.0
61.00	740.0
62.10	558.0
63.00	1368.0
64.90	534.0
68.00	707.0
69.00	31528.0
72.90	667.0
74.00	3138.0
75.00	5627.0
76.00	1711.0
77.10	37256.0
78.10	1670.0
79.10	2102.0
80.10	2422.0
80.90	2441.0
82.10	774.0
83.00	782.0
84.90	520.0
85.10	516.0
86.00	1157.0
87.20	321.0
91.10	840.0
92.00	947.0
93.00	4827.0
94.20	453.0
98.00	3742.0
99.00	3915.0
100.20	438.0
101.00	1161.0
102.90	453.0
104.10	1812.0
105.10	730.0
106.00	308.0
107.00	12387.0
108.00	1875.0
108.90	492.0
110.00	20184.0
111.10	3008.0
111.90	497.0
116.10	666.0
117.00	10180.0
118.20	724.0
122.00	903.0
123.00	1025.0
123.90	578.0
124.90	870.0
127.00	37384.0
128.10	3385.0
129.00	16400.0
130.00	1771.0
134.10	334.0
135.00	1182.0
136.00	880.0
136.90	1009.0
140.00	312.0
140.90	1945.0
141.90	609.0
142.90	701.0
146.00	563.0
147.10	1133.0
148.00	2530.0
149.00	897.0
151.00	406.0
152.90	883.0
153.90	703.0
155.10	1386.0
156.10	1180.0
157.90	393.0
160.00	735.0
161.10	1366.0
162.10	306.0
165.10	639.0
165.90	638.0
167.00	3911.0
168.00	3602.0
168.90	574.0
171.80	667.0
173.00	787.0
173.80	630.0
174.10	697.0
175.10	2002.0

Instrument :
BNA_M
ClientSampleId :
DFTPP19

176.00	536.0
177.00	879.0
177.90	488.0
179.00	2693.0
180.00	3270.0
181.10	1680.0
184.10	570.0
185.00	1739.0
186.10	9864.0
187.00	3354.0
188.00	490.0
189.10	1014.0
191.10	472.0
191.90	1089.0
193.00	1221.0
194.90	330.0
196.00	2887.0
196.70	666.0
197.10	717.0
198.00	77072.0
199.00	4307.0
200.00	463.0
201.50	313.0
203.10	901.0
204.00	2665.0
205.10	6305.0
206.10	20376.0
207.10	5309.0
208.10	1502.0
209.00	407.0
210.10	494.0
211.10	910.0
216.00	355.0
217.00	6744.0
218.00	396.0
221.00	2138.0
221.90	750.0
223.00	1493.0
224.00	9830.0
225.00	2745.0
226.00	489.0
227.00	5431.0
228.20	840.0
229.00	1437.0
231.00	620.0
235.10	552.0
237.10	907.0
240.10	540.0
242.10	501.0
243.20	319.0
244.10	6882.0
244.90	835.0
246.00	1204.0
252.90	556.0
254.20	473.0
255.10	42160.0
256.10	5965.0
257.00	916.0
258.00	2773.0
259.10	404.0
264.90	1571.0
273.10	1227.0
274.00	3330.0
275.00	19296.0
275.90	2349.0
277.00	1176.0
278.00	831.0
281.10	331.0
282.10	483.0
283.10	599.0
285.10	366.0
293.00	544.0
296.00	4706.0
297.00	897.0
302.90	399.0
315.00	557.0
323.00	1602.0
324.10	342.0
333.90	691.0
341.00	361.0
352.90	329.0
354.00	656.0
365.00	2408.0
372.00	911.0
404.10	367.0
423.00	2938.0
424.10	1436.0
424.80	391.0
441.00	7362.0
442.00	45840.0
443.00	9286.0
444.00	1180.0

Instrument :
BNA_M
ClientSampleId :
DFTPP19

m/z	Abundance
37.00	396.0
37.90	816.0
39.00	4016.0
40.00	3161.0
44.00	4327.0
49.00	745.0
50.10	14811.0
51.10	54928.0
52.10	2277.0
56.00	1730.0
57.00	3012.0
61.00	727.0
62.00	646.0
63.00	2243.0
64.10	352.0
65.00	1357.0
68.00	697.0
69.00	47080.0
73.10	1055.0
74.00	4772.0
75.00	7841.0
76.10	2635.0
77.10	52288.0
78.00	3724.0
79.10	3932.0
79.90	2507.0
81.00	3488.0
82.10	1211.0
83.00	1059.0
85.00	1134.0
86.10	970.0
87.00	553.0
91.00	1049.0
92.10	1248.0
93.00	7610.0
94.00	307.0
98.00	6461.0
99.00	5072.0
99.80	544.0
101.00	2985.0
103.00	858.0
103.90	1663.0
104.90	1432.0
106.10	389.0
107.00	20888.0
108.00	2997.0
108.90	712.0
110.00	30280.0
111.00	5366.0
111.90	848.0
112.80	317.0
115.90	1092.0
117.00	14457.0
118.00	1793.0
122.10	1452.0
123.10	1885.0
124.00	1119.0
125.00	658.0
127.00	60472.0
128.10	4292.0
129.00	25168.0
130.00	2005.0
130.90	306.0
134.00	1166.0
135.10	2539.0
135.80	741.0
137.10	1595.0
138.00	339.0
140.00	462.0
141.00	3889.0
142.00	1228.0
142.80	669.0
146.10	933.0
147.00	1606.0
148.00	3795.0
149.00	949.0
151.10	622.0
152.90	1053.0
153.90	1471.0
154.90	2031.0
155.90	2658.0
157.10	1068.0
158.00	370.0
159.00	595.0
159.90	800.0
161.00	2057.0
162.10	624.0
165.00	1566.0
166.00	1384.0
167.10	6192.0
168.00	4449.0

Instrument :
BNA_M
ClientSampleId :
DFTPP19

168.90	1294.0
172.00	977.0
172.90	712.0
174.00	1177.0
175.00	2915.0
176.20	799.0
176.80	1551.0
177.80	435.0
179.00	4796.0
180.00	4718.0
181.00	1768.0
185.10	2482.0
186.00	19520.0
187.00	5307.0
188.20	540.0
189.00	1703.0
191.10	915.0
192.00	1833.0
193.10	1991.0
194.10	569.0
196.00	3990.0
198.00	136256.0
199.00	8157.0
200.00	618.0
201.40	626.0
202.90	792.0
204.00	5390.0
205.00	7883.0
206.10	39272.0
207.10	6287.0
208.10	1577.0
208.90	531.0
210.00	591.0
211.10	1213.0
211.90	369.0
215.00	348.0
215.90	834.0
217.00	9336.0
217.90	705.0
221.10	4822.0
221.80	1213.0
223.00	2374.0
224.10	20624.0
225.00	6153.0
226.10	952.0
227.00	10013.0
227.90	1135.0
229.00	1873.0
231.10	705.0
231.90	350.0
234.10	798.0
234.80	329.0
235.20	509.0
237.10	1440.0
239.10	320.0
241.10	364.0
242.00	1018.0
243.00	1626.0
244.00	15297.0
245.00	1755.0
246.00	2812.0
246.90	709.0
249.00	586.0
250.80	390.0
253.00	501.0
254.10	824.0
255.00	79664.0
256.00	11107.0
257.00	1078.0
258.10	4521.0
258.90	601.0
264.00	360.0
265.00	2037.0
265.90	432.0
273.00	2164.0
274.00	5282.0
275.00	31512.0
276.00	3571.0
277.00	3132.0
277.80	645.0
281.00	476.0
283.90	346.0
285.20	467.0
293.10	1075.0
296.00	9539.0
297.10	1914.0
302.10	358.0
303.10	1195.0
313.90	634.0
315.00	1453.0
316.10	626.0
321.00	302.0
322.10	417.0
323.10	2574.0
323.90	468.0

Instrument :
BNA_M
ClientSampleId :
DFTPP19

326.80	384.0
327.00	382.0
328.00	517.0
333.00	311.0
334.00	2178.0
335.00	487.0
341.10	443.0
346.00	892.0
352.10	1231.0
353.00	807.0
354.00	1336.0
355.00	468.0
365.00	3409.0
365.80	606.0
371.00	320.0
372.00	1475.0
383.00	597.0
402.10	481.0
403.00	579.0
404.20	592.0
420.90	1085.0
422.10	968.0
423.10	4694.0
424.00	2180.0
425.10	626.0
441.00	15945.0
442.00	109360.0
443.00	21120.0
443.90	1624.0

Instrument :
BNA_M
ClientSampleId :
DFTPP19

m/z	Abundance
38.10	379.0
39.00	3766.0
40.00	3545.0
44.00	3210.0
45.00	374.0
48.90	511.0
50.10	12712.0
51.10	46248.0
52.00	2685.0
55.90	1222.0
57.10	3486.0
57.90	390.0
60.90	704.0
62.10	669.0
63.00	1567.0
65.00	941.0
68.10	851.0
69.00	40944.0
73.00	802.0
74.10	4150.0
75.10	7260.0
76.10	2025.0
77.10	44752.0
78.00	3137.0
79.00	3012.0
80.00	2808.0
81.00	3886.0
82.10	557.0
82.90	1030.0
85.00	1152.0
85.90	1022.0
87.00	337.0
90.90	740.0
92.20	1103.0
93.00	6756.0
93.90	474.0
95.80	373.0
98.10	5123.0
99.00	4779.0
101.10	1518.0
103.00	356.0
104.00	1600.0
105.00	1714.0
106.00	471.0
107.00	18440.0
108.10	2460.0
108.90	706.0
110.00	27488.0
111.00	4351.0
112.00	472.0
116.10	1057.0
117.00	16896.0
117.90	1321.0
122.10	1149.0
123.00	2390.0
124.10	843.0
124.90	793.0
127.00	55696.0
128.00	4513.0
129.00	23672.0
130.00	2162.0
131.00	329.0
134.20	680.0
135.00	1495.0
136.10	1230.0
137.10	954.0
140.00	323.0
141.00	2326.0
141.90	1238.0
142.90	783.0
145.90	488.0
147.00	1532.0
148.00	3651.0
149.00	1281.0
150.00	622.0
152.10	343.0
152.90	1021.0
153.90	623.0
155.00	1874.0
156.10	2799.0
157.00	440.0
158.00	429.0
159.00	1007.0
160.00	1362.0
160.90	1960.0
161.80	341.0
165.00	1671.0
166.00	1174.0
167.10	6077.0
168.00	4633.0
168.90	884.0

Instrument :
BNA_M
ClientSampleId :
DFTPP19

172.00	807.0
173.00	959.0
174.10	1409.0
175.00	2776.0
176.00	778.0
177.00	1121.0
178.10	553.0
179.10	5278.0
180.10	4192.0
181.00	2422.0
185.00	1907.0
186.00	16584.0
187.00	6482.0
188.00	862.0
189.00	916.0
190.90	959.0
192.00	1733.0
193.10	2303.0
194.10	666.0
195.00	346.0
196.00	3418.0
197.10	873.0
198.00	127968.0
199.00	10345.0
200.10	607.0
201.60	474.0
202.90	779.0
204.10	4290.0
205.10	7187.0
206.10	32448.0
207.10	7415.0
208.00	1837.0
208.80	425.0
209.20	319.0
210.00	731.0
211.10	1631.0
214.90	527.0
215.90	517.0
217.00	9867.0
217.90	1542.0
220.90	2853.0
222.00	1507.0
223.10	2523.0
224.10	17504.0
225.00	5051.0
226.10	541.0
227.00	7837.0
227.90	1101.0
229.00	1660.0
231.10	532.0
234.00	370.0
235.00	666.0
236.00	375.0
237.10	1632.0
238.20	326.0
241.00	792.0
242.10	1321.0
243.10	979.0
244.00	13325.0
245.00	1609.0
246.00	3276.0
247.00	590.0
249.00	900.0
253.00	466.0
254.10	666.0
255.00	76496.0
256.00	10720.0
257.00	1123.0
258.00	4703.0
259.10	583.0
265.00	2196.0
272.00	380.0
273.10	2897.0
274.00	5983.0
275.10	33248.0
276.00	3686.0
277.10	1587.0
278.10	1127.0
283.00	585.0
283.80	316.0
285.20	770.0
292.90	1122.0
294.00	488.0
296.00	10318.0
297.00	1248.0
303.00	725.0
314.10	416.0
315.00	1131.0
315.90	698.0
323.00	2954.0
327.10	900.0
333.10	349.0
334.10	2354.0
335.00	778.0
340.90	460.0

Instrument :
BNA_M
ClientSampleId :
DFTPP19

345.90	373.0
352.10	1358.0
353.10	748.0
354.00	1227.0
355.20	338.0
365.00	3831.0
365.90	557.0
370.80	312.0
371.10	352.0
372.00	1836.0
372.90	512.0
383.00	887.0
402.00	674.0
403.00	878.0
403.80	474.0
421.00	1035.0
422.00	706.0
423.00	6892.0
424.10	2873.0
424.90	433.0
441.00	22472.0
442.00	127608.0
443.10	27920.0
444.10	1946.0

Instrument :
BNA_M
ClientSampleId :
DFTPP19

Scan 2523 (17.527 min): BM000441.D
DFTPP19

m/z	Abundance
40.00	2893.0
44.00	4255.0
72.90	352.0
190.90	366.0
193.00	507.0
207.10	2749.0
208.90	786.0

Instrument :
BNA_M
ClientSampleId :
DFTPP19