
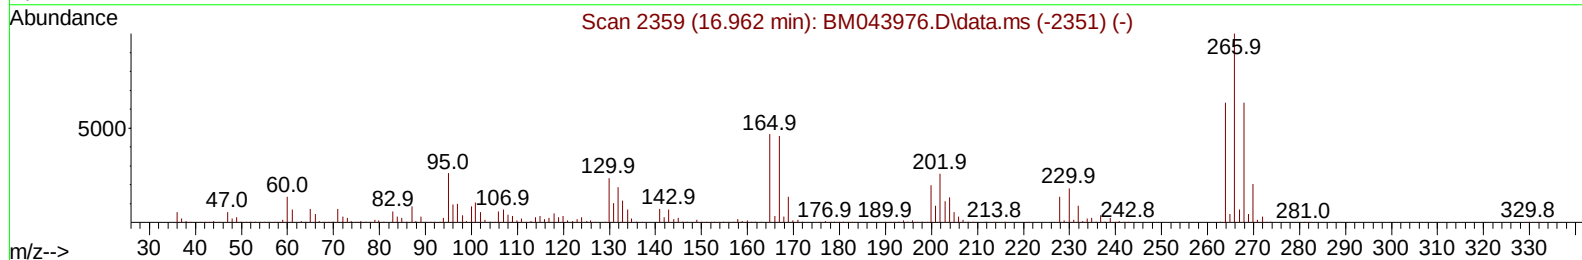
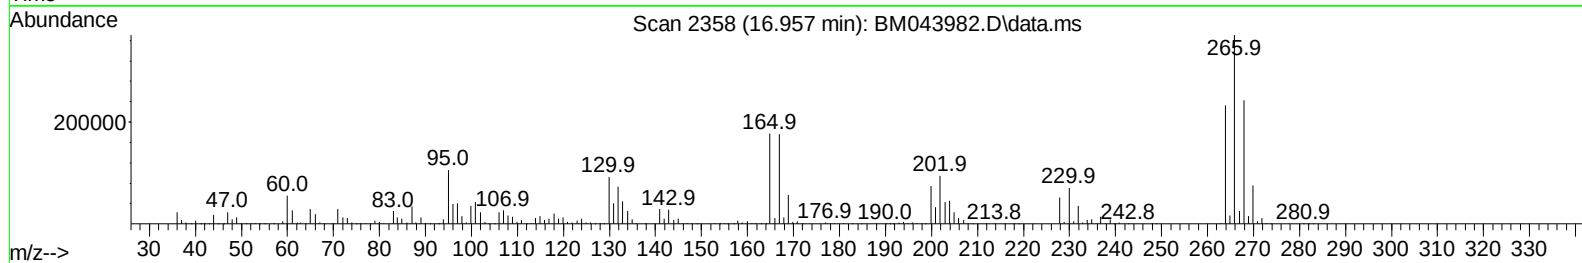


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020624\
Data File : BM043982.D
Acq On : 06 Feb 2024 08:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 04:11:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 07:03:31 2024
Response via : Initial Calibration

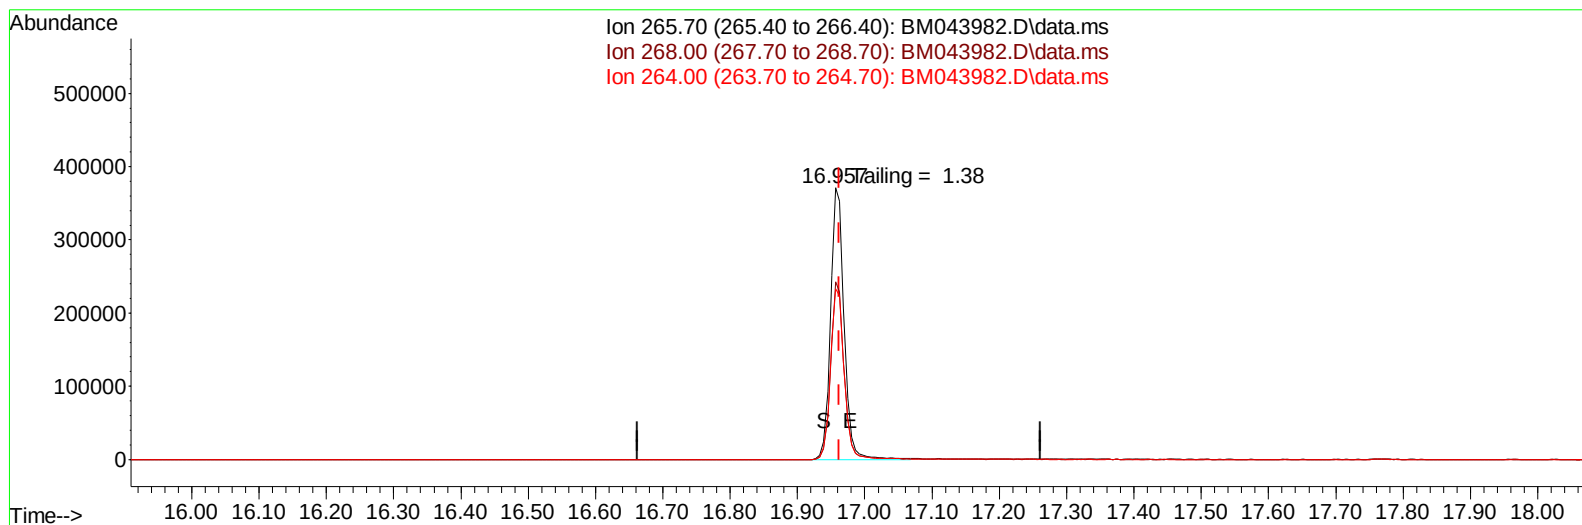

TIC: BM043982.D\data.ms

(70) Pentachlorophenol (C)




16.957min (-0.005) 0.00 ng

response 520298

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	65.44
264.00	63.30	62.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020624\
Data File : BM043982.D
Acq On : 06 Feb 2024 08:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 04:11:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 07:03:31 2024
Response via : Initial Calibration

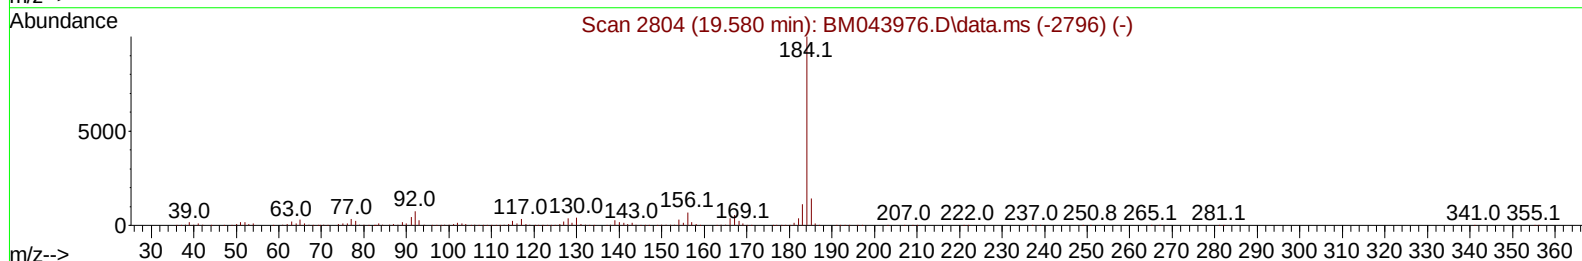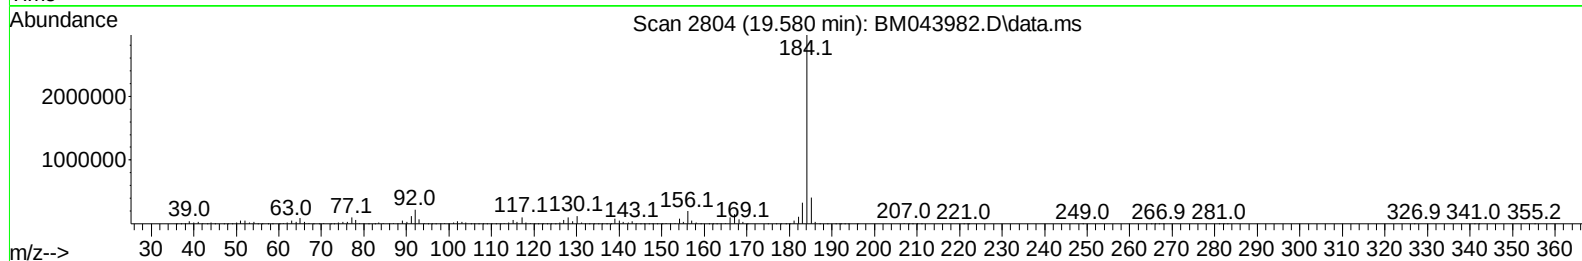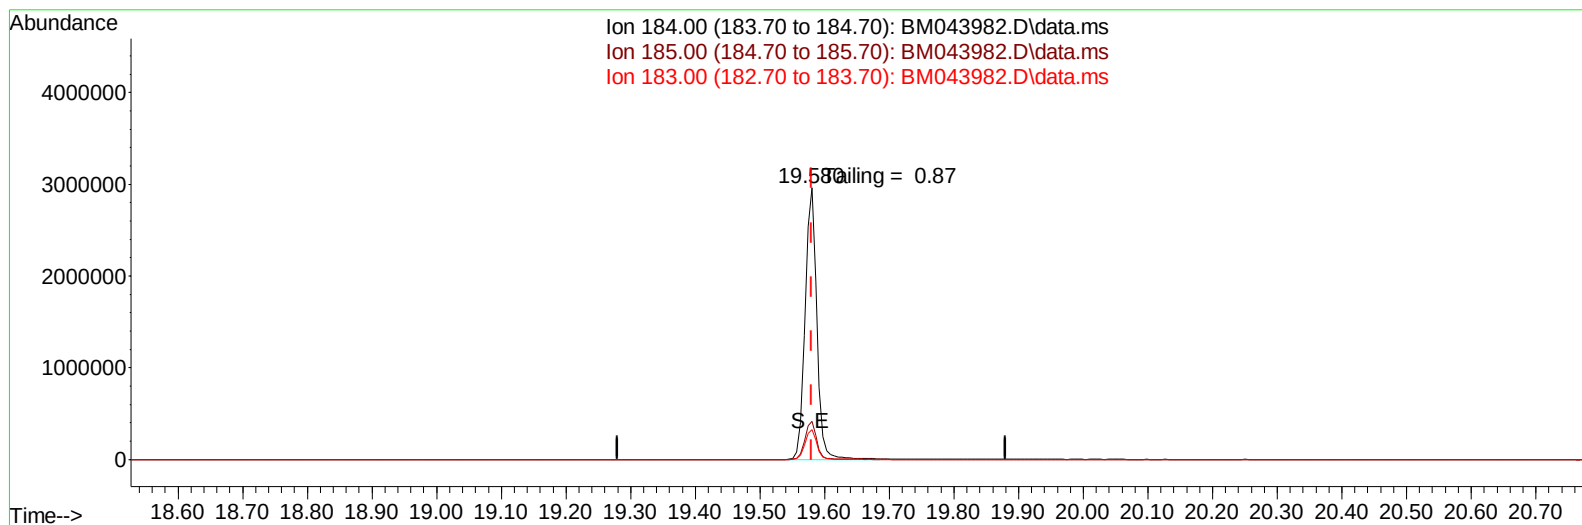

TIC: BM043982.D\data.ms

(77) Benzidine**19.580min (+ 0.000) 1132226.84 ng****response 3792449**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.07
183.00	11.10	11.04
0.00	0.00	0.00