


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020624\
Data File : BM043982.D
Acq On : 06 Feb 2024 08:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020524.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 06 07:03:31 2024

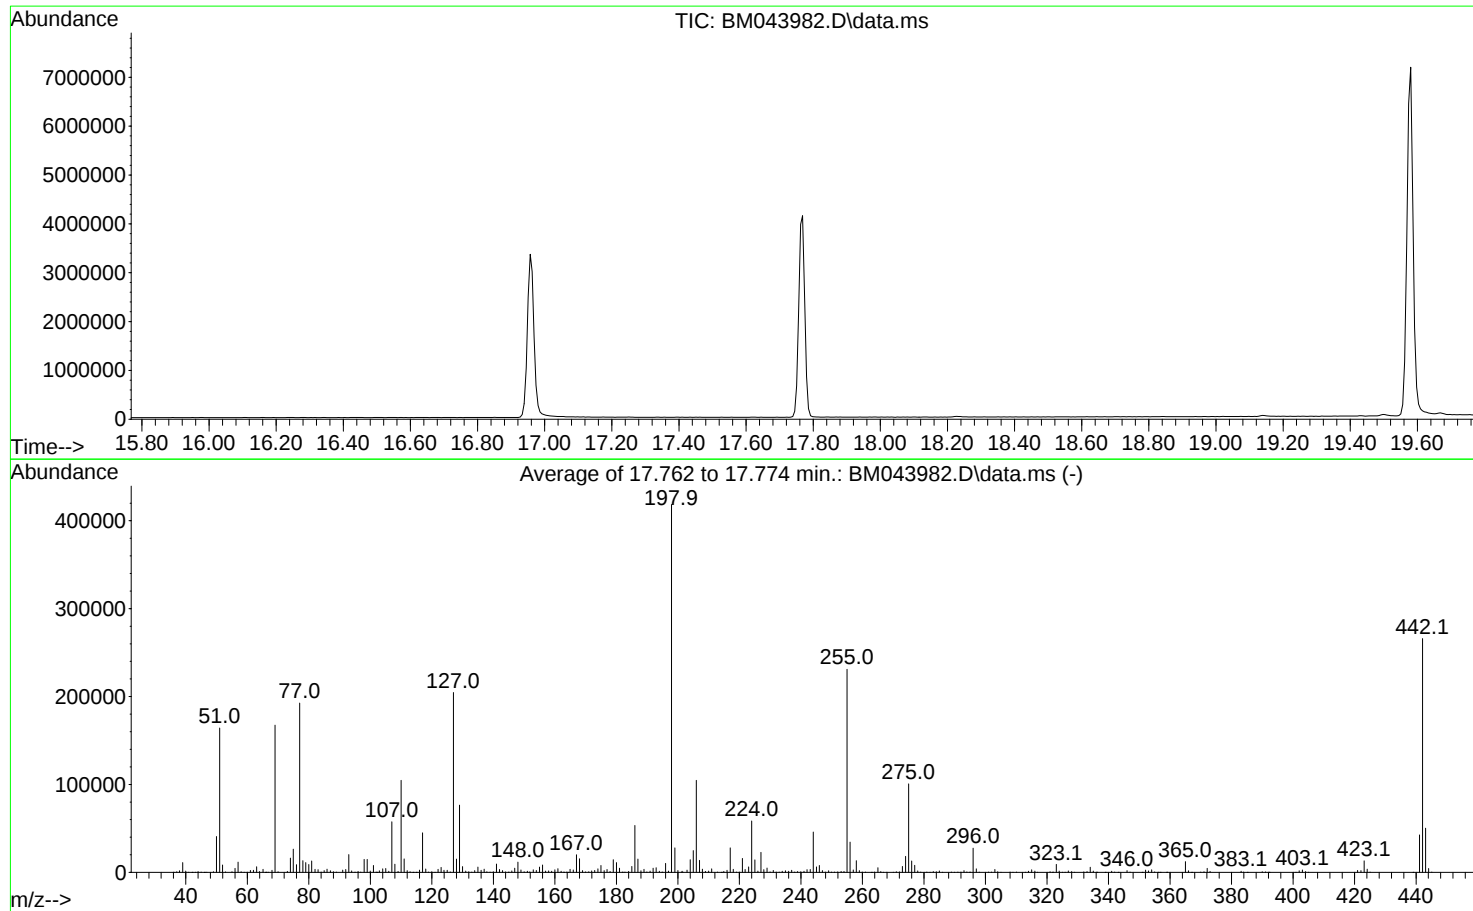




AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	164227	PASS
68	69	0.00	2	1.4	2331	PASS
69	198	0.00	100	40.0	167443	PASS
70	69	0.00	2	0.4	671	PASS
127	198	10	80	48.9	204515	PASS
197	198	0.00	2	0.4	1518	PASS
198	198	100	100	100.0	418475	PASS
199	198	5	9	6.7	27867	PASS
275	198	10	60	24.1	100661	PASS
365	198	1	100	2.9	12191	PASS
441	198	0.01	100	10.2	42605	PASS
442	442	50	100	100.0	265920	PASS
443	442	15	24	18.9	50211	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020624\
Data File : BM043982.D
Acq On : 06 Feb 2024 08:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 07 04:11:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 07:03:31 2024
Response via : Initial Calibration

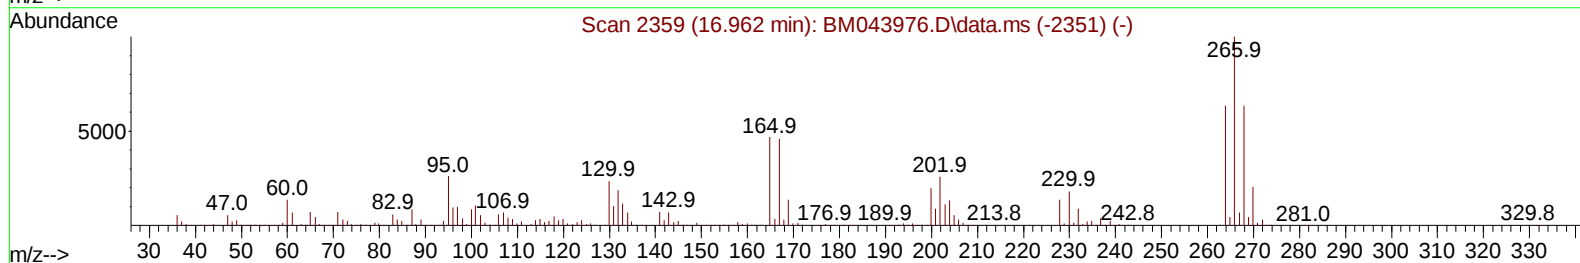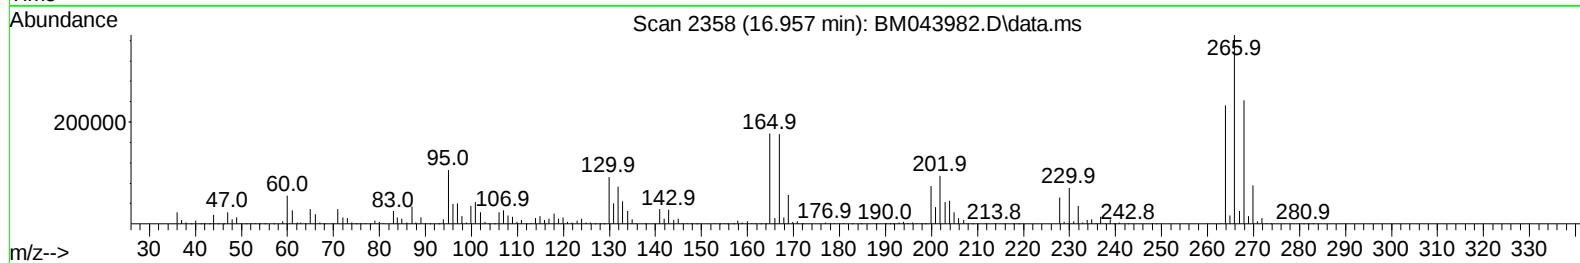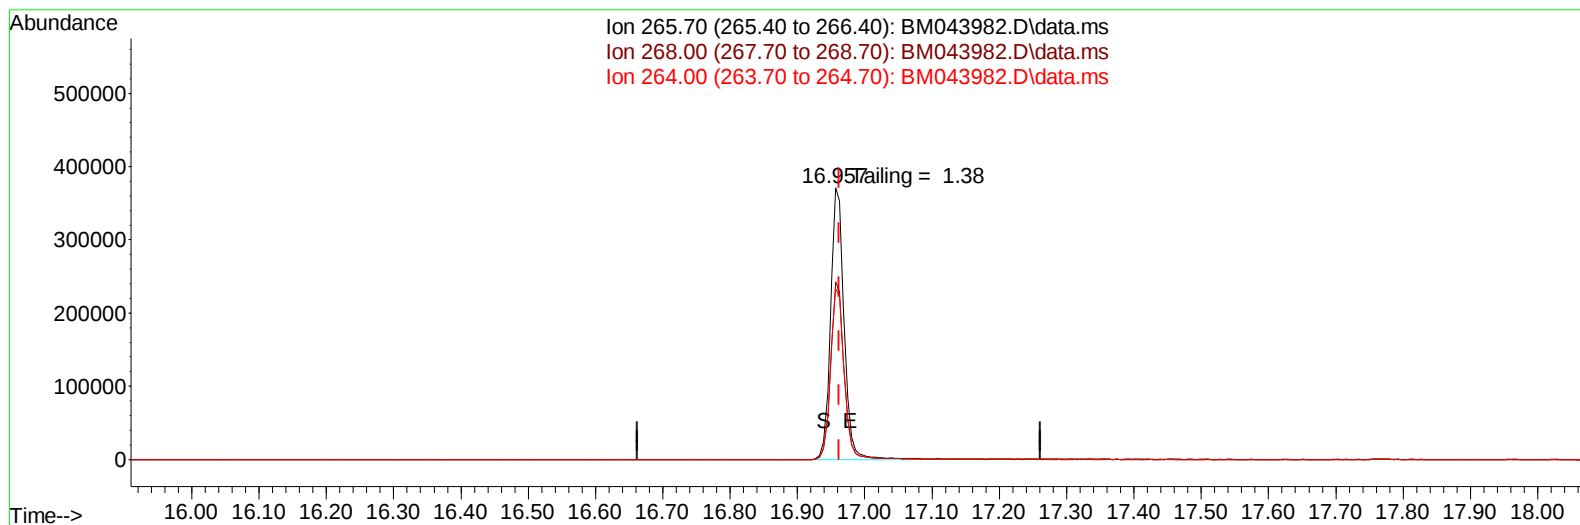

TIC: BM043982.D\data.ms

(70) Pentachloropheno1 (C)

16.957min (-0.005) 0.00 ng




response 520298

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.30	65.44
264.00	63.30	62.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020624\
Data File : BM043982.D
Acq On : 06 Feb 2024 08:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 07 04:11:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020524.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 07:03:31 2024
Response via : Initial Calibration

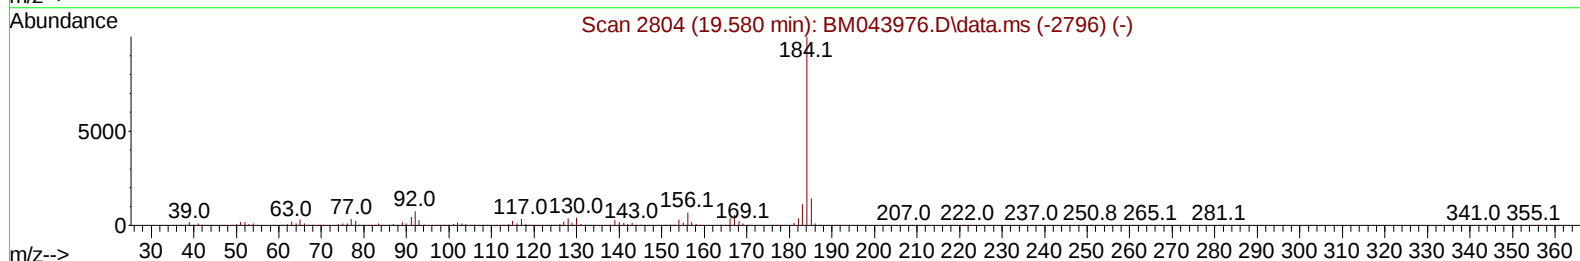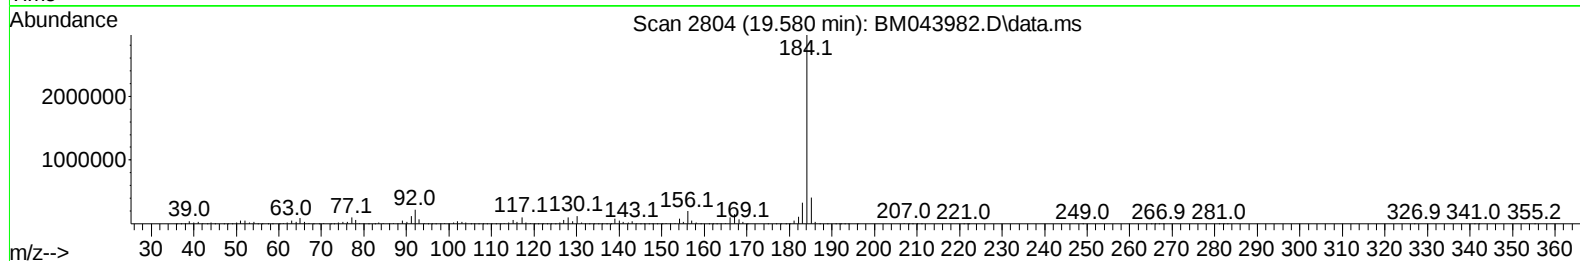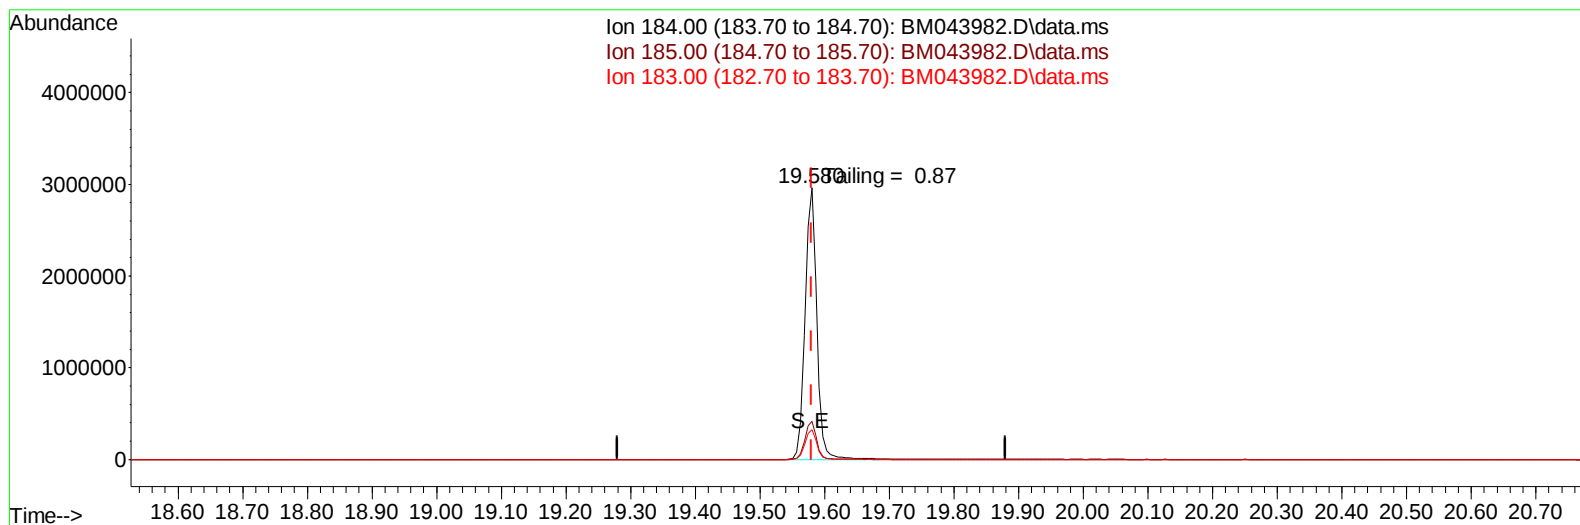

TIC: BM043982.D\data.ms

(77) Benzidine

19.580min (+ 0.000) 1132226.84 ng

response 3792449

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.07
183.00	11.10	11.04
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/6/2024	BNA_M	<u>BM043982.D</u>
Compound Name	Response	Retention Time
DDT	1627223	20.815
DDD	27605	20.374
DDE	1947	19.862
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
29552	1656775	1.78

Instrument :
BNA_M
ClientSampleId :
DFTPP