
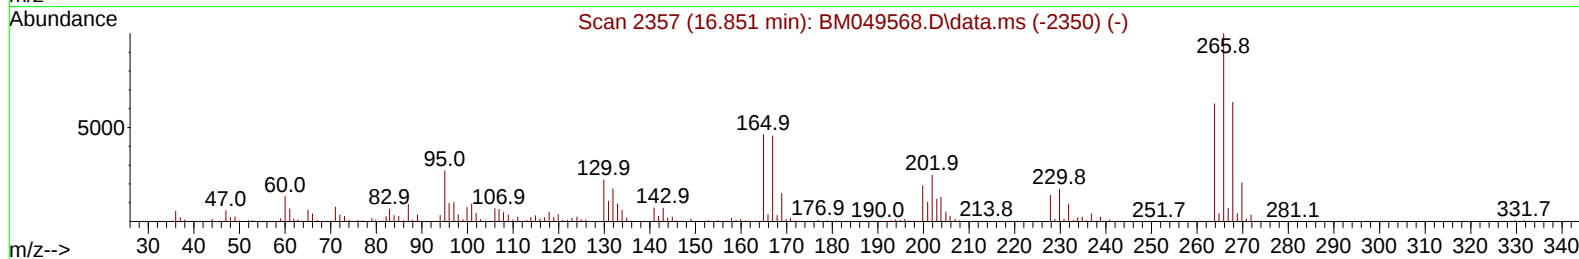
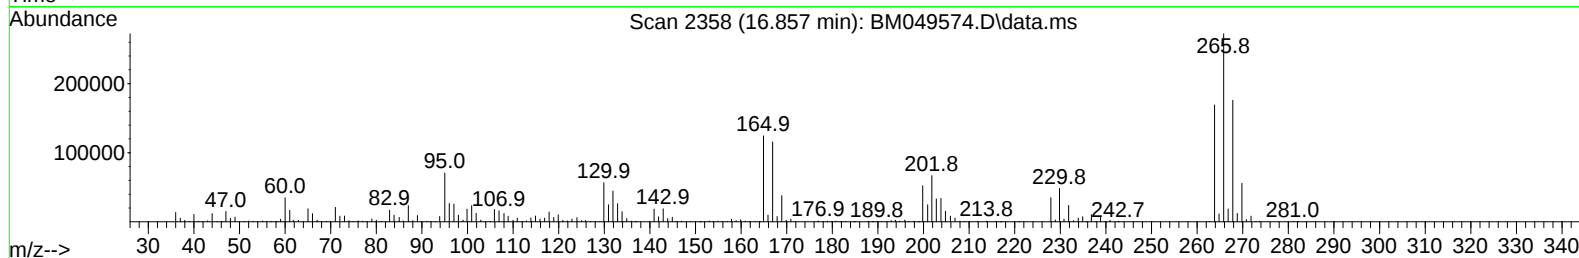


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020625\
Data File : BM049574.D
Acq On : 06 Feb 2025 09:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 11:21:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 04:55:28 2025
Response via : Initial Calibration

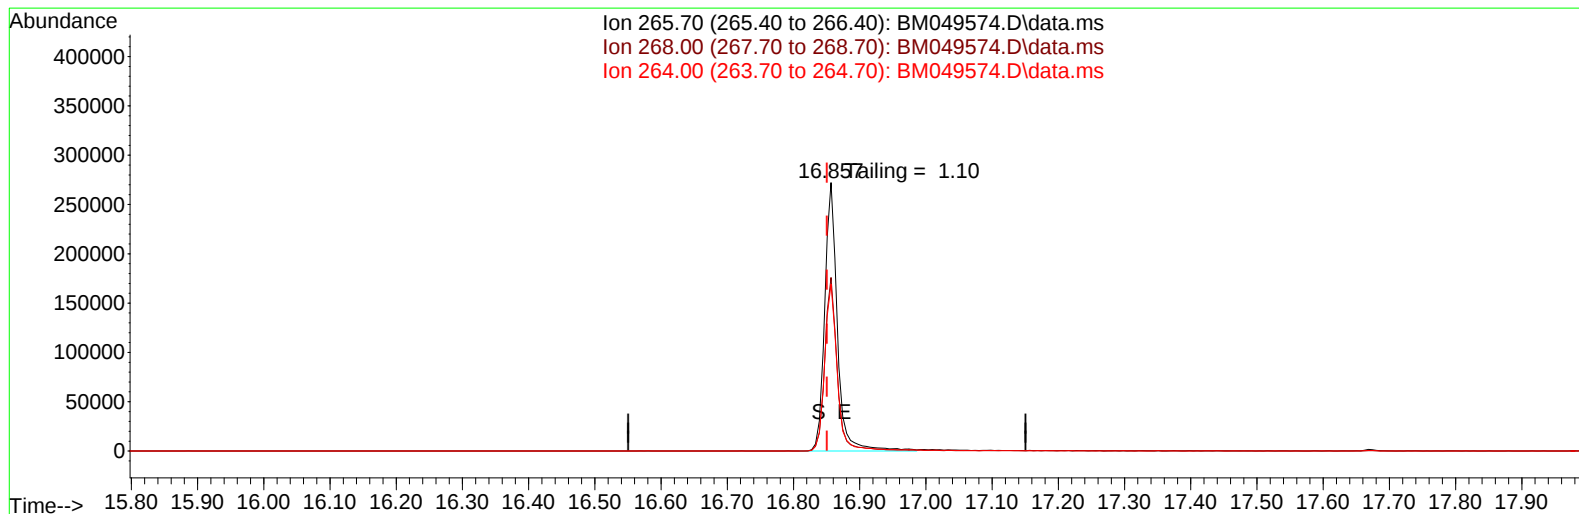

TIC: BM049574.D\data.ms

(70) Pentachlorophenol (C)




16.857min (+ 0.006) 68938.79 ng

response 363868

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	64.66
264.00	62.50	62.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020625\
Data File : BM049574.D
Acq On : 06 Feb 2025 09:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 11:21:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 04:55:28 2025
Response via : Initial Calibration

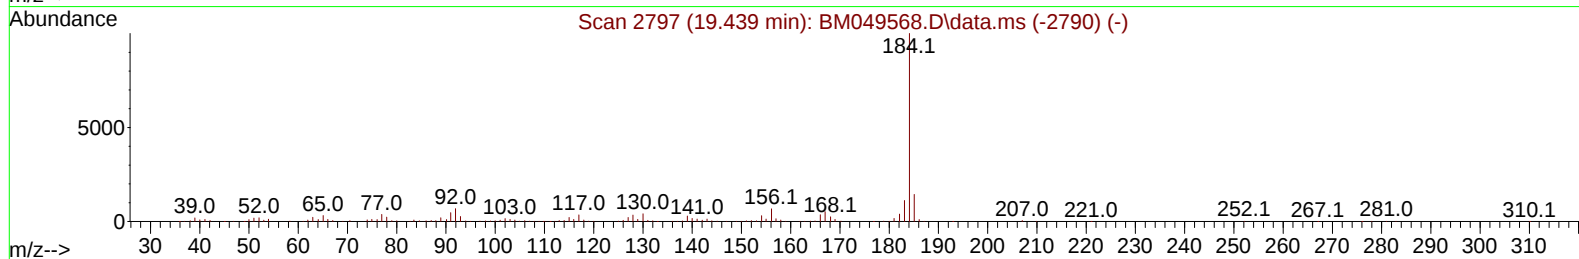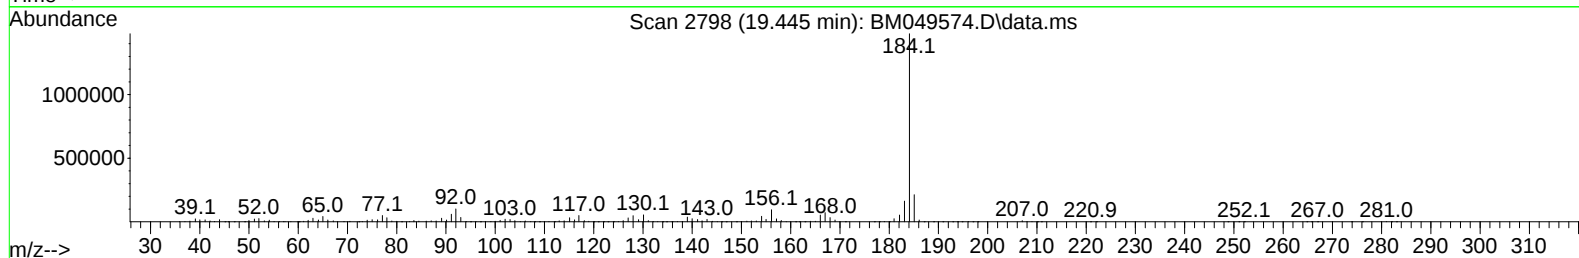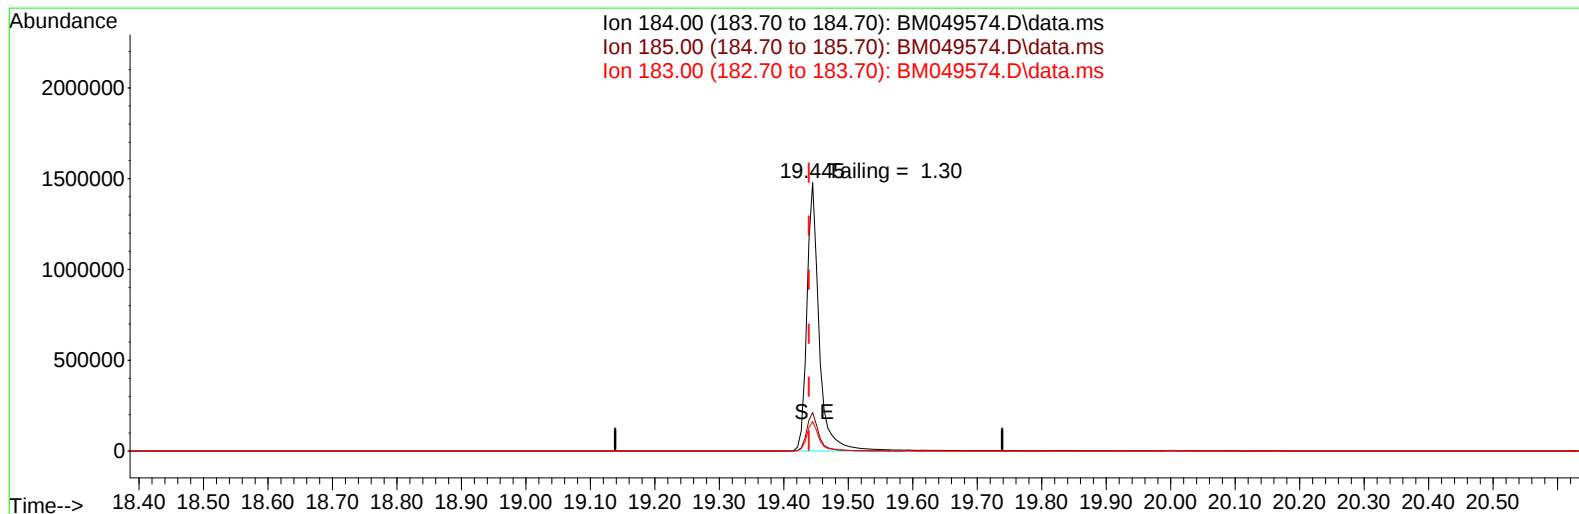

TIC: BM049574.D\data.ms

(77) Benzidine

19.445min (+ 0.006) 3788.91 ng

response 1962980

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.40
183.00	11.10	10.97
0.00	0.00	0.00