

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020625\
 Data File : BM049589.D
 Acq On : 06 Feb 2025 21:36
 Operator : RC/JU
 Sample : PB166339BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB166339BL

Quant Time: Feb 07 01:31:47 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 06 04:55:28 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.822	152	283332	20.000	ng	0.00
21) Naphthalene-d8	10.622	136	984021	20.000	ng	0.00
39) Acenaphthene-d10	14.463	164	559062	20.000	ng	0.00
64) Phenanthrene-d10	17.204	188	984652	20.000	ng	0.00
76) Chrysene-d12	21.439	240	607178	20.000	ng	0.00
86) Perylene-d12	24.468	264	486136	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.399	112	2512073	142.576	ng	0.00
7) Phenol-d6	6.981	99	3055343	132.362	ng	0.00
23) Nitrobenzene-d5	8.975	82	1873446	97.930	ng	0.00
42) 2,4,6-Tribromophenol	15.945	330	825688	124.643	ng	0.00
45) 2-Fluorobiphenyl	13.092	172	4488226	104.001	ng	0.00
79) Terphenyl-d14	19.833	244	6183994	155.526	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020625\
Data File : BM049589.D
Acq On : 06 Feb 2025 21:36
Operator : RC/JU
Sample : PB166339BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB166339BL


Quant Time: Feb 07 01:31:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 04:55:28 2025
Response via : Initial Calibration

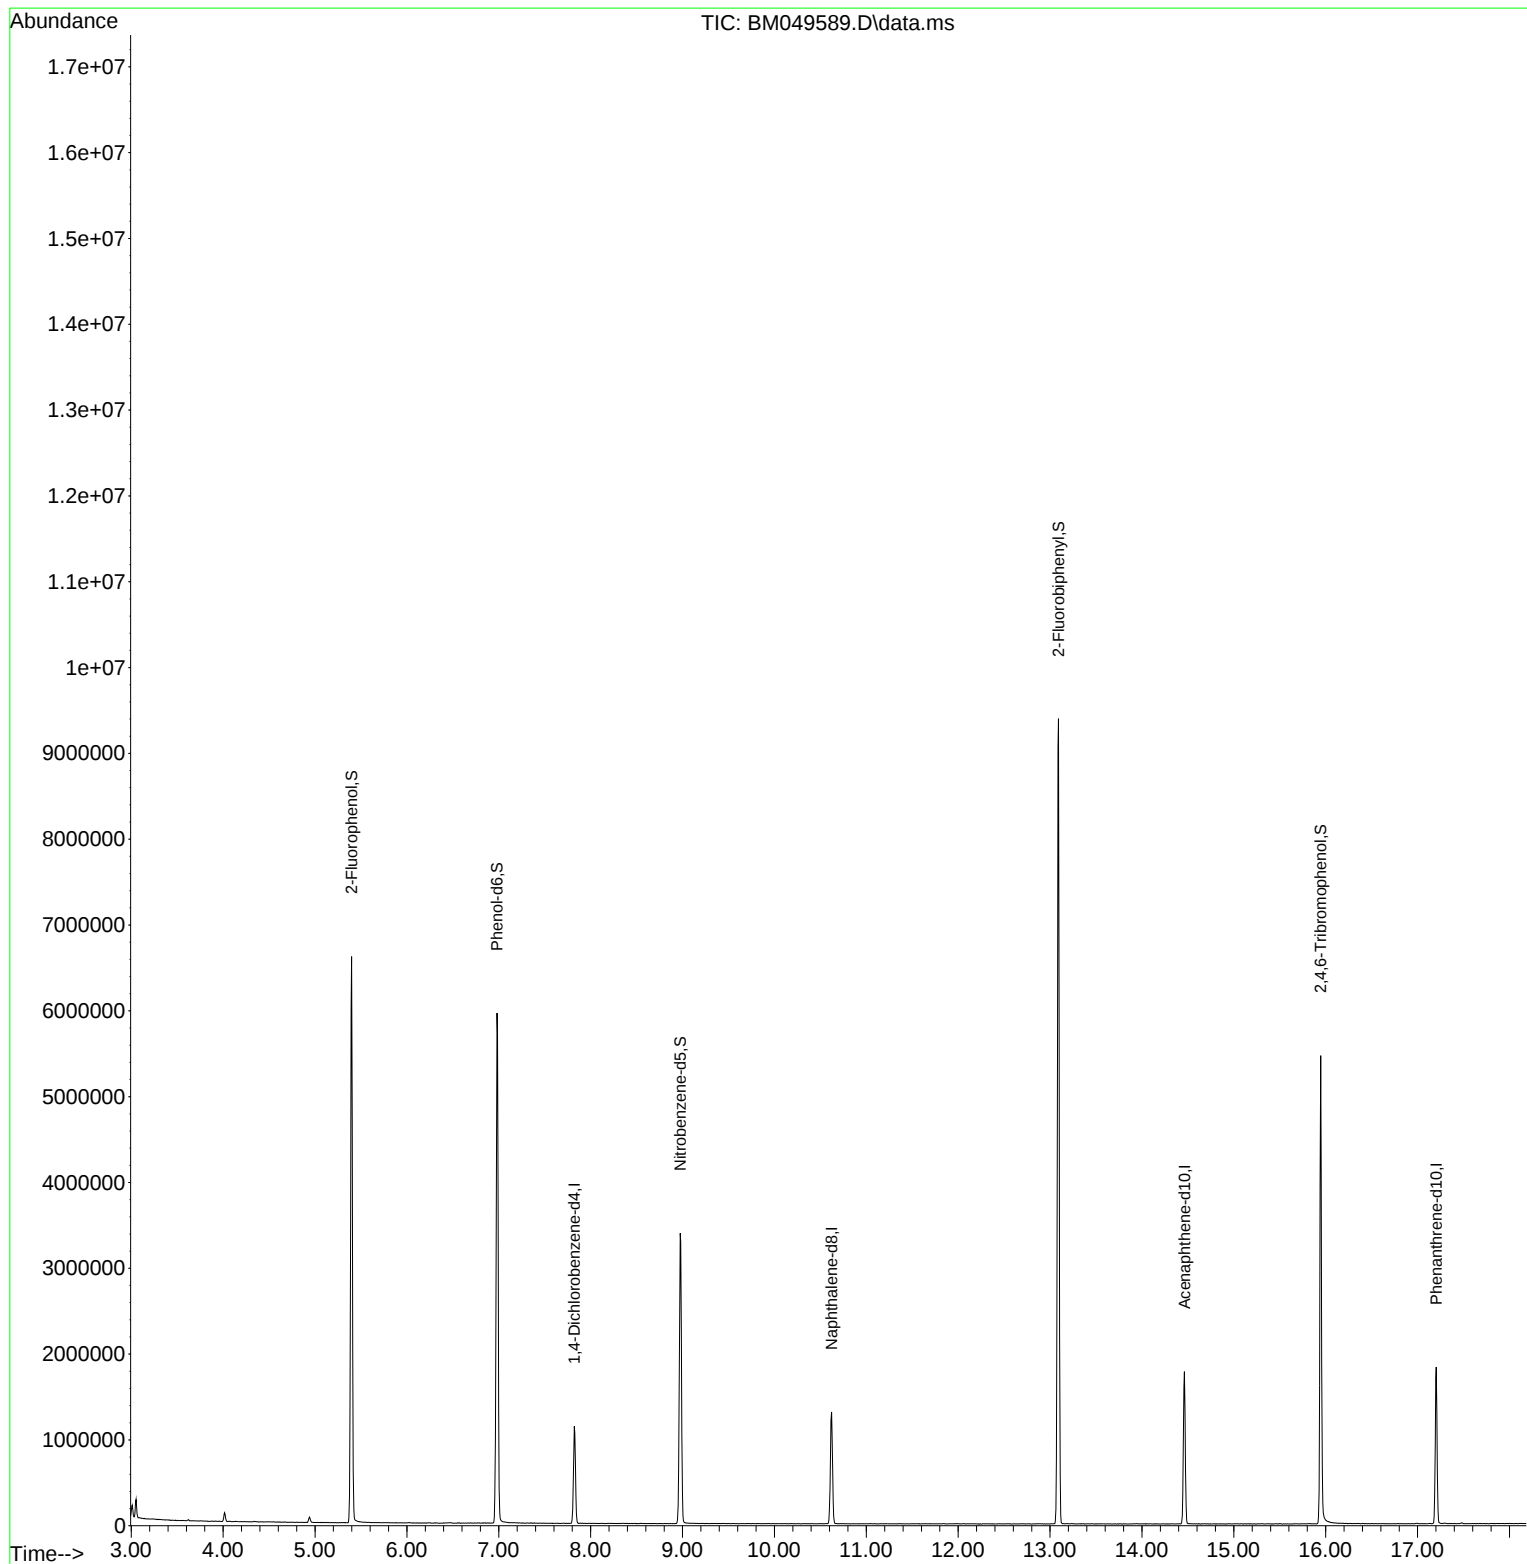


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020625\
Data File : BM049589.D
Acq On : 06 Feb 2025 21:36
Operator : RC/JU
Sample : PB166339BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB166339BL

Quant Time: Feb 07 01:31:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 04:55:28 2025
Response via : Initial Calibration




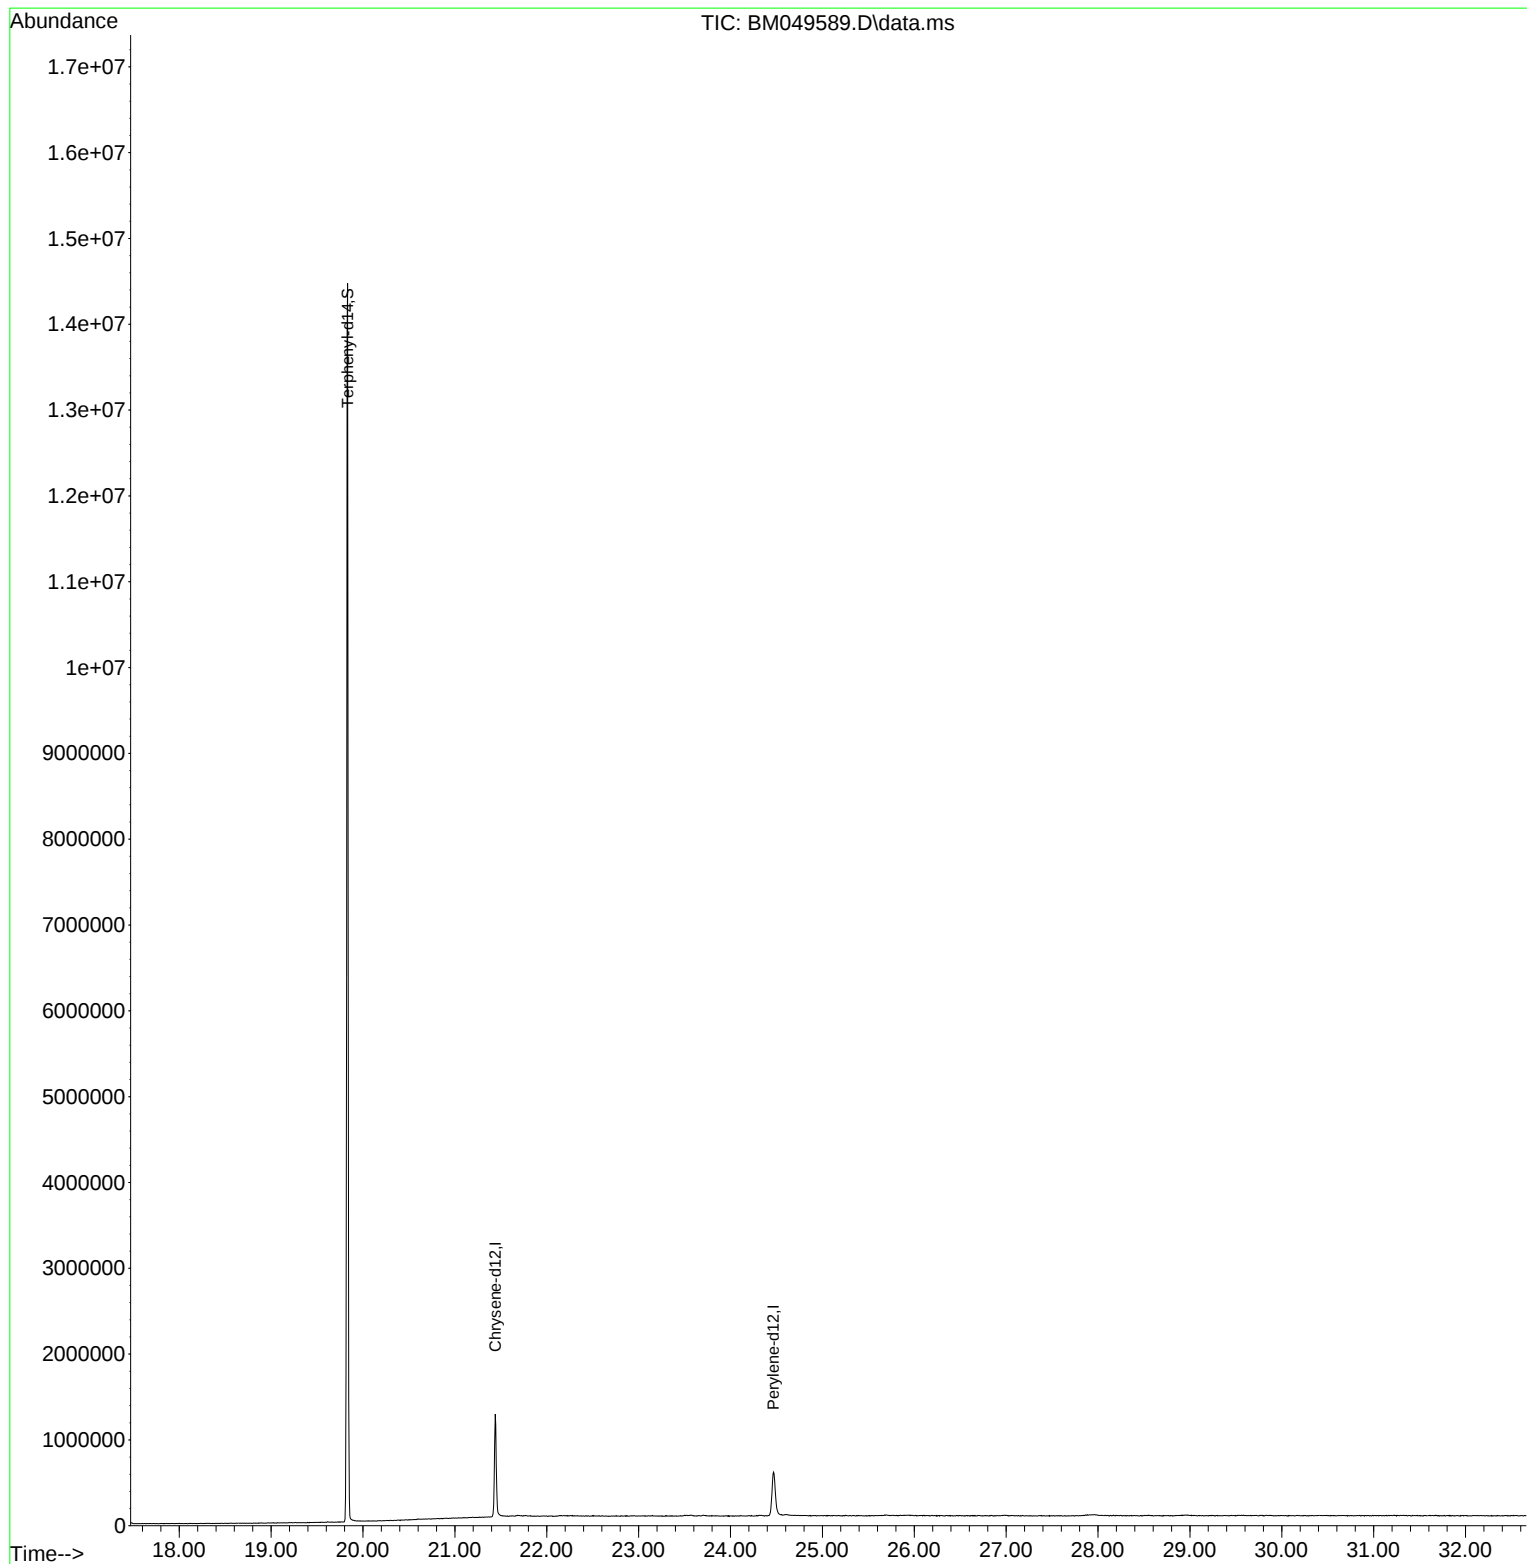


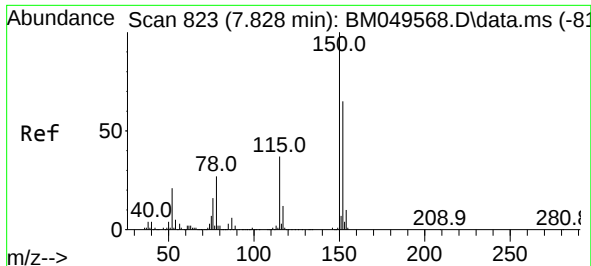

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.822 min Scan# 81
Delta R.T. -0.006 min
Lab File: BM049589.D
Acq: 06 Feb 2025 21:36




Instrument :
BNA_M
ClientSampleId :
PB166339BL


Tgt Ion:152 Resp: 283332
Ion Ratio Lower Upper
152 100
150 155.2 122.6 184.0
115 58.2 45.4 68.0

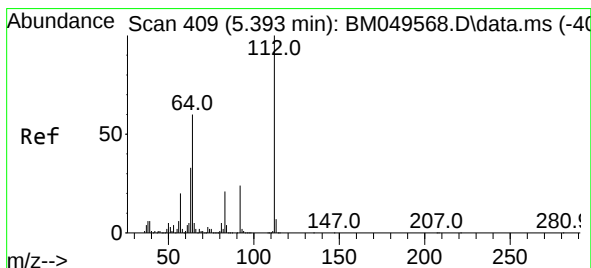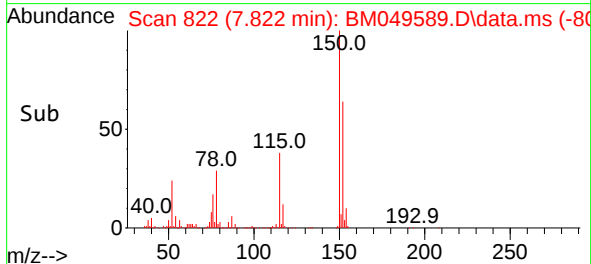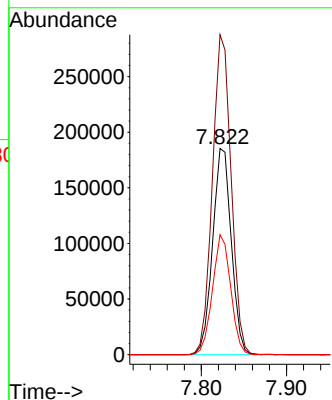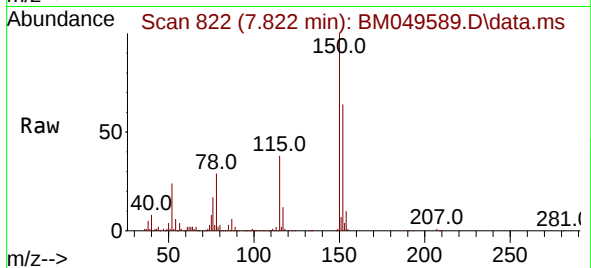

#5
2-Fluorophenol
Concen: 142.576 ng
RT: 5.399 min Scan# 410
Delta R.T. 0.006 min
Lab File: BM049589.D
Acq: 06 Feb 2025 21:36

Tgt Ion:112 Resp: 2512073
Ion Ratio Lower Upper
112 100
64 58.8 47.8 71.8
63 31.9 26.2 39.4


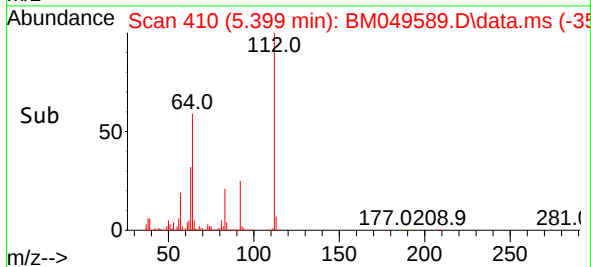
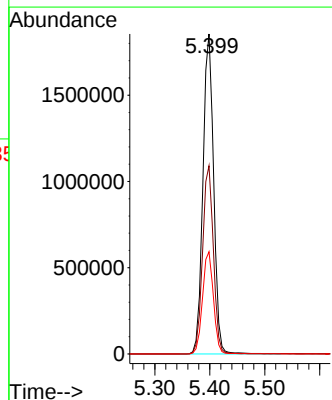
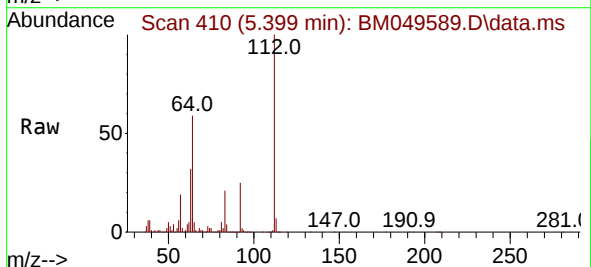


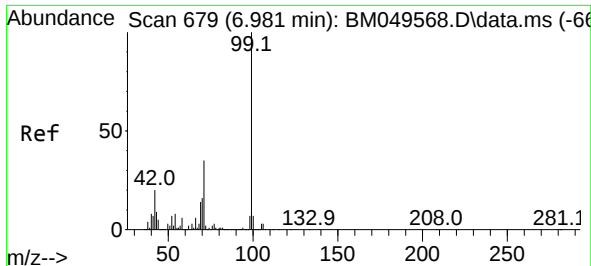

#7
Phenol-d6
Concen: 132.362 ng
RT: 6.981 min Scan# 61
Delta R.T. 0.000 min
Lab File: BM049589.D
Acq: 06 Feb 2025 21:36




Instrument :
BNA_M
ClientSampleId :
PB166339BL


Tgt Ion: 99 Resp: 3055343
Ion Ratio Lower Upper
99 100
42 19.7 16.0 24.0
71 35.4 27.8 41.6

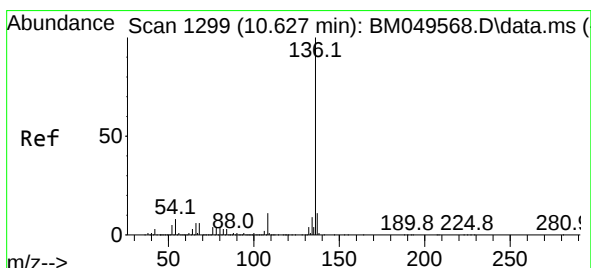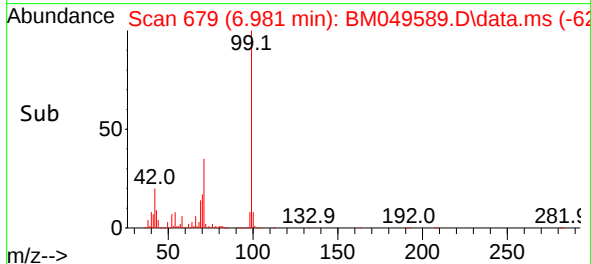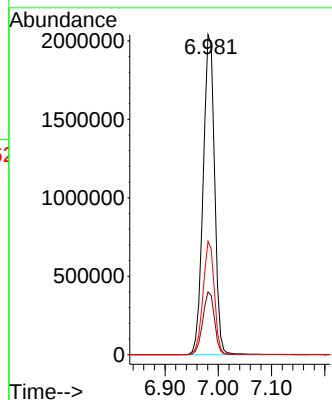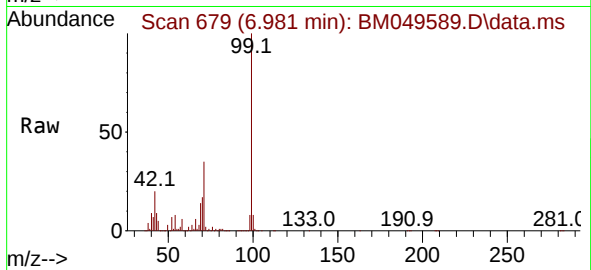

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.622 min Scan# 1298
Delta R.T. -0.006 min
Lab File: BM049589.D
Acq: 06 Feb 2025 21:36

Tgt Ion: 136 Resp: 984021
Ion Ratio Lower Upper
136 100
137 11.0 8.6 13.0
54 8.2 6.6 10.0
68 6.0 4.8 7.2


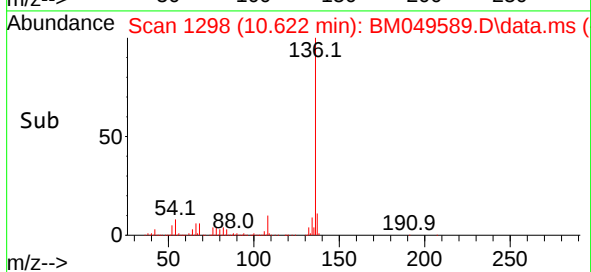
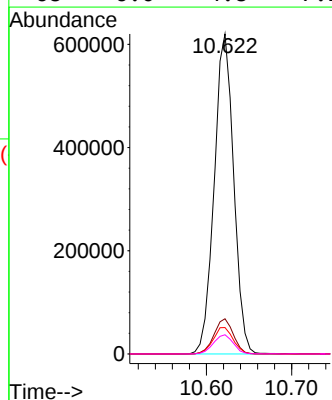
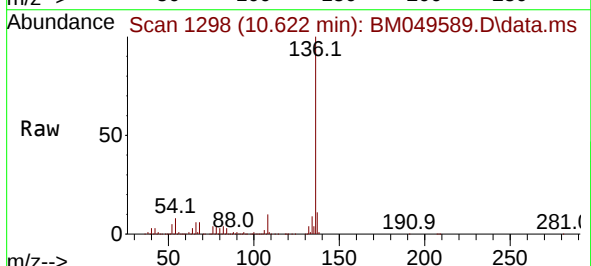


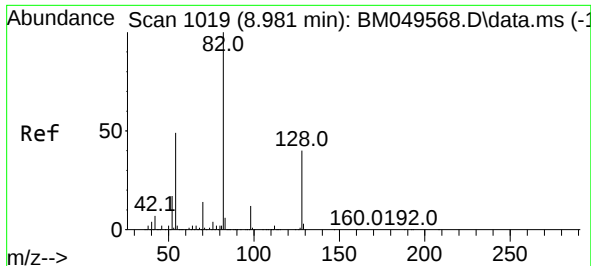

#23
Nitrobenzene-d5
Concen: 97.930 ng
RT: 8.975 min Scan# 1018
Delta R.T. -0.006 min
Lab File: BM049589.D
Acq: 06 Feb 2025 21:36




Instrument :
BNA_M
ClientSampleId :
PB166339BL


Tgt Ion: 82 Resp: 1873446
Ion Ratio Lower Upper
82 100
128 38.6 31.6 47.4
54 49.6 39.4 59.0

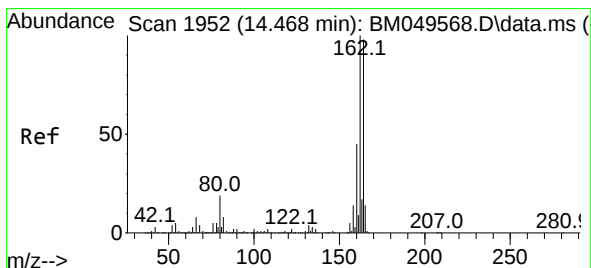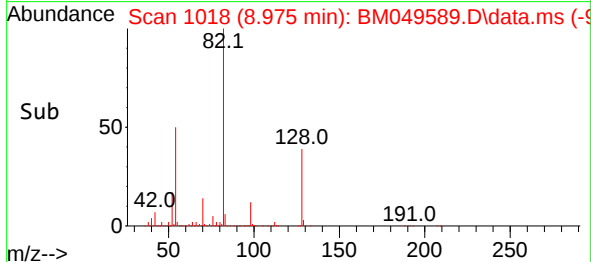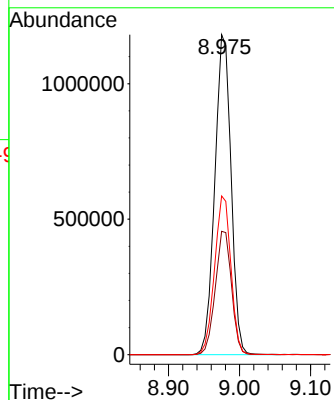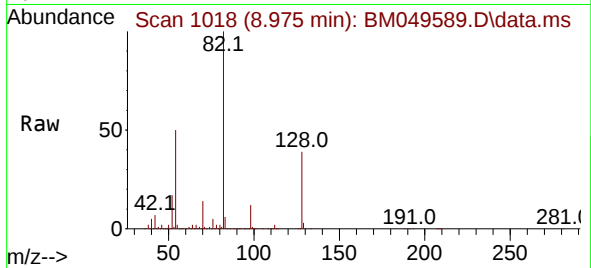

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.463 min Scan# 1951
Delta R.T. -0.006 min
Lab File: BM049589.D
Acq: 06 Feb 2025 21:36

Tgt Ion:164 Resp: 559062
Ion Ratio Lower Upper
164 100
162 97.1 81.4 122.0
160 45.7 36.2 54.4


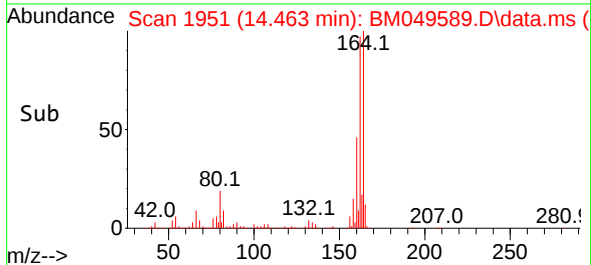
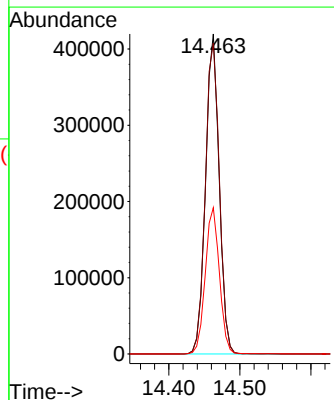
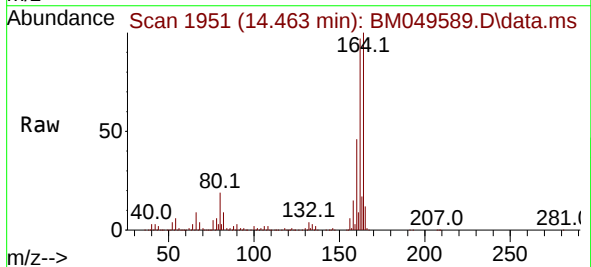


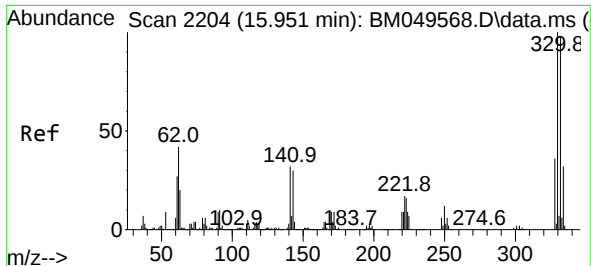

#42
2,4,6-Tribromophenol
Concen: 124.643 ng
RT: 15.945 min Scan# 21
Delta R.T. -0.006 min
Lab File: BM049589.D
Acq: 06 Feb 2025 21:36




Instrument :
BNA_M
ClientSampleId :
PB166339BL


Tgt Ion:330 Resp: 825688
Ion Ratio Lower Upper
330 100
332 95.6 77.3 115.9
141 35.7 28.2 42.2

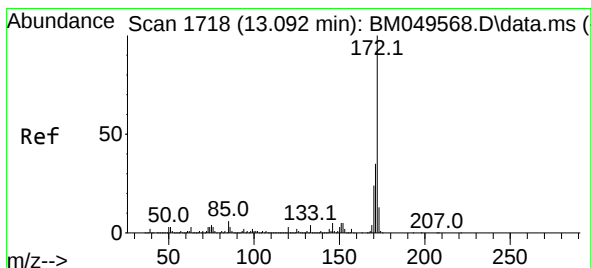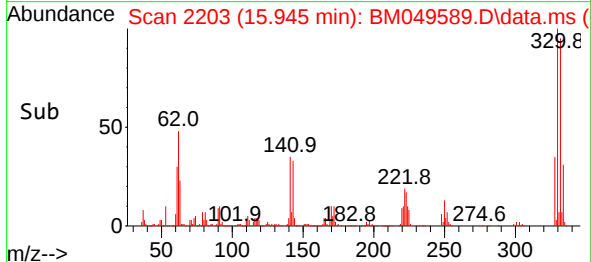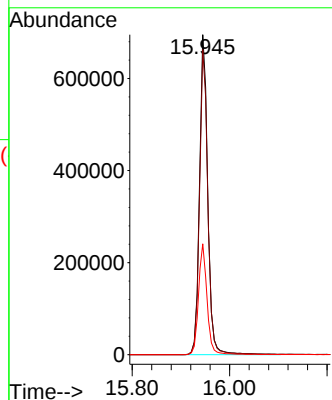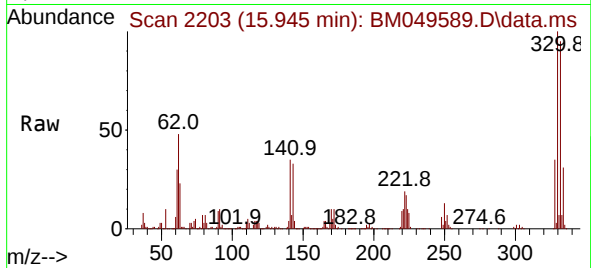

#45
2-Fluorobiphenyl
Concen: 104.001 ng
RT: 13.092 min Scan# 1718
Delta R.T. 0.000 min
Lab File: BM049589.D
Acq: 06 Feb 2025 21:36

Tgt Ion:172 Resp: 4488226
Ion Ratio Lower Upper
172 100
171 34.9 28.0 42.0
170 23.5 19.0 28.4

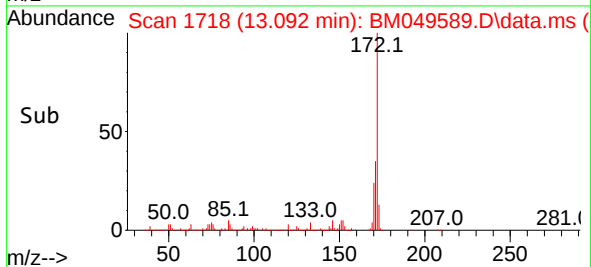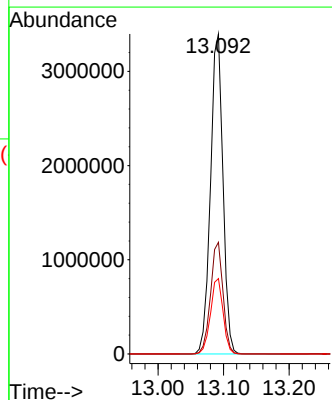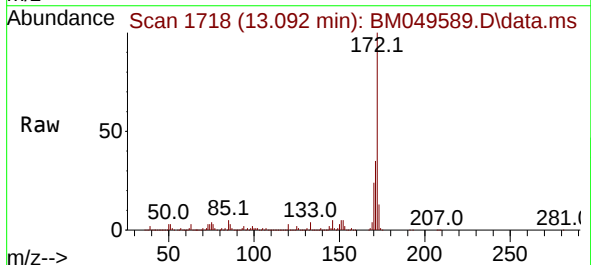

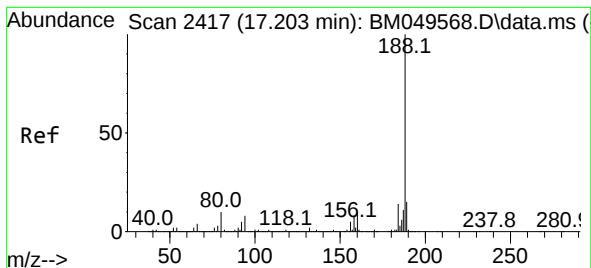

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.204 min Scan# 2417

Delta R.T. 0.000 min

Lab File: BM049589.D

Acq: 06 Feb 2025 21:36

Instrument :

BNA_M

ClientSampleId :

PB166339BL





Tgt Ion:188 Resp: 984652

Ion Ratio Lower Upper

188 100

94 8.0 6.7 10.1

80 9.4 7.7 11.5

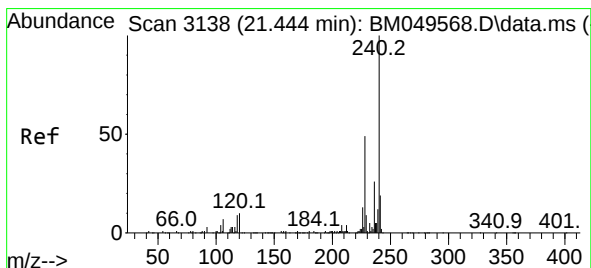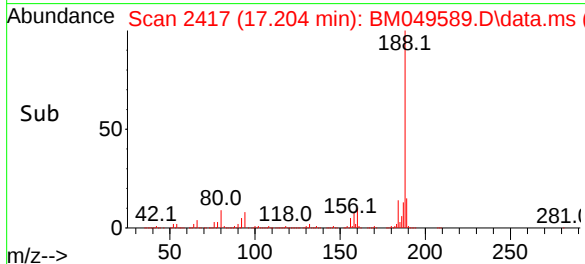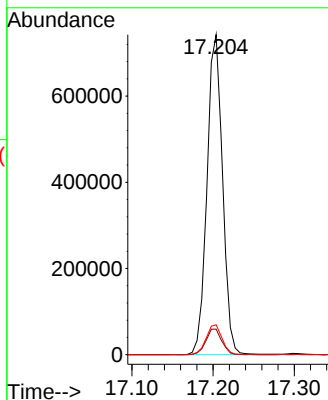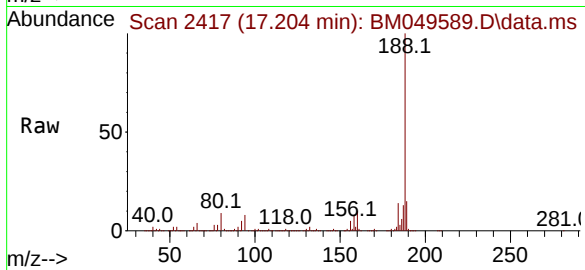

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.439 min Scan# 3137

Delta R.T. -0.006 min

Lab File: BM049589.D

Acq: 06 Feb 2025 21:36




Tgt Ion:240 Resp: 607178


Ion Ratio Lower Upper

240 100

120 10.4 7.8 11.8

236 26.5 20.6 31.0


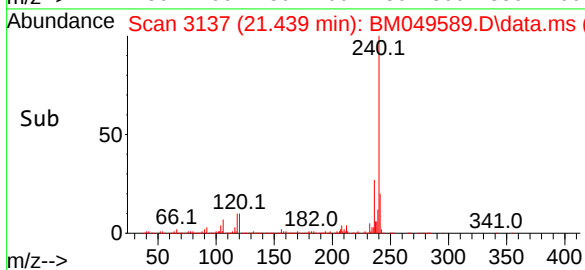
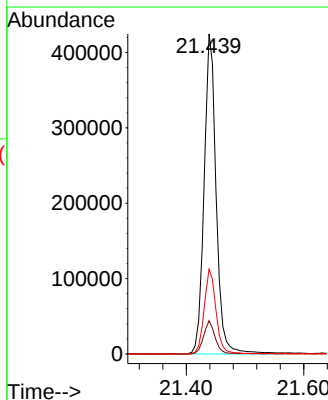
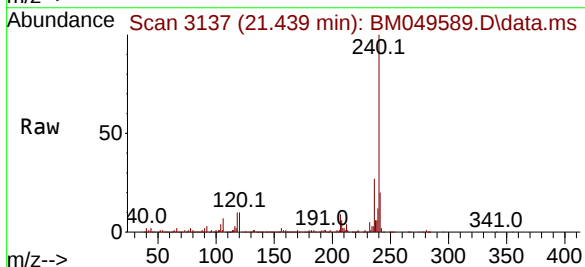


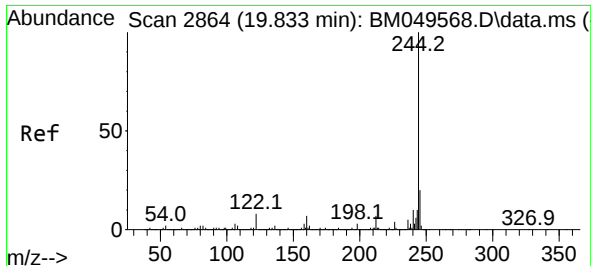

#79
 Terphenyl-d14
 Concen: 155.526 ng
 RT: 19.833 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: BM049589.D
 Acq: 06 Feb 2025 21:36

Instrument :
 BNA_M
 ClientSampleId :
 PB166339BL

Tgt Ion:244 Resp: 6183994
 Ion Ratio Lower Upper
 244 100
 212 7.0 5.8 8.6
 122 7.0 6.2 9.2

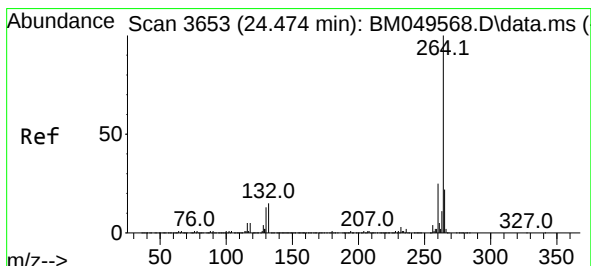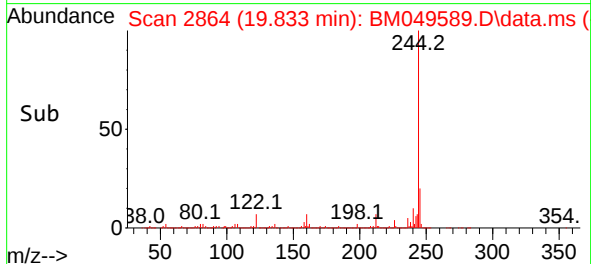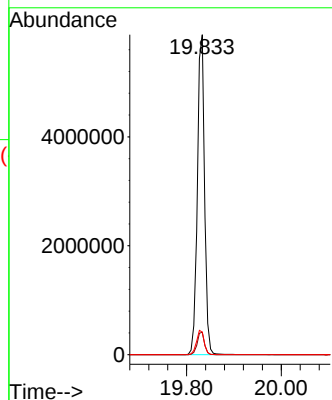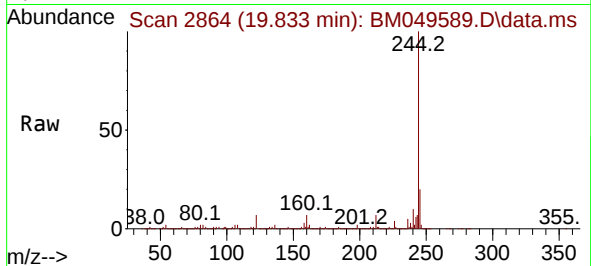

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.468 min Scan# 3652
 Delta R.T. -0.006 min
 Lab File: BM049589.D
 Acq: 06 Feb 2025 21:36

Tgt Ion:264 Resp: 486136
 Ion Ratio Lower Upper
 264 100
 260 23.5 19.8 29.6
 265 21.5 17.5 26.3

