


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020625\
Data File : BM049574.D
Acq On : 06 Feb 2025 09:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 06 04:55:28 2025

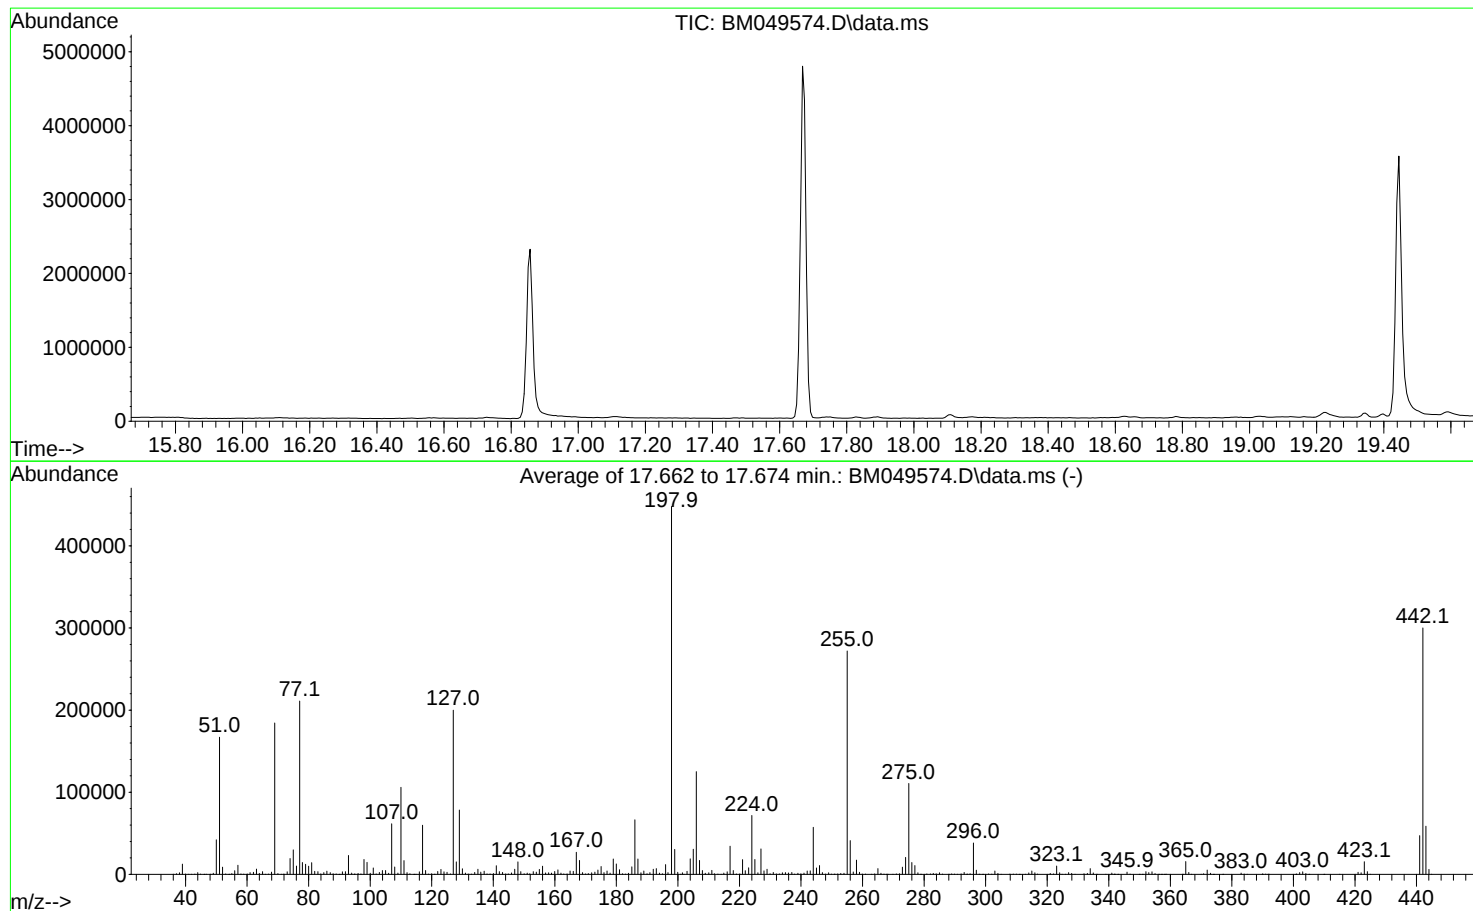




AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	167070	PASS
68	69	0.00	2	1.5	2755	PASS
69	198	0.00	100	41.1	184255	PASS
70	69	0.00	2	0.6	1076	PASS
127	198	10	80	44.6	200000	PASS
197	198	0.00	2	0.5	2181	PASS
198	198	100	100	100.0	447957	PASS
199	198	5	9	6.8	30424	PASS
275	198	10	60	24.7	110723	PASS
365	198	1	100	3.5	15633	PASS
441	198	0.01	100	10.5	47120	PASS
442	442	50	100	100.0	300117	PASS
443	442	15	24	19.6	58720	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020625\
Data File : BM049574.D
Acq On : 06 Feb 2025 09:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 06 11:21:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 04:55:28 2025
Response via : Initial Calibration

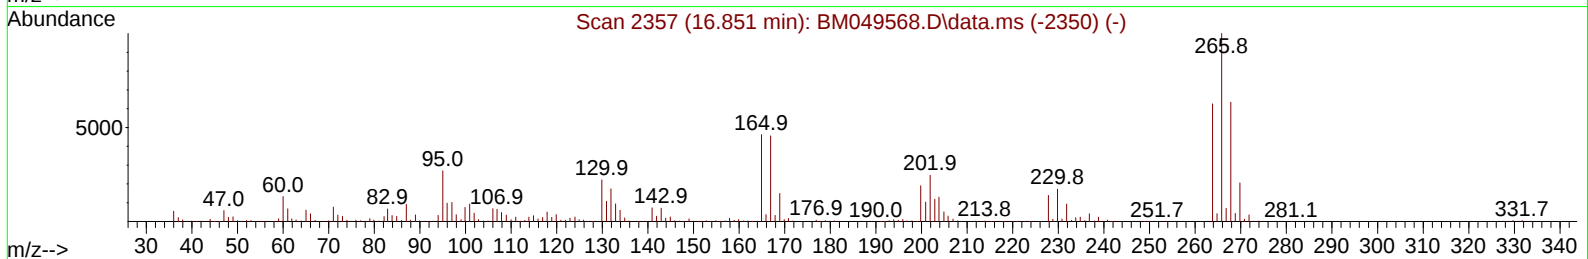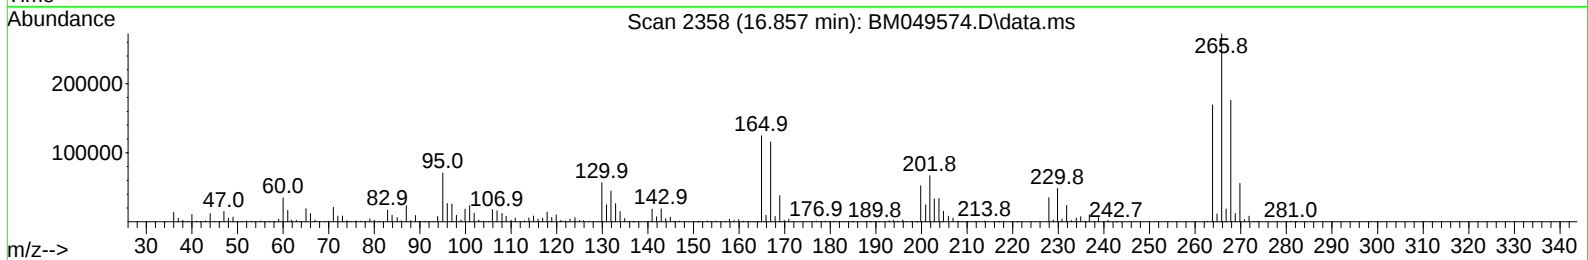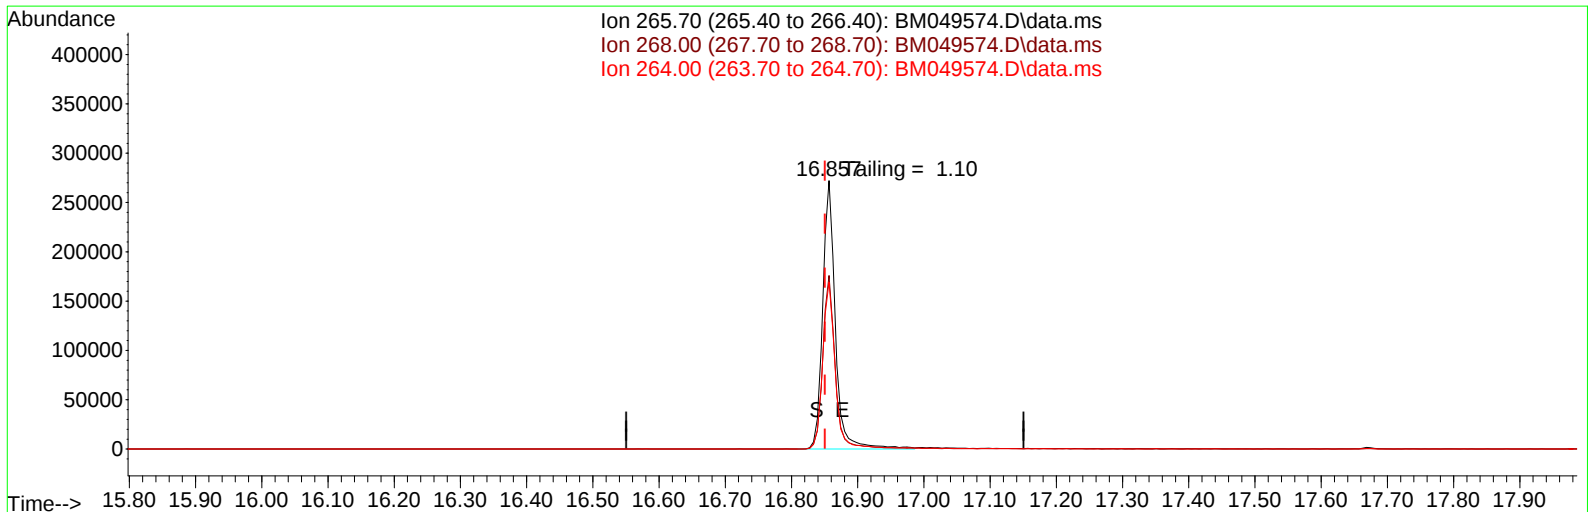

TIC: BM049574.D\data.ms

(70) Pentachlorophenol (C)

16.857min (+ 0.006) 68938.79 ng




response 363868

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	64.66
264.00	62.50	62.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020625\
Data File : BM049574.D
Acq On : 06 Feb 2025 09:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 06 11:21:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 04:55:28 2025
Response via : Initial Calibration

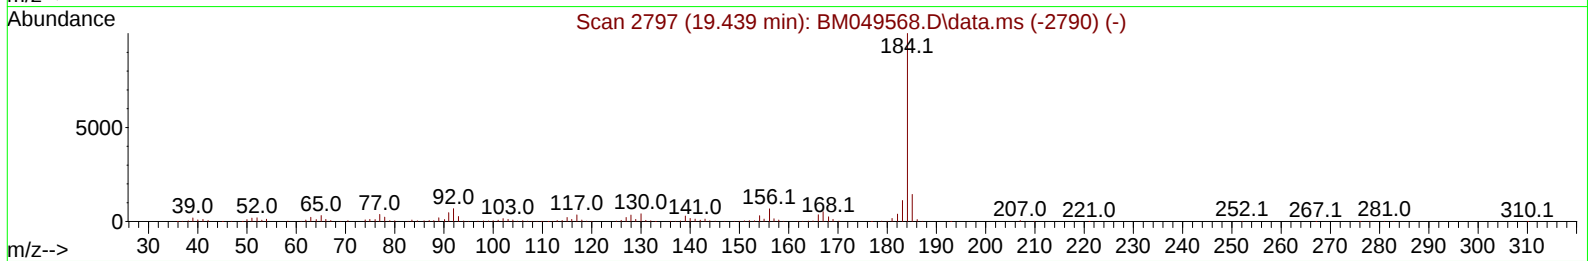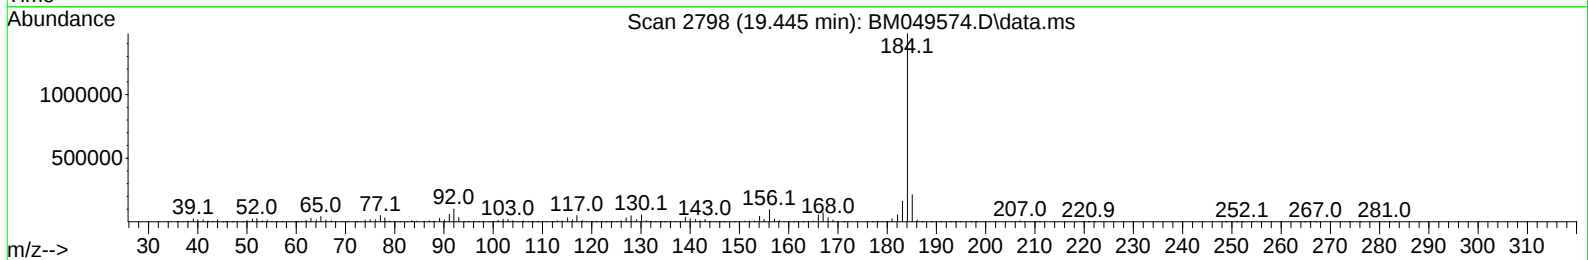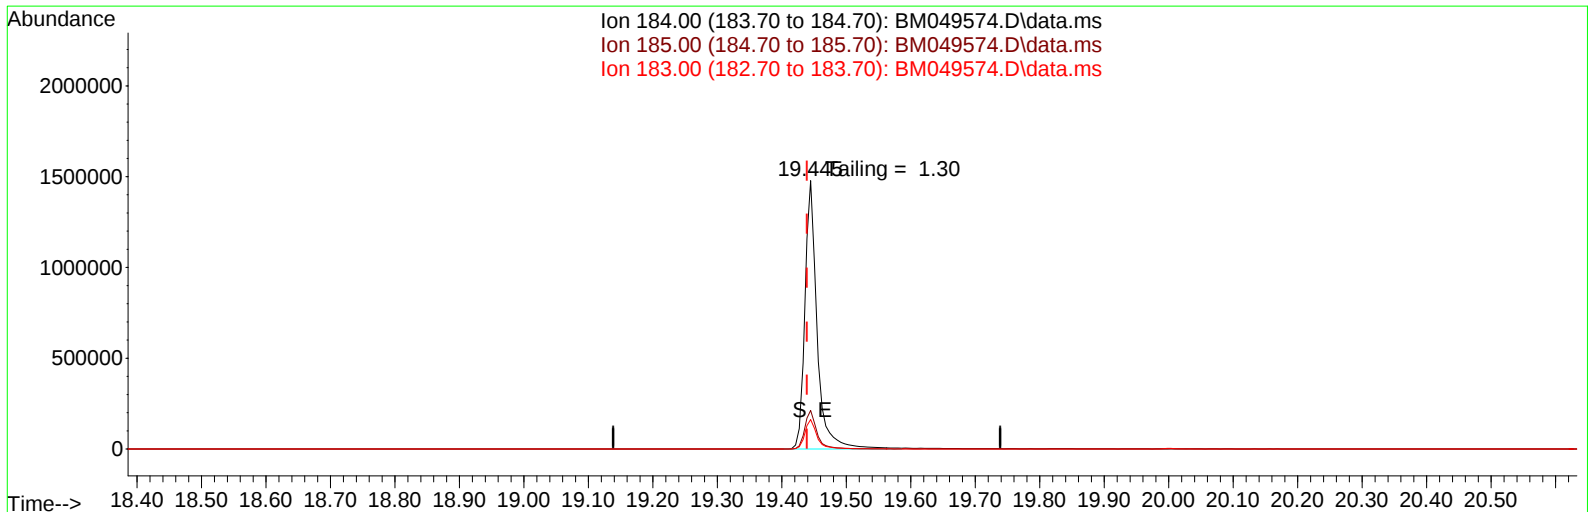

TIC: BM049574.D\data.ms

(77) Benzidine

19.445min (+ 0.006) 3788.91 ng

response 1962980

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.40
183.00	11.10	10.97
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/6/2025	BNA_M	<u>BM049574.D</u>
Compound Name	Response	Retention Time
DDT	900788	20.692
DDD	24796	20.251
DDE	3824	19.745
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28620	929408	3.08

Instrument :
BNA_M
ClientSampleId :
DFTPP