


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020625\
Data File : BM049587.D
Acq On : 06 Feb 2025 20:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 06 04:55:28 2025

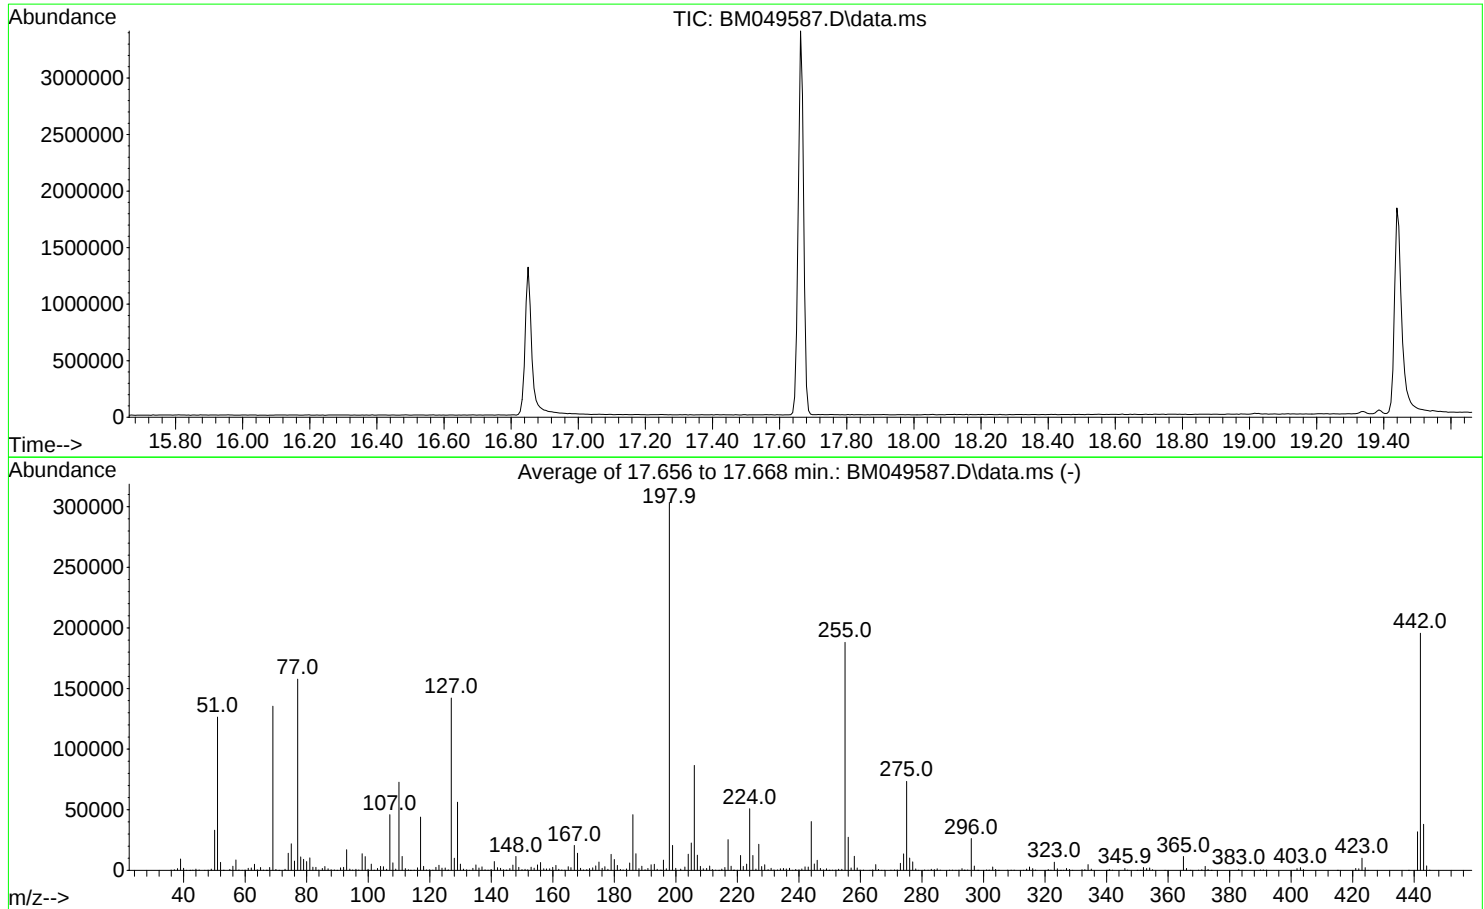




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.7	126470	PASS
68	69	0.00	2	1.7	2329	PASS
69	198	0.00	100	44.6	135461	PASS
70	69	0.00	2	0.6	817	PASS
127	198	10	80	46.9	142205	PASS
197	198	0.00	2	0.4	1298	PASS
198	198	100	100	100.0	303467	PASS
199	198	5	9	6.8	20603	PASS
275	198	10	60	24.2	73405	PASS
365	198	1	100	3.8	11443	PASS
441	198	0.01	100	10.5	31773	PASS
442	442	50	100	100.0	195587	PASS
443	442	15	24	19.4	38016	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020625\
Data File : BM049587.D
Acq On : 06 Feb 2025 20:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 07 01:57:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 04:55:28 2025
Response via : Initial Calibration

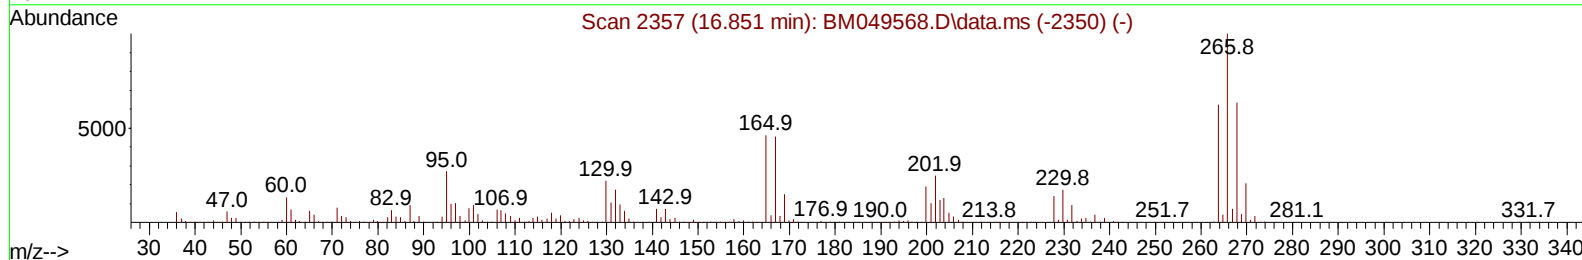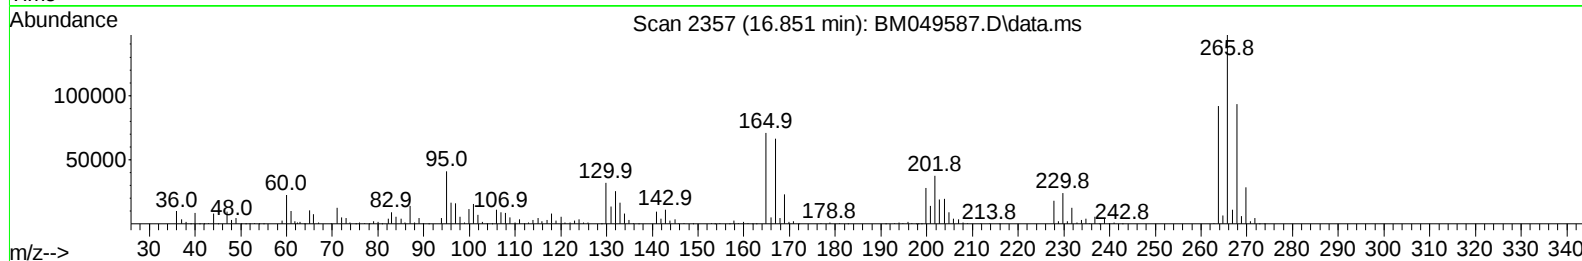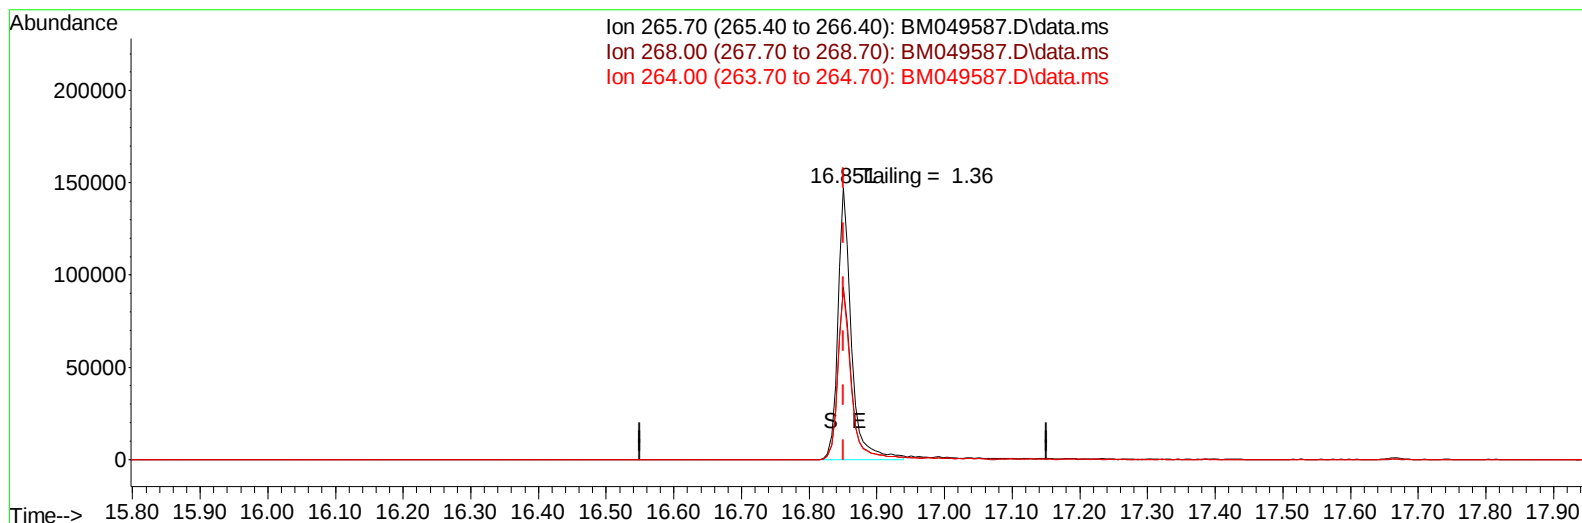

TIC: BM049587.D\data.ms

(70) Pentachlorophenol (C)

16.851min (+ 0.000) 287468.81 ng




response 203278

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	63.37
264.00	62.50	62.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020625\
Data File : BM049587.D
Acq On : 06 Feb 2025 20:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 07 01:57:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 04:55:28 2025
Response via : Initial Calibration

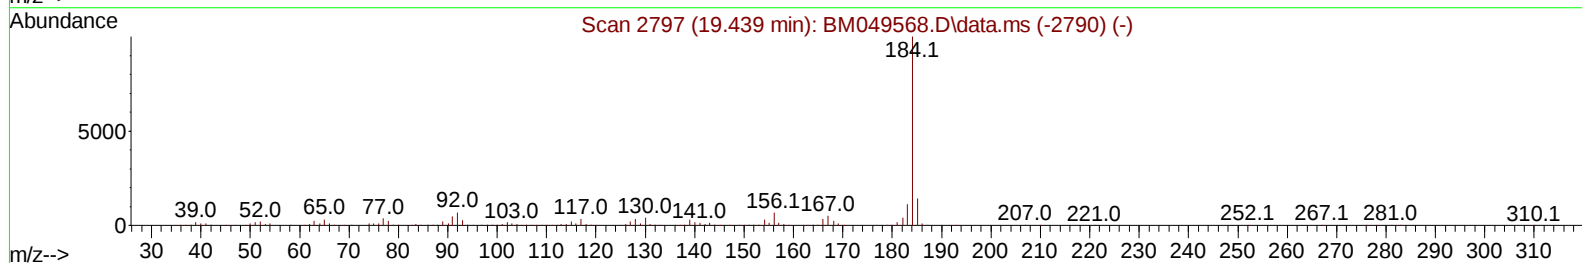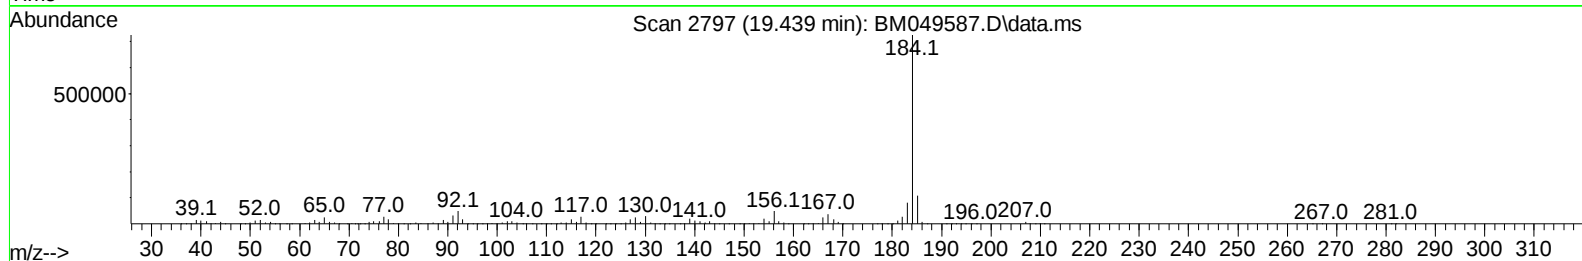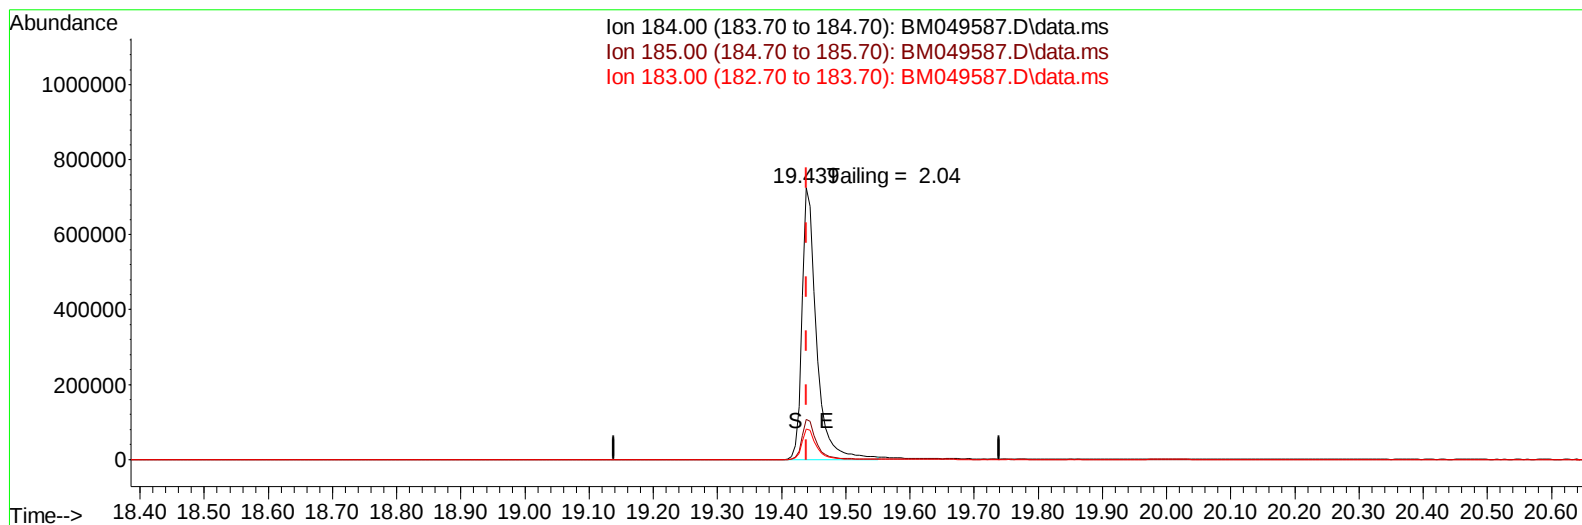

TIC: BM049587.D\data.ms

(77) Benzidine

19.439min (+ 0.000) 99810.22 ng

response 1159645

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.87
183.00	11.10	11.33
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/6/2025	BNA_M	<u>BM049587.D</u>
Compound Name	Response	Retention Time
DDT	502324	20.686
DDD	9999	20.245
DDE	1837	19.739
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11836	514160	2.30

Instrument :
BNA_M
ClientSampleId :
DFTPP