
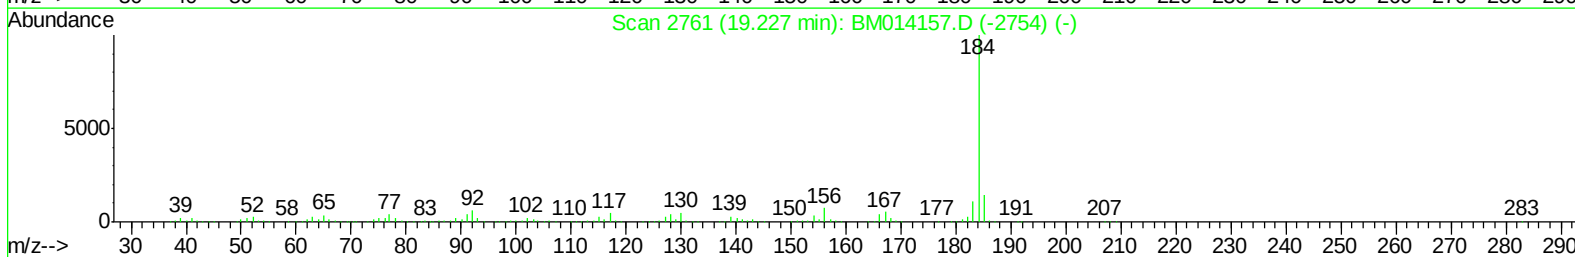
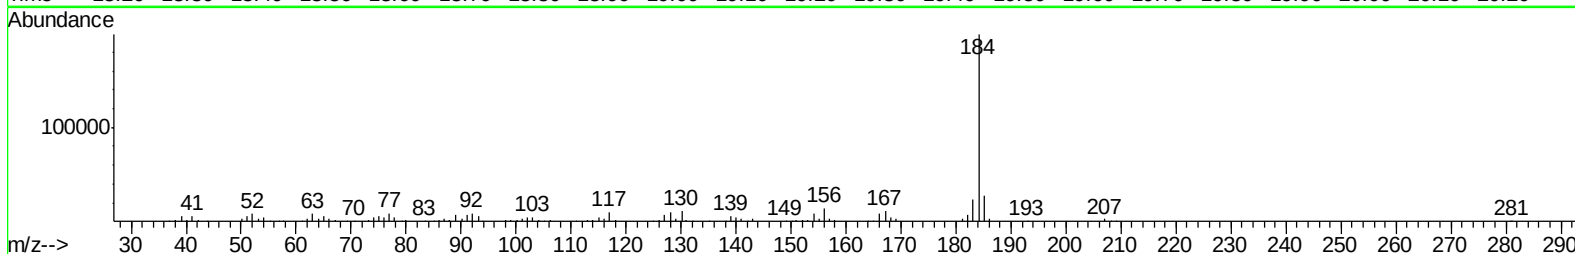


Data Path : Z:\HPCHEM1\BNA M\Data\BM020718\
Data File : BM014165.D
Acq On : 07 Feb 2018 17:43
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 08:07:26 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 07 17:16:49 2018
Response via : Initial Calibration

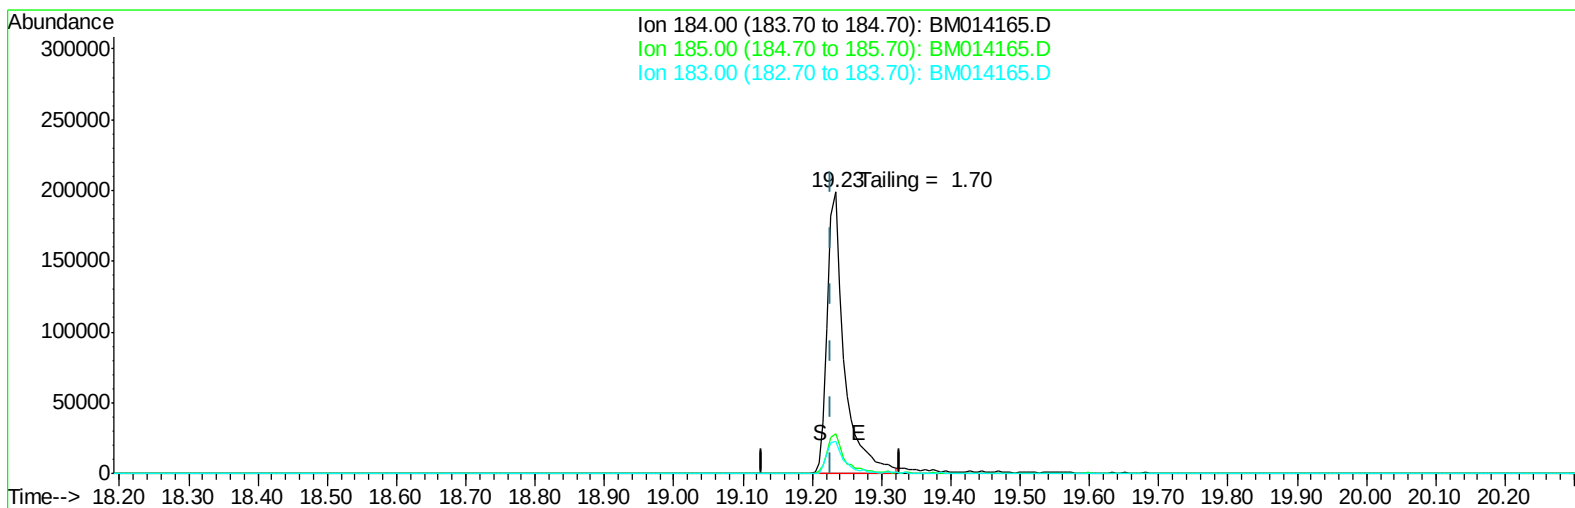

TIC: BM014165.D

(76) Benzidine




19.233min (+0.006) 0.00ng m

response 338695

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.10
183.00	11.10	11.55
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\Data\BM020718\
Data File : BM014165.D
Acq On : 07 Feb 2018 17:43
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 08:07:26 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 07 17:16:49 2018
Response via : Initial Calibration

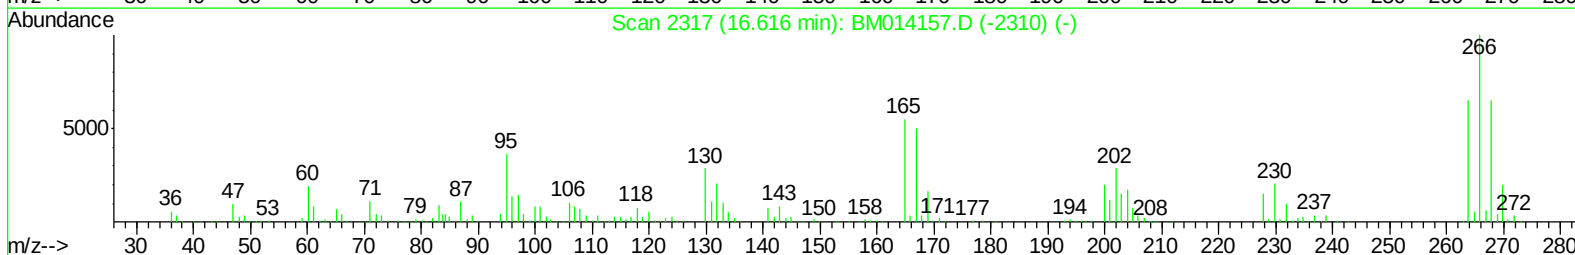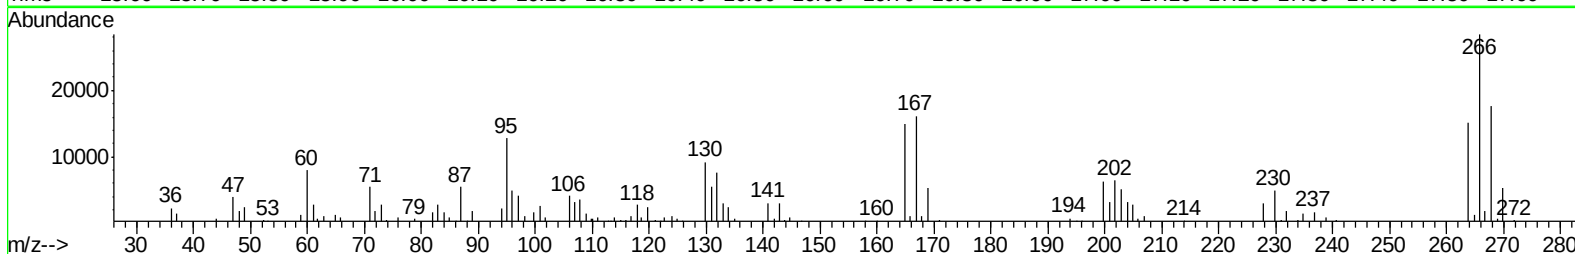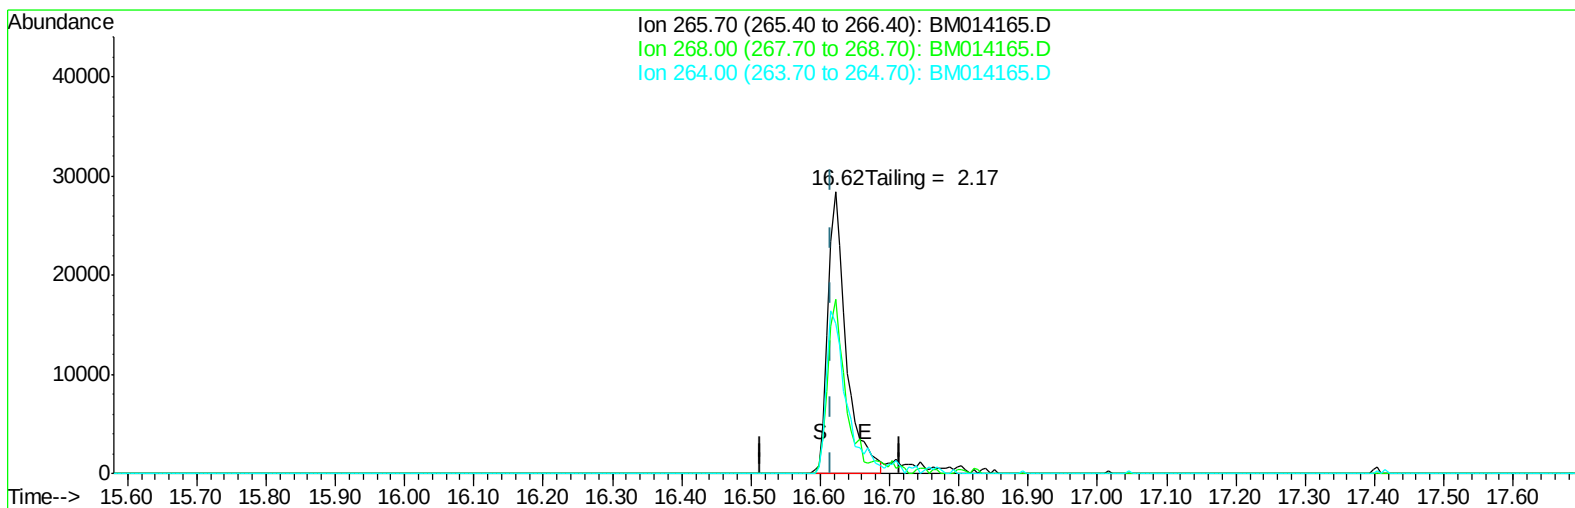

TIC: BM014165.D

(69) Pentachlorophenol (C)

16.621min (+0.006) 0.00ng

response 52569

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	61.82
264.00	61.20	53.36
0.00	0.00	0.00