

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020718\
 Data File : BM014165.D
 Acq On : 07 Feb 2018 17:43
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Feb 08 08:07:26 2018
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM020718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 07 17:16:49 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ng	-7.55
21) Naphthalene-d8	0.00	136	0	0.00	ng	-10.32
38) Acenaphthene-d10	0.00	164	0	0.00	ng	-14.20
63) Phenanthrene-d10	0.00	188	0	0.00	ng	-16.96
75) Chrysene-d12	0.00	240	0	0.00	ng	-21.17
86) Perylene-d12	0.00	264	0	0.00	ng	-23.34
System Monitoring Compounds						
5) 2-Fluorophenol	0.00	112	0	0.00	ng	
7) Phenol-d6	0.00	99	0	0.00	ng	
23) Nitrobenzene-d5	0.00	82	0	0.00	ng	
41) 2,4,6-Tribromophenol	0.00	330	0	0.00	ng	
44) 2-Fluorobiphenyl	0.00	172	0	0.00	ng	
78) Terphenyl-d14	0.00	244	0	0.00	ng	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020718\
Data File : BM014165.D
Acq On : 07 Feb 2018 17:43
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 08 08:07:26 2018
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 07 17:16:49 2018
Response via : Initial Calibration


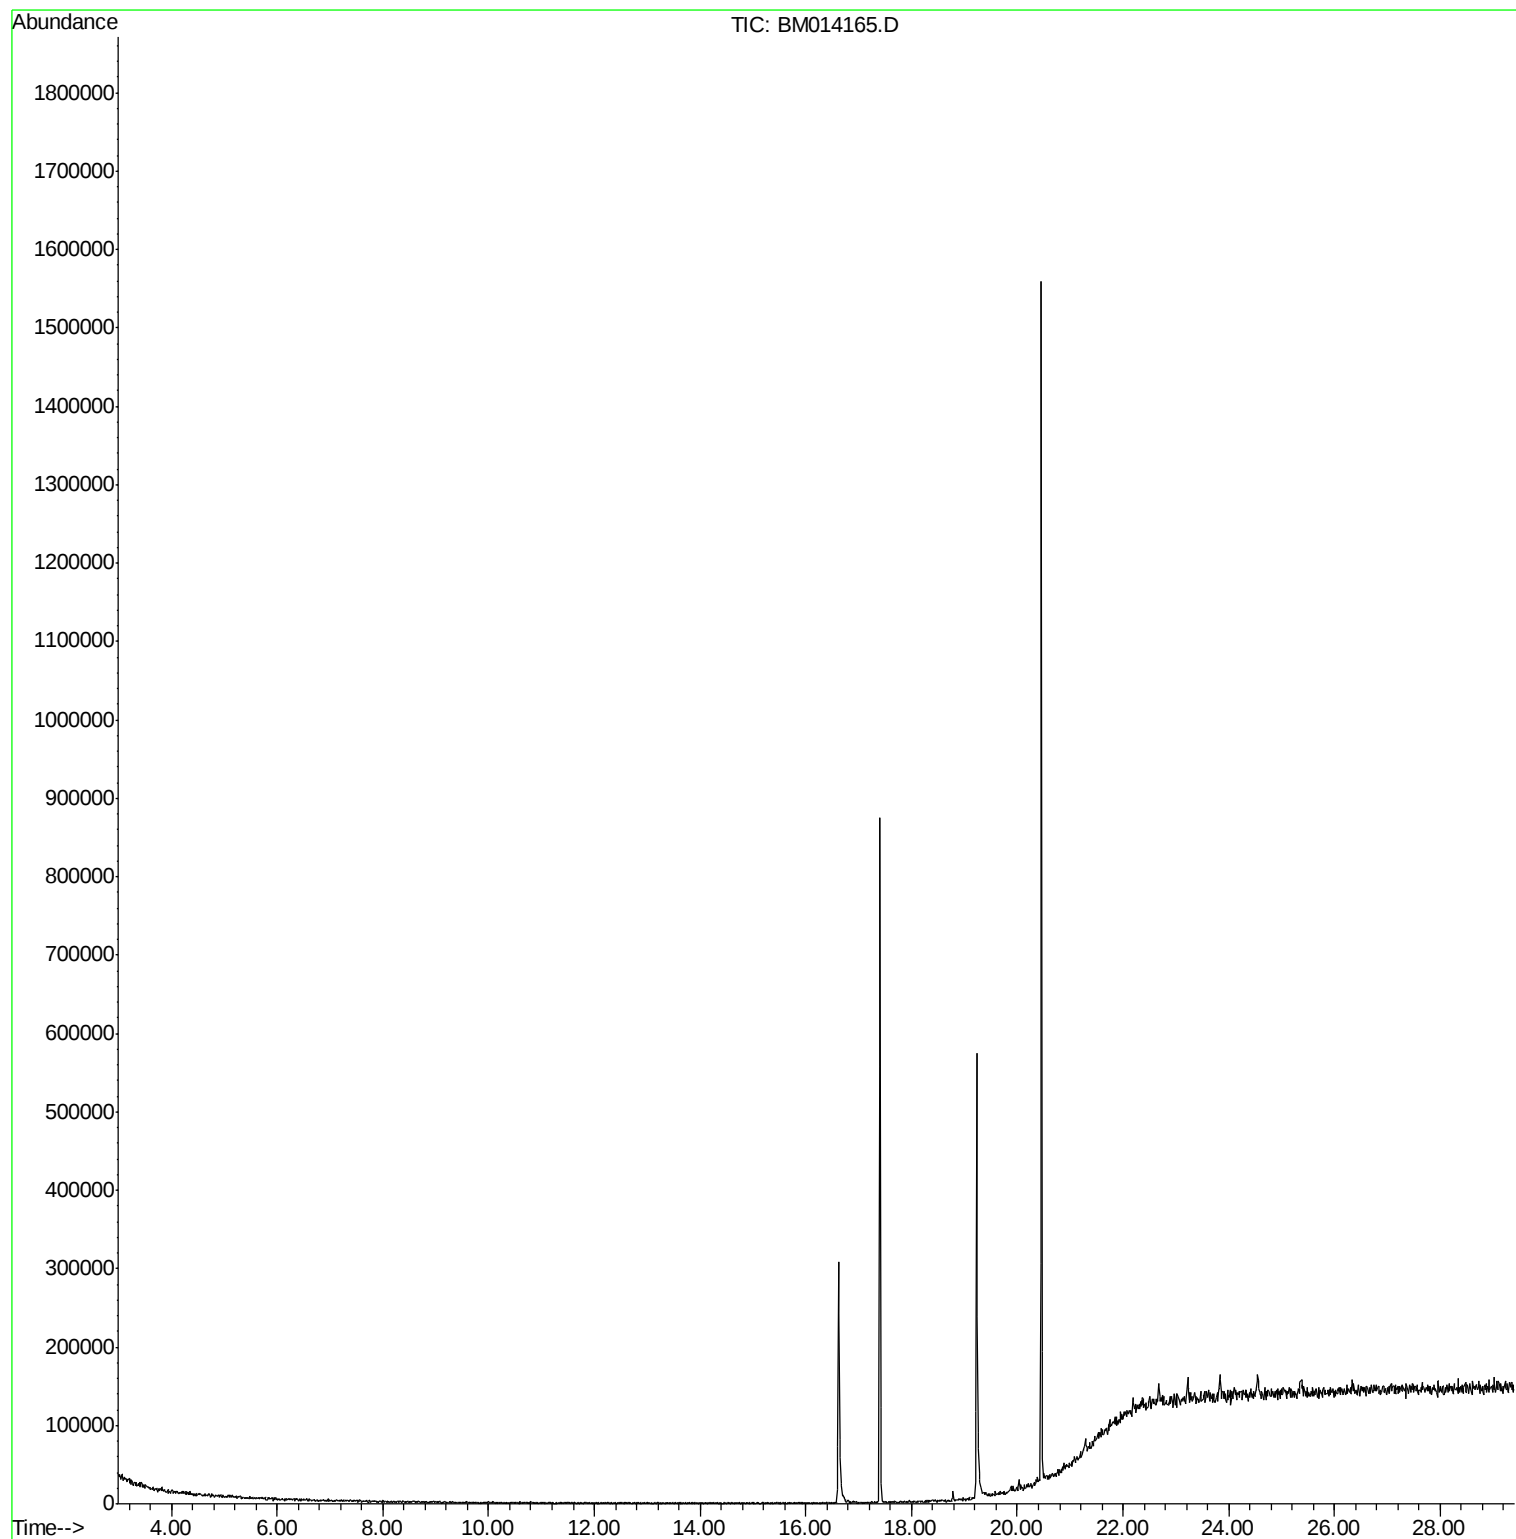


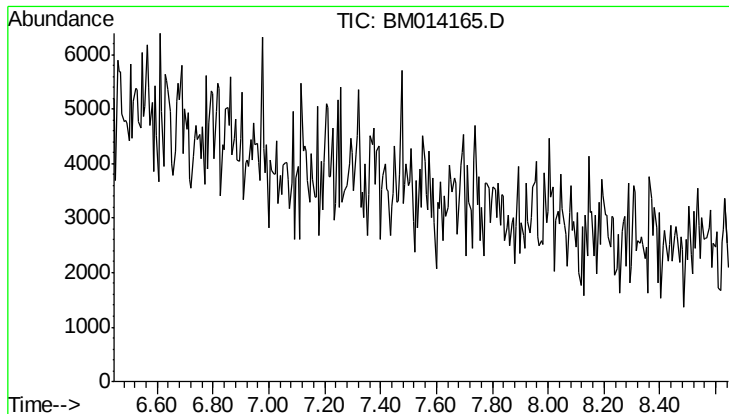

#1
 1,4-Dichlorobenzene-d4
 Concen: 0.00 ng
 Expected RT: 7.55 min
 Lab File: BM014165.D
 Acq: 07 Feb 2018 17:43


Instrument :
 BNA_M
 ClientSampleId :
 DFTPP


Tgt Ion: 152
 Sig Exp Ratio
 152 100
 150 149.4
 115 53.7

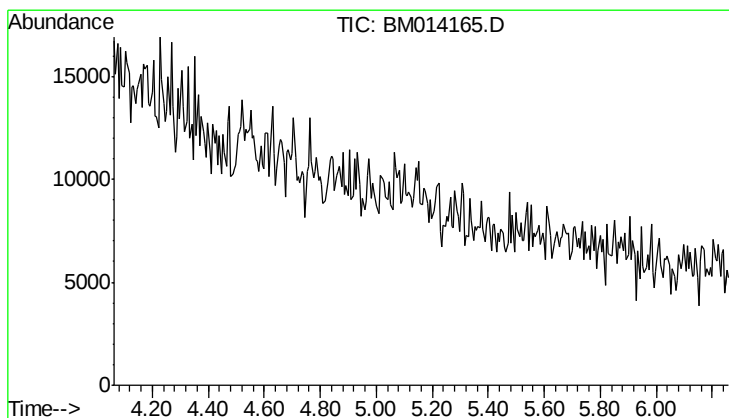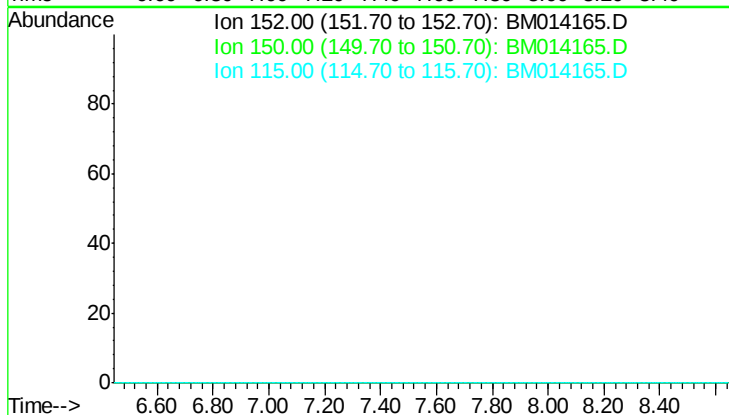

#5
 2-Fluorophenol
 Concen: 0.00 ng
 Expected RT: 5.16 min
 Lab File: BM014165.D
 Acq: 07 Feb 2018 17:43

Tgt Ion: 112
 Sig Exp Ratio
 112 100
 64 48.2
 63 24.1

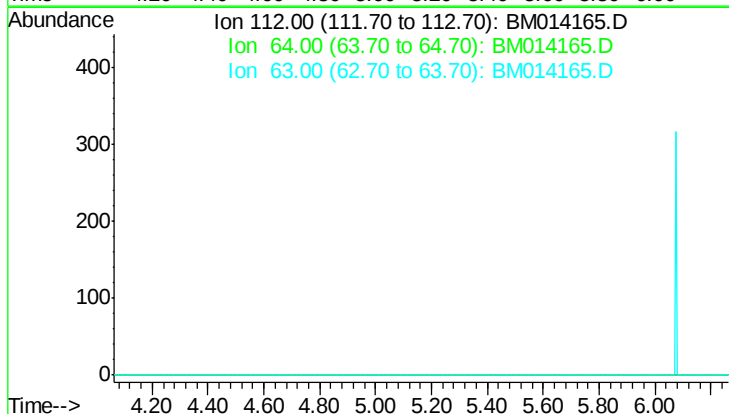

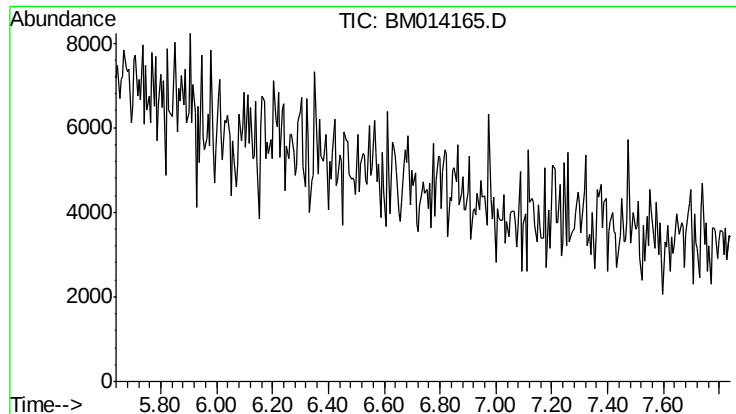

#7

Phenol-d6

Concen: 0.00 ng

Expected RT: 6.74 min

Lab File: BM014165.D

Acq: 07 Feb 2018 17:43

Instrument :

BNA_M

ClientSampleId :

DFTPP



Tgt Ion: 99

Sig Exp Ratio

99 100

42 13.7

71 29.3

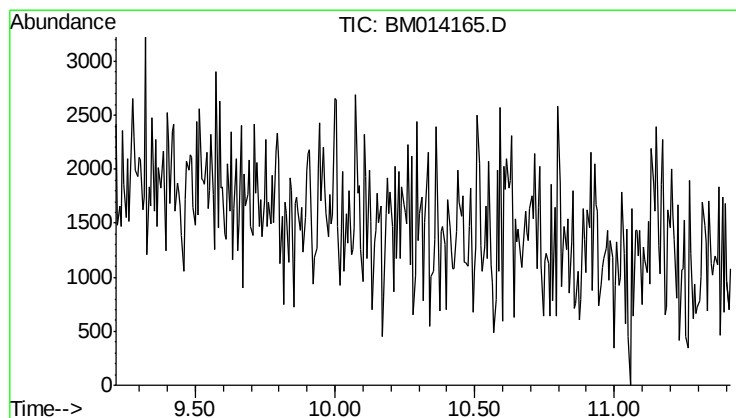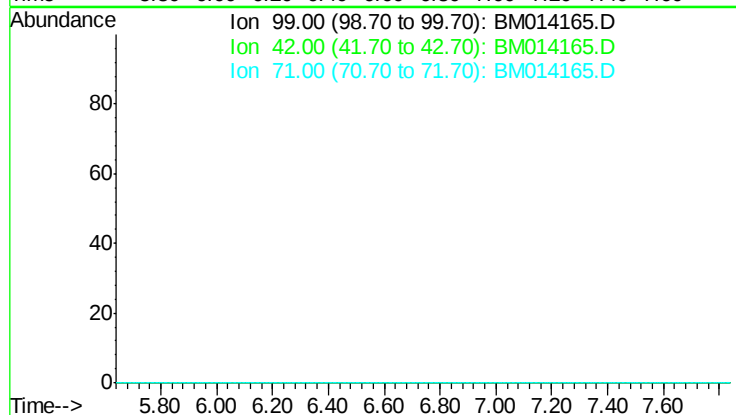

#21

Naphthalene-d8

Concen: 0.00 ng

Expected RT: 10.32 min

Lab File: BM014165.D

Acq: 07 Feb 2018 17:43

Tgt Ion: 136


Sig Exp Ratio


136 100

137 10.9

54 5.7

68 4.6


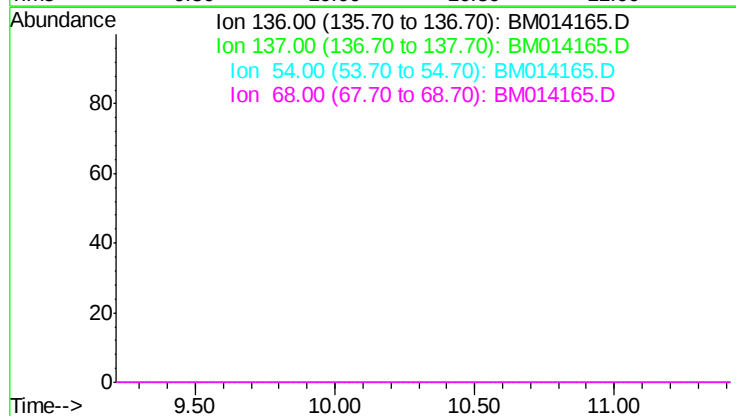


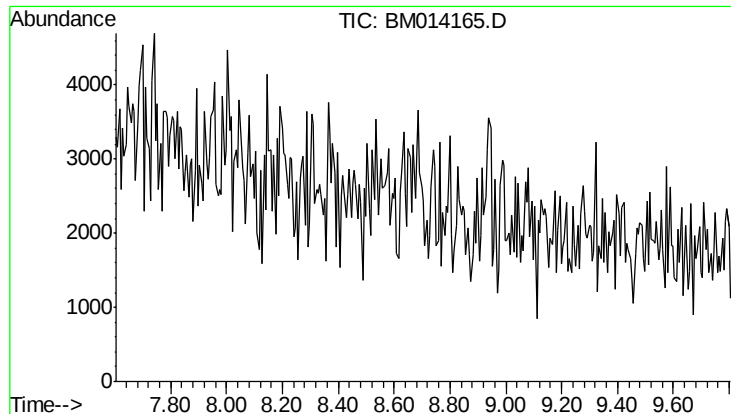

#23
 Nitrobenzene-d5
 Concen: 0.00 ng
 Expected RT: 8.70 min
 Lab File: BM014165.D
 Acq: 07 Feb 2018 17:43


Instrument :
 BNA_M
 ClientSampleId :
 DFTPP


Tgt Ion	Exp Ratio
82	100
128	41.0
54	50.7

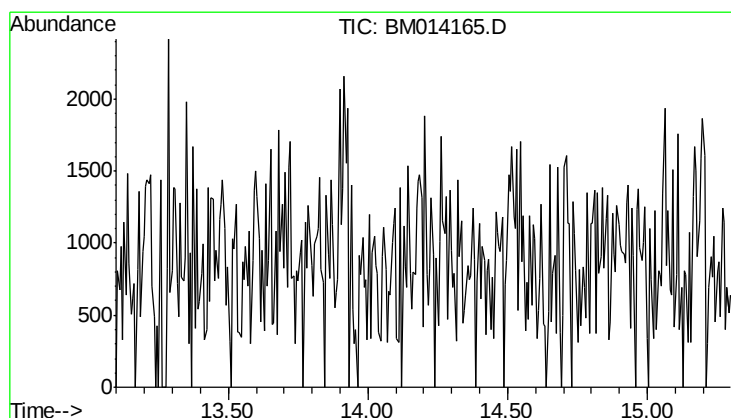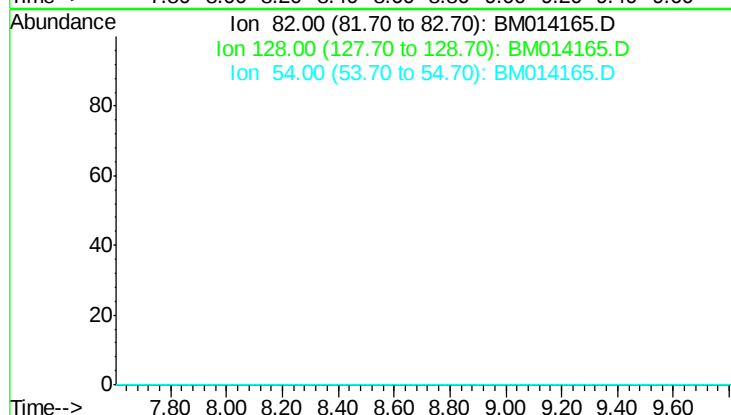

#38
 Acenaphthene-d10
 Concen: 0.00 ng
 Expected RT: 14.20 min
 Lab File: BM014165.D
 Acq: 07 Feb 2018 17:43

Tgt Ion	Exp Ratio
164	100
162	103.0
160	44.7

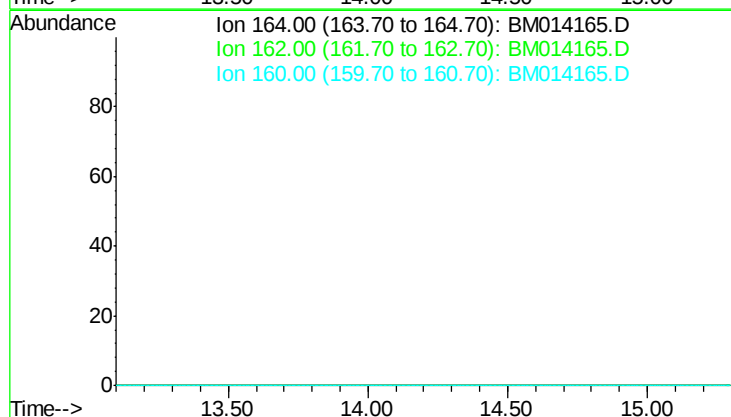


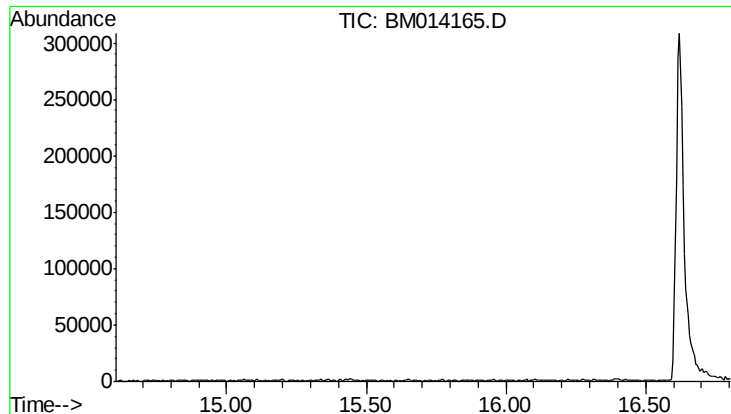


#41
 2,4,6-Tribromophenol
 Concen: 0.00 ng
 Expected RT: 15.70 min
 Lab File: BM014165.D
 Acq: 07 Feb 2018 17:43

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Tgt Ion: 330


Sig	Exp Ratio
330	100
332	0.0
141	0.0

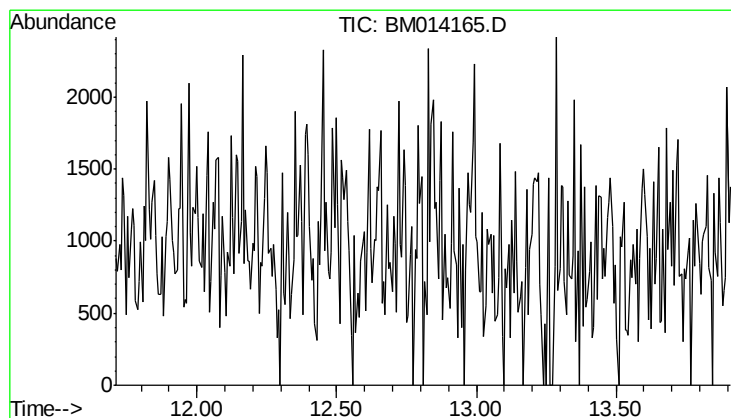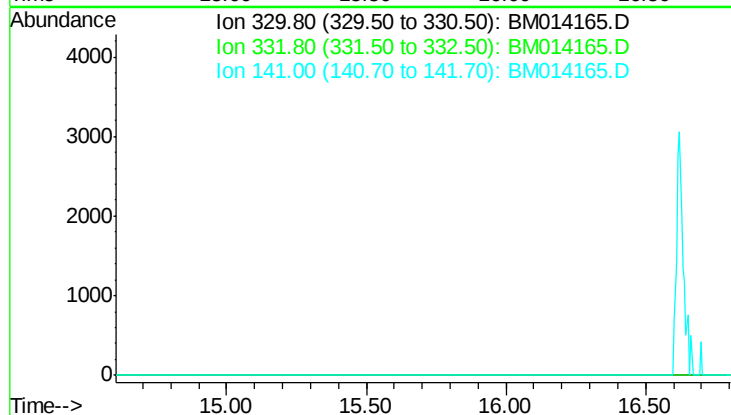


#44
 2-Fluorobiphenyl
 Concen: 0.00 ng
 Expected RT: 12.81 min
 Lab File: BM014165.D
 Acq: 07 Feb 2018 17:43

Tgt Ion: 172

Sig	Exp Ratio
172	100
171	35.6
170	23.5


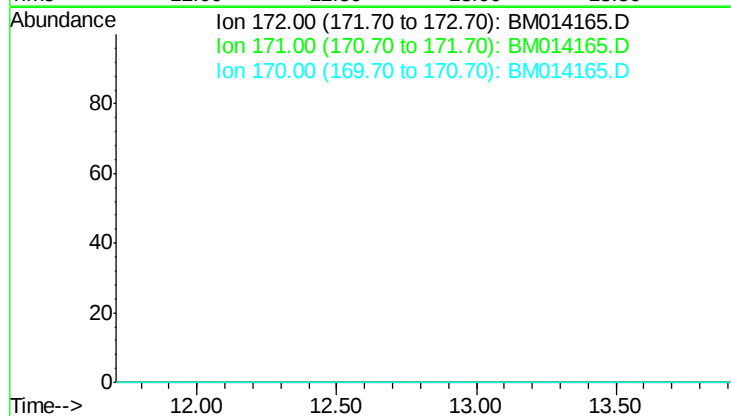


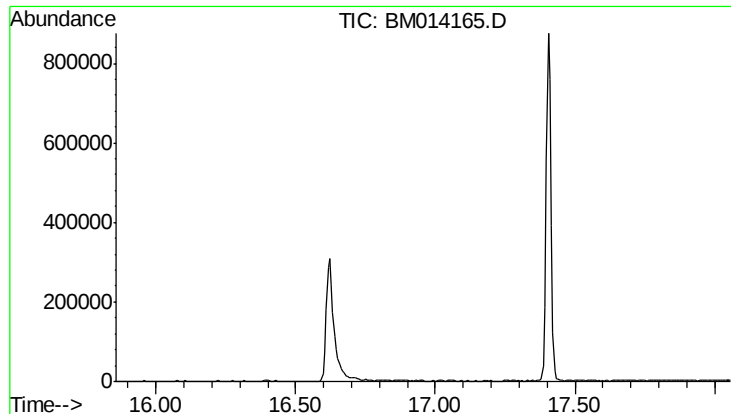

#63
 Phenanthrene-d10
 Concen: 0.00 ng
 Expected RT: 16.96 min
 Lab File: BM014165.D
 Acq: 07 Feb 2018 17:43


Instrument :
 BNA_M
 ClientSampleId :
 DFTPP


Tgt Ion	Exp Ratio
188	100
94	10.9
80	11.6

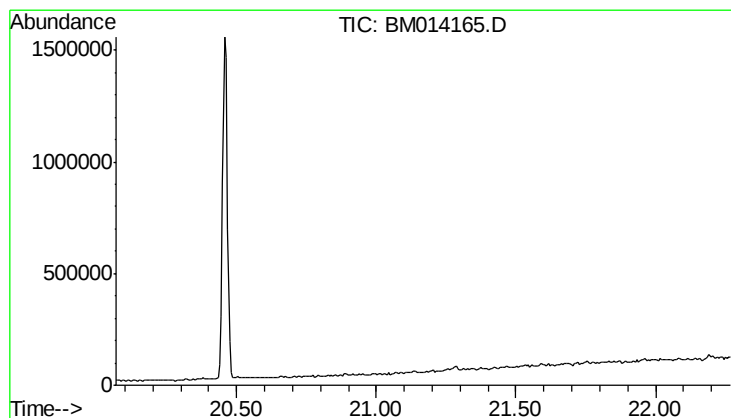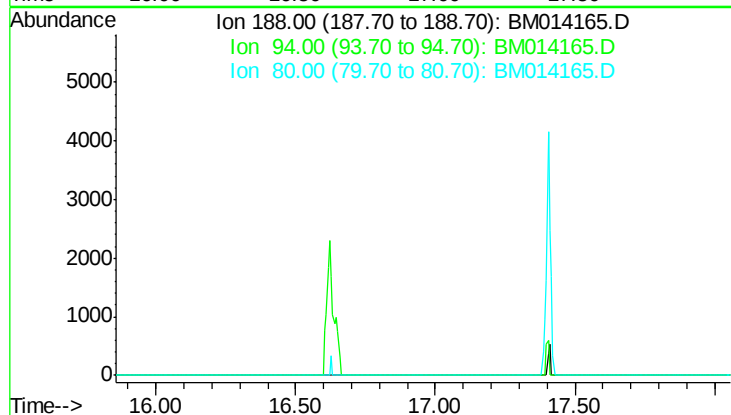

#75
 Chrysene-d12
 Concen: 0.00 ng
 Expected RT: 21.17 min
 Lab File: BM014165.D
 Acq: 07 Feb 2018 17:43

Tgt Ion	Exp Ratio
240	100
120	10.2
236	25.0


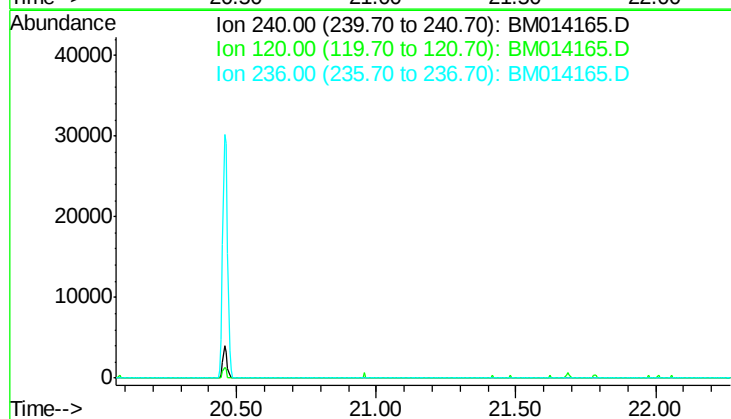


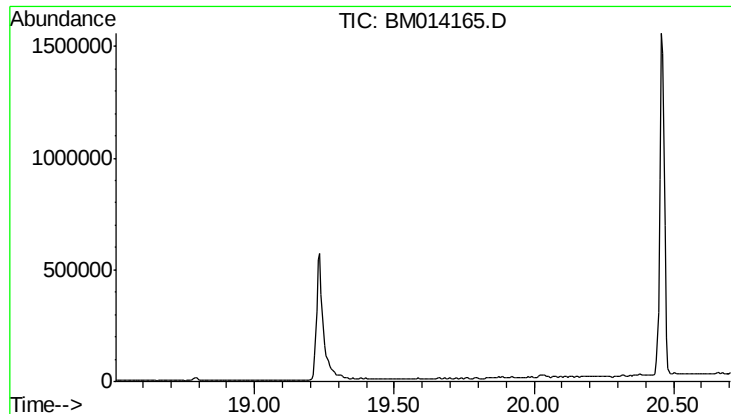

#78
 Terphenyl-d14
 Concen: 0.00 ng
 Expected RT: 19.60 min
 Lab File: BM014165.D
 Acq: 07 Feb 2018 17:43

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Tgt Ion	Exp Ratio
244	100
212	6.1
122	7.8

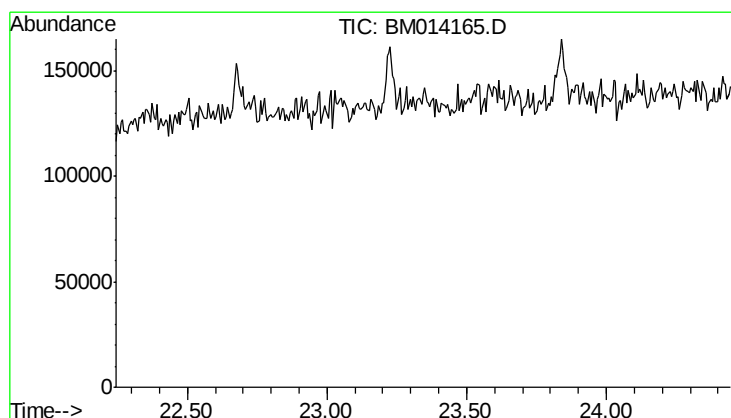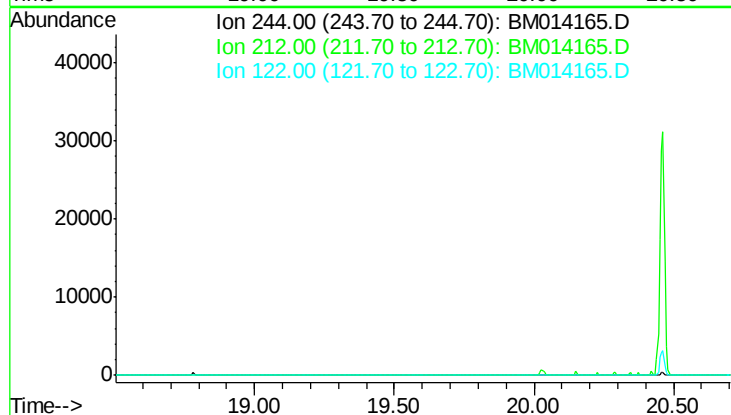

#86
 Perylene-d12
 Concen: 0.00 ng
 Expected RT: 23.34 min
 Lab File: BM014165.D
 Acq: 07 Feb 2018 17:43

Tgt Ion	Exp Ratio
264	100
260	23.2
265	21.6

