


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020718\
 Data File : BM014165.D
 Acq On : 07 Feb 2018 17:43
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM020718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 07 17:16:49 2018

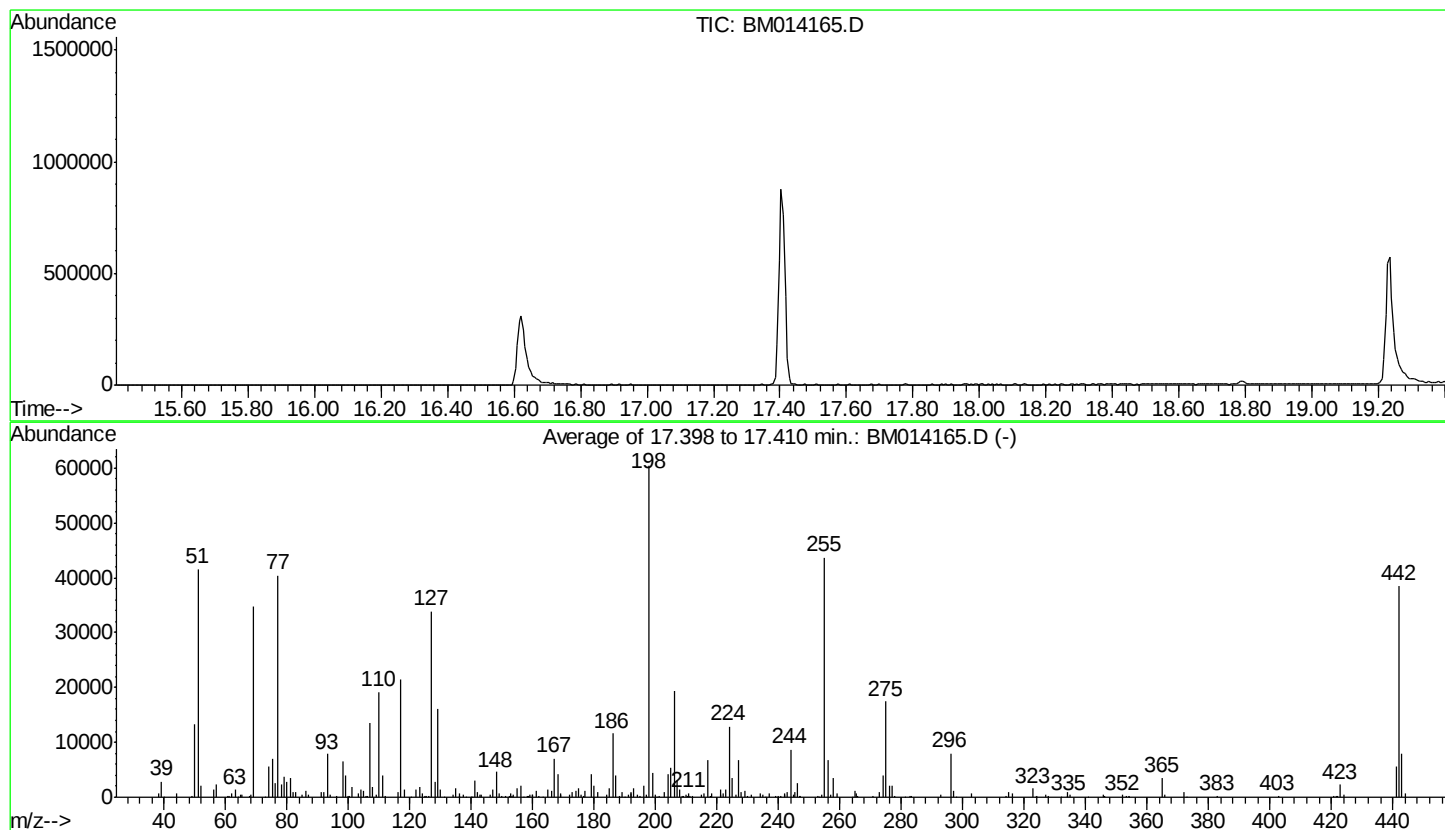

AutoFind: Scans 2450, 2451, 2452; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	68.8	41557	PASS
68	69	0.00	2	1.2	406	PASS
69	198	0.00	100	57.7	34861	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.0	33866	PASS
197	198	0.00	2	0.7	393	PASS
198	198	100	100	100.0	60445	PASS
199	198	5	9	7.4	4473	PASS
275	198	10	60	28.9	17485	PASS
365	198	1	100	5.9	3554	PASS
441	443	0.01	100	70.5	5673	PASS
442	198	50	100	63.9	38605	PASS
443	442	15	24	20.9	8050	PASS