

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020816\
 Data File : BM004196.D
 Acq On : 08 Feb 2016 12:47
 Operator : SJ/IZ
 Sample : PB88221BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK21

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.117	3	5	10	rVB	2912	3447	0.34%	0.049%
2	6.834	632	637	648	rBB	73903	113528	11.20%	1.599%
3	6.993	658	664	673	rBB	62857	96351	9.51%	1.357%
4	7.187	692	697	706	rBB	77631	121652	12.00%	1.714%
5	7.657	771	777	784	rBB	53195	82500	8.14%	1.162%
6	8.369	893	898	908	rBB	107010	163579	16.14%	2.305%
7	8.816	968	974	983	rBB	80167	128203	12.65%	1.806%
8	9.534	1091	1096	1104	rBB	64223	98934	9.76%	1.394%
9	10.075	1182	1188	1200	rBB	102387	167795	16.55%	2.364%
10	10.446	1244	1251	1258	rBB	96009	156923	15.48%	2.211%
11	10.587	1269	1275	1292	rBV	116686	195241	19.26%	2.751%
12	12.045	1521	1523	1526	rBB2	961	1140	0.11%	0.016%
13	13.728	1803	1809	1818	rBB	255220	345288	34.07%	4.865%
14	14.004	1850	1856	1870	rBB	273835	405782	40.04%	5.717%
15	14.316	1904	1909	1916	rBB2	173643	251807	24.84%	3.548%
16	14.539	1942	1947	1962	rBB	62355	100474	9.91%	1.416%
17	15.316	2073	2079	2086	rBB	381496	548722	54.14%	7.731%
18	15.451	2097	2102	2109	rBB	89752	113633	11.21%	1.601%
19	15.551	2117	2119	2123	rBB	2269	2290	0.23%	0.032%
20	17.069	2371	2377	2384	rBB2	260035	353467	34.87%	4.980%
21	17.169	2388	2394	2407	rVV	490812	678001	66.89%	9.552%
22	19.110	2721	2724	2728	rBB	3587	4059	0.40%	0.057%
23	19.363	2763	2767	2772	rBV	3038	3100	0.31%	0.044%
24	19.474	2781	2786	2797	rBV	631822	870497	85.89%	12.264%
25	21.280	3088	3093	3103	rBV	433290	523082	51.61%	7.370%
26	21.821	3183	3185	3189	rBV2	1020	1363	0.13%	0.019%
27	22.780	3344	3348	3352	rBV2	4410	6668	0.66%	0.094%
28	23.374	3442	3449	3462	rBV	554182	1013561	100.00%	14.280%
29	23.515	3466	3473	3490	rVB2	290857	542513	53.53%	7.643%
30	24.021	3555	3559	3564	rVB4	2493	4171	0.41%	0.059%


Sum of corrected areas: 7097771

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020816\
Data File : BM004196.D
Acq On : 08 Feb 2016 12:47
Operator : SJ/IZ
Sample : PB88221BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK21

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

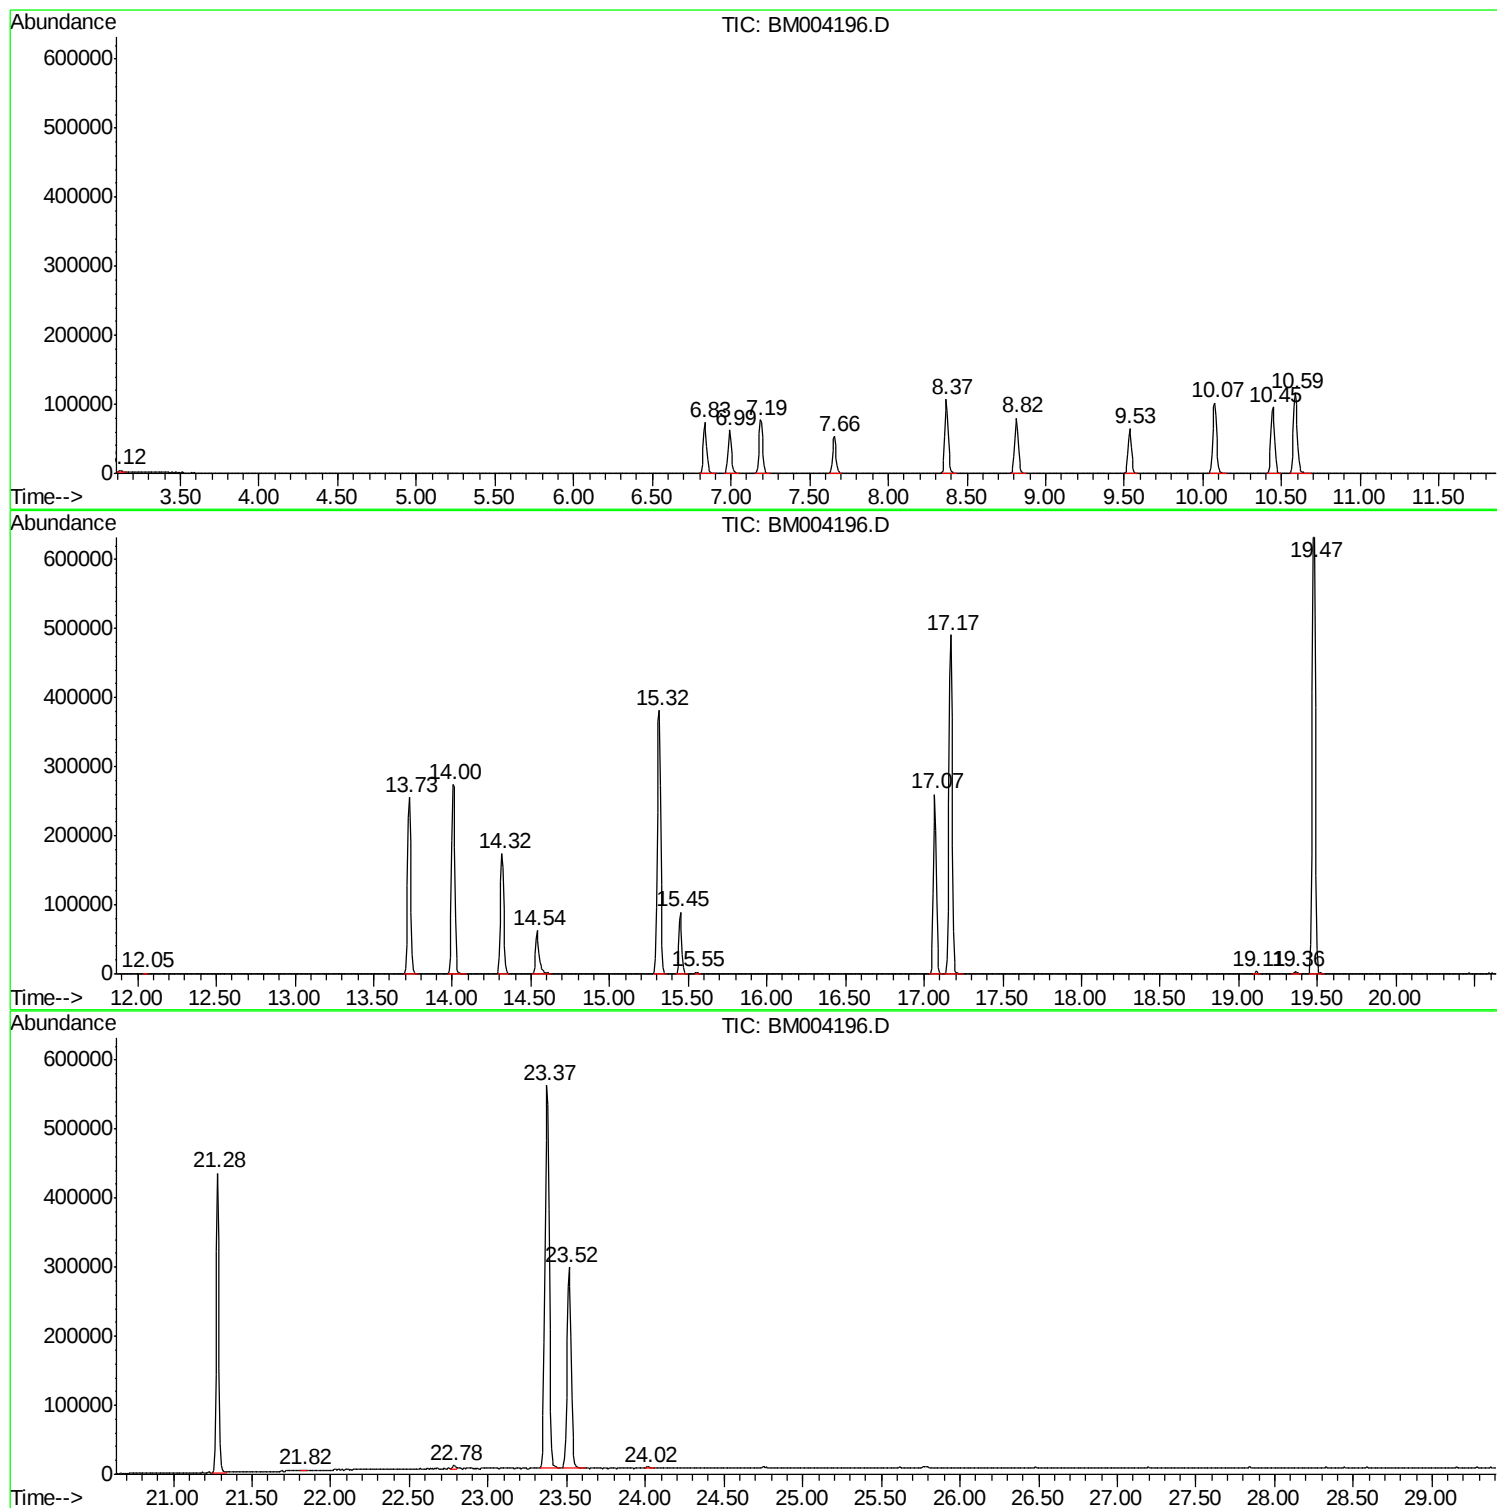

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020816\
Data File : BM004196.D
Acq On : 08 Feb 2016 12:47
Operator : SJ/IZ
Sample : PB88221BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK21

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020816\
Data File : BM004196.D
Acq On : 08 Feb 2016 12:47
Operator : SJ/IZ
Sample : PB88221BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK21

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc