

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020816\
 Data File : BM004211.D
 Acq On : 08 Feb 2016 22:22
 Operator : SJ/IZ
 Sample : H1340-11DL 25X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04K1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.640	90	94	98	rBB	2645	2922	0.25%	0.040%
2	6.840	635	638	643	rBB	1821	2817	0.24%	0.038%
3	6.998	661	665	668	rBB	2458	3362	0.29%	0.046%
4	7.192	695	698	702	rBB	2552	3239	0.28%	0.044%
5	7.657	771	777	784	rBB	89796	137776	11.83%	1.875%
6	8.822	971	975	979	rBB	2240	3297	0.28%	0.045%
7	10.086	1186	1190	1195	rBB	2336	3310	0.28%	0.045%
8	10.445	1244	1251	1257	rBV	145418	241997	20.77%	3.293%
9	13.721	1804	1808	1813	rBB	8489	10716	0.92%	0.146%
10	13.768	1813	1816	1821	rBB	3973	5275	0.45%	0.072%
11	14.010	1852	1857	1864	rBB	10133	14509	1.25%	0.197%
12	14.316	1903	1909	1916	rBV2	238472	358184	30.74%	4.875%
13	14.380	1916	1920	1924	rVB	17087	23108	1.98%	0.314%
14	14.715	1974	1977	1981	rBB	3040	3857	0.33%	0.052%
15	15.310	2074	2078	2083	rBB	16987	22395	1.92%	0.305%
16	15.368	2084	2088	2092	rBB	10616	13233	1.14%	0.180%
17	15.810	2161	2163	2168	rBB	1460	2424	0.21%	0.033%
18	16.886	2342	2346	2350	rVB	4068	4948	0.42%	0.067%
19	17.068	2371	2377	2381	rBV	322993	456614	39.19%	6.214%
20	17.109	2381	2384	2389	rVV	138660	174636	14.99%	2.377%
21	17.162	2389	2393	2396	rVV	18652	25128	2.16%	0.342%
22	17.198	2396	2399	2405	rVB	28448	38614	3.31%	0.526%
23	17.474	2439	2446	2452	rBB2	11782	17232	1.48%	0.235%
24	17.945	2522	2526	2530	rBV	9899	13541	1.16%	0.184%
25	17.992	2530	2534	2539	rVB	15871	20384	1.75%	0.277%
26	18.074	2544	2548	2551	rBB	5024	5812	0.50%	0.079%
27	18.139	2554	2559	2563	rBV3	23260	38000	3.26%	0.517%
28	18.174	2563	2565	2569	rVB	7537	8498	0.73%	0.116%
29	18.451	2608	2612	2616	rBV	7733	9792	0.84%	0.133%
30	18.498	2616	2620	2625	rVB2	4851	6681	0.57%	0.091%
31	18.698	2650	2654	2657	rBV2	2394	3016	0.26%	0.041%
32	18.751	2659	2663	2666	rVV	2563	2545	0.22%	0.035%
33	18.868	2678	2683	2688	rBV	4101	6519	0.56%	0.089%
34	18.933	2688	2694	2698	rVV2	3220	5775	0.50%	0.079%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020816\
 Data File : BM004211.D
 Acq On : 08 Feb 2016 22:22
 Operator : SJ/IZ
 Sample : H1340-11DL 25X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04K1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
 Title : SVOA CALIBRATION

35	19.015	2704	2708	2714	rVB2	4010	6004	0.52%	0.082%
36	19.139	2723	2729	2737	rVB	282323	382539	32.83%	5.206%
37	19.239	2742	2746	2750	rBV	2292	2591	0.22%	0.035%
38	19.380	2763	2770	2778	rVB2	6019	10967	0.94%	0.149%
39	19.474	2780	2786	2787	rBV3	78843	100059	8.59%	1.362%
40	19.503	2787	2791	2799	rVB	230040	327580	28.12%	4.458%
41	19.574	2799	2803	2807	rBV2	9196	11025	0.95%	0.150%
42	19.686	2818	2822	2826	rVB	12536	15616	1.34%	0.213%
43	19.745	2828	2832	2838	rBV	12081	15559	1.34%	0.212%
44	19.827	2841	2846	2853	rBV4	10744	26267	2.25%	0.357%
45	19.886	2853	2856	2861	rVB	4514	5299	0.45%	0.072%
46	19.968	2865	2870	2871	rBV3	8311	12595	1.08%	0.171%
47	20.003	2871	2876	2881	rVB3	36912	53530	4.59%	0.729%
48	20.103	2888	2893	2897	rBV	32680	40236	3.45%	0.548%
49	20.156	2897	2902	2906	rVV2	17809	31000	2.66%	0.422%
50	20.197	2906	2909	2913	rVB	15501	17608	1.51%	0.240%
51	20.239	2913	2916	2921	rVB	4486	6116	0.52%	0.083%
52	20.303	2922	2927	2930	rBV	8978	11219	0.96%	0.153%
53	20.345	2930	2934	2938	rBV2	9400	13076	1.12%	0.178%
54	20.562	2967	2971	2974	rBV3	2161	3422	0.29%	0.047%
55	20.603	2974	2978	2979	rVV2	3787	4755	0.41%	0.065%
56	20.639	2979	2984	2987	rVV2	7180	12700	1.09%	0.173%
57	20.715	2993	2997	3000	rVV3	5532	8725	0.75%	0.119%
58	20.756	3000	3004	3010	rVV	17494	24540	2.11%	0.334%
59	20.815	3010	3014	3016	rVV3	1719	2799	0.24%	0.038%
60	20.845	3016	3019	3022	rVV	2110	3225	0.28%	0.044%
61	20.921	3025	3032	3035	rVV3	23826	36082	3.10%	0.491%
62	20.956	3035	3038	3042	rVV3	23850	36869	3.16%	0.502%
63	21.003	3042	3046	3050	rVV2	22040	41417	3.55%	0.564%
64	21.050	3050	3054	3061	rVB2	17639	26372	2.26%	0.359%
65	21.186	3072	3077	3082	rVB	1048915	1165089	100.00%	15.856%
66	21.274	3082	3092	3096	rVV2	550654	913894	78.44%	12.438%
67	21.309	3096	3098	3109	rVB	168942	204654	17.57%	2.785%
68	21.397	3109	3113	3115	rBV3	2929	4180	0.36%	0.057%
69	21.433	3115	3119	3125	rBV2	35542	56979	4.89%	0.775%
70	21.492	3125	3129	3132	rBV3	11414	14605	1.25%	0.199%
71	21.539	3133	3137	3141	rVV3	17916	26791	2.30%	0.365%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020816\
Data File : BM004211.D
Acq On : 08 Feb 2016 22:22
Operator : SJ/IZ
Sample : H1340-11DL 25X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04K1DL

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
Title : SVOA CALIBRATION

72	21.592	3141	3146	3151	rVB2	26563	42636	3.66%	0.580%
73	21.639	3151	3154	3157	rBV3	3392	4266	0.37%	0.058%
74	21.721	3165	3168	3172	rBV	3542	6768	0.58%	0.092%
75	21.768	3172	3176	3179	rVV3	9004	15198	1.30%	0.207%
76	21.827	3179	3186	3189	rVV	25975	46687	4.01%	0.635%
77	21.874	3192	3194	3200	rVV2	14279	19066	1.64%	0.259%
78	21.939	3202	3205	3208	rVV3	5931	9230	0.79%	0.126%
79	21.980	3208	3212	3215	rVV2	11164	17634	1.51%	0.240%
80	22.021	3215	3219	3222	rVV2	14397	22914	1.97%	0.312%
81	22.056	3222	3225	3230	rVV4	17341	25256	2.17%	0.344%
82	22.115	3231	3235	3240	rVB3	9651	15734	1.35%	0.214%
83	22.309	3263	3268	3282	rBV8	17712	39780	3.41%	0.541%
84	22.421	3285	3287	3288	rBV2	3194	2705	0.23%	0.037%
85	22.591	3311	3316	3323	rBV5	10663	23714	2.04%	0.323%
86	22.674	3328	3330	3335	rVB4	4406	5407	0.46%	0.074%
87	22.756	3340	3344	3348	rBV	6638	10024	0.86%	0.136%
88	22.838	3349	3358	3363	rBV	135307	324479	27.85%	4.416%
89	23.009	3382	3387	3392	rBV	22345	35393	3.04%	0.482%
90	23.144	3406	3410	3411	rBV3	6555	9319	0.80%	0.127%
91	23.315	3433	3439	3444	rBV	71179	130024	11.16%	1.770%
92	23.368	3444	3448	3451	rVV2	35898	64472	5.53%	0.877%
93	23.409	3451	3455	3462	rVB	104796	182226	15.64%	2.480%
94	23.509	3464	3472	3478	rBV	303046	563935	48.40%	7.675%
95	23.556	3478	3480	3488	rVB2	32036	48895	4.20%	0.665%
96	24.009	3550	3557	3563	rBV2	20458	42363	3.64%	0.577%
97	24.744	3676	3682	3691	rVB2	19764	45464	3.90%	0.619%
98	25.603	3821	3828	3835	rVB4	12889	32962	2.83%	0.449%
99	25.756	3845	3854	3864	rVB	43600	124383	10.68%	1.693%
100	26.444	3964	3971	3982	rVB	23544	70816	6.08%	0.964%


Sum of corrected areas: 7347890

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020816\
Data File : BM004211.D
Acq On : 08 Feb 2016 22:22
Operator : SJ/IZ
Sample : H1340-11DL 25X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04K1DL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

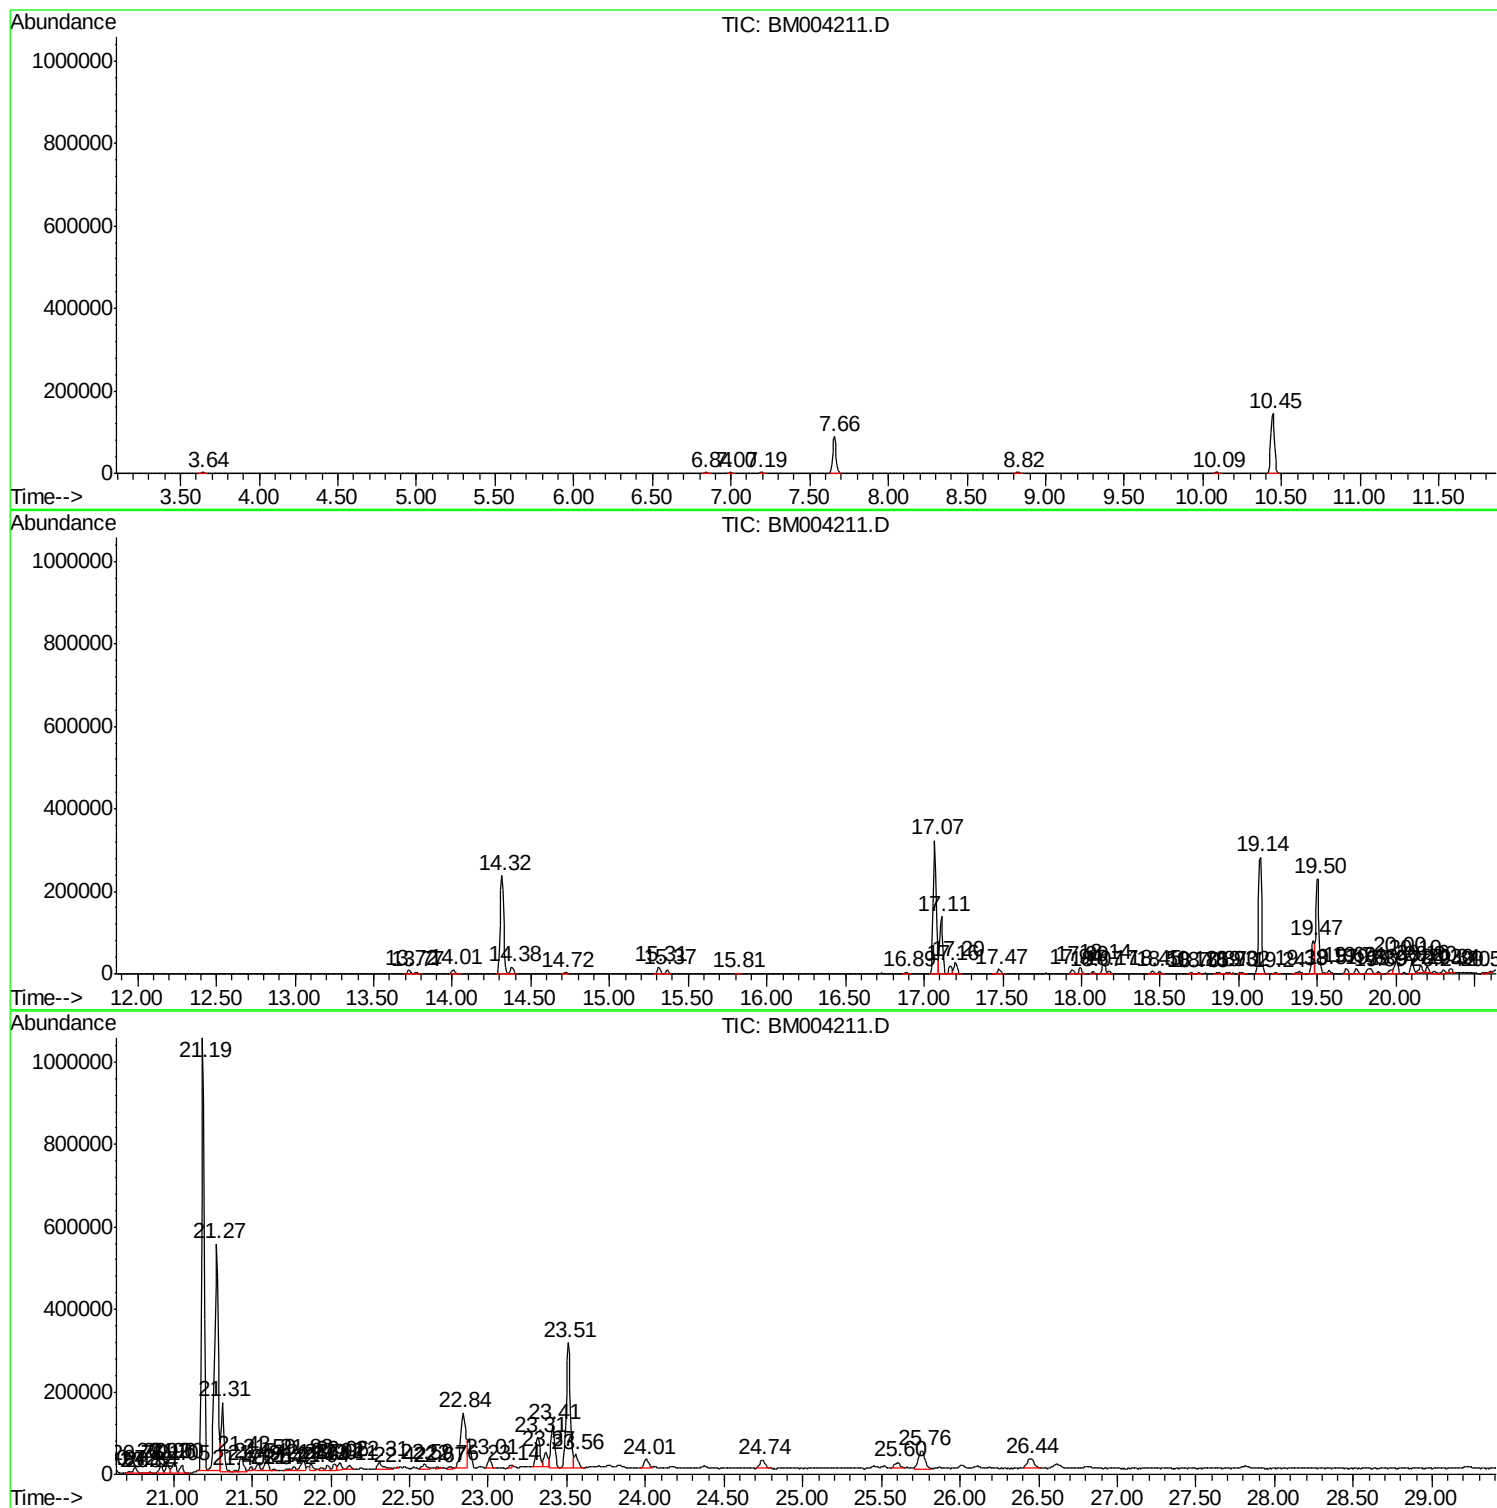

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020816\
Data File : BM004211.D
Acq On : 08 Feb 2016 22:22
Operator : SJ/IZ
Sample : H1340-11DL 25X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04K1DL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020816\
Data File : BM004211.D
Acq On : 08 Feb 2016 22:22
Operator : SJ/IZ
Sample : H1340-11DL 25X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04K1DL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc