


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020816\
 Data File : BM004194.D
 Acq On : 08 Feb 2016 10:07
 Operator : SJ/IZ
 Sample : DFTPP48
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP48

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
 Title : SVOA CALIBRATION
 Last Update : Tue Feb 09 01:37:43 2016

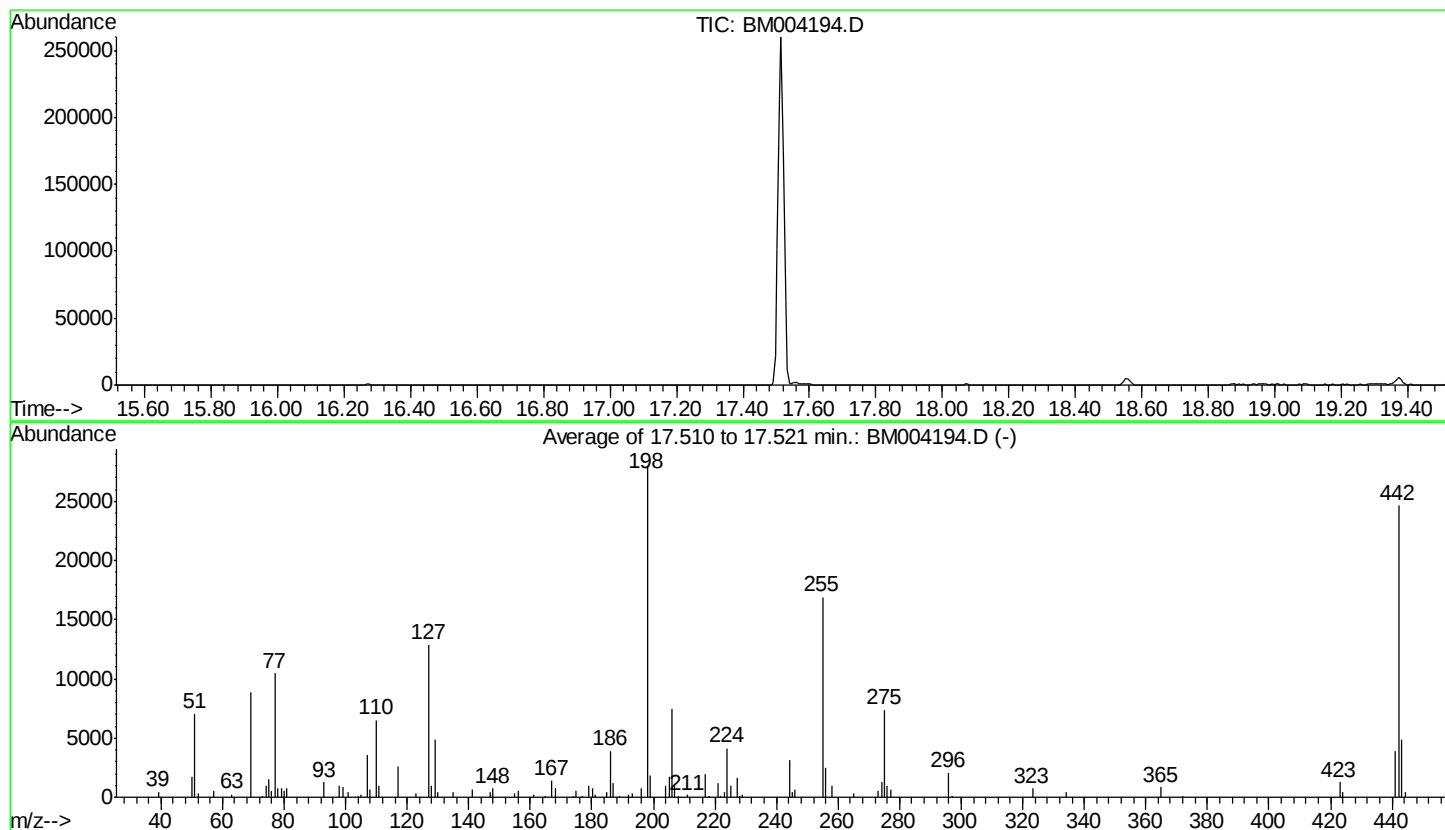

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.2	7059	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.5	8828	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.1	12923	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	28008	PASS
199	198	5	9	6.4	1793	PASS
275	198	10	60	26.4	7383	PASS
365	198	1	100	3.0	851	PASS
441	443	0.01	100	79.7	3874	PASS
442	198	50	100	87.8	24602	PASS
443	442	15	24	19.7	4858	PASS

m/z	Abundance
39.10	541.0
50.10	1975.0
51.10	8110.0
52.00	416.0
57.00	610.0
63.10	367.0
69.00	10010.0
73.00	311.0
74.00	1067.0
75.00	1593.0
76.00	557.0
77.10	11623.0
78.00	792.0
79.00	799.0
80.00	556.0
81.00	885.0
93.00	1426.0
98.00	1078.0
99.00	994.0
101.00	496.0
104.90	334.0
107.00	3761.0
108.00	652.0
110.00	7062.0
111.00	1182.0
117.00	2783.0
123.00	404.0
127.10	13979.0
128.10	1084.0
129.00	5188.0
130.00	499.0
135.00	458.0
141.00	646.0
147.00	457.0
148.00	726.0
155.00	358.0
156.10	568.0
161.10	337.0
164.90	324.0
167.10	1422.0
168.00	787.0
175.00	549.0
179.00	1053.0
180.00	757.0
181.00	346.0
185.00	508.0
186.10	3963.0
187.00	1209.0
192.00	370.0
193.00	379.0
196.00	850.0
198.00	28280.0
199.00	1867.0
204.10	977.0
205.10	1597.0
206.10	7388.0
207.00	1167.0
211.10	305.0
217.00	1962.0
221.10	1210.0
223.00	409.0
224.10	3942.0
225.10	979.0
227.00	1598.0
229.00	340.0
244.10	2928.0
245.00	408.0
246.00	530.0
255.10	15910.0
256.10	2333.0
258.00	849.0
265.00	301.0
273.00	447.0
274.00	1090.0
275.10	6639.0
276.10	958.0
277.00	559.0
296.00	1829.0
323.10	629.0
334.10	397.0
365.10	671.0
423.10	992.0
424.20	358.0
441.10	3037.0
442.10	19248.0
443.20	3775.0
444.10	391.0

Instrument :
BNA_M
ClientSampleId :
DFTPP48

m/z	Abundance
39.10	570.0
50.10	1867.0
51.10	8308.0
52.00	411.0
57.00	582.0
63.10	381.0
69.00	10311.0
74.10	1124.0
75.00	1938.0
76.00	578.0
77.10	12301.0
78.10	849.0
79.00	906.0
80.00	616.0
81.00	979.0
93.00	1457.0
98.00	1188.0
99.00	918.0
101.00	474.0
104.00	356.0
105.00	354.0
107.00	4223.0
108.00	703.0
110.00	7652.0
111.00	1113.0
117.00	3128.0
123.00	455.0
127.10	15332.0
128.00	1138.0
129.00	5898.0
130.00	512.0
135.10	507.0
141.00	793.0
147.00	471.0
148.00	837.0
155.00	436.0
156.00	650.0
161.00	367.0
167.00	1571.0
168.00	848.0
174.00	320.0
175.00	604.0
177.00	314.0
179.00	1146.0
180.10	882.0
181.00	392.0
185.00	605.0
186.10	4633.0
187.00	1380.0
189.00	300.0
192.00	334.0
193.00	457.0
196.00	961.0
198.00	33080.0
199.00	2143.0
204.00	1126.0
205.10	2074.0
206.10	9141.0
207.10	1268.0
208.00	304.0
211.00	317.0
217.00	2372.0
218.10	302.0
221.10	1272.0
221.80	373.0
223.00	508.0
224.10	4936.0
225.10	1191.0
227.10	1978.0
228.00	314.0
229.00	410.0
244.10	3897.0
245.10	487.0
246.00	771.0
255.10	20416.0
256.10	3037.0
258.00	1170.0
265.00	418.0
273.00	633.0
274.10	1589.0
275.10	8957.0
276.00	1214.0
277.00	804.0
296.00	2527.0
297.00	360.0
323.10	832.0
334.10	572.0
365.10	1017.0
372.10	412.0
423.10	1534.0
424.10	465.0

Instrument :
BNA_M
ClientSampleId :
DFTPP48

441.10	4585.0
442.10	29368.0
443.10	6049.0
444.10	461.0

Instrument :
BNA_M
ClientSampleId :
DFTPP48

m/z	Abundance
39.00	350.0
50.10	1250.0
51.10	4760.0
57.00	347.0
69.00	6163.0
74.00	681.0
75.00	1069.0
76.00	374.0
77.10	7443.0
78.10	509.0
79.00	515.0
80.10	376.0
81.00	534.0
93.00	861.0
98.00	670.0
99.00	596.0
101.00	333.0
107.00	2583.0
108.00	443.0
110.00	4896.0
111.00	662.0
117.00	2026.0
127.10	9458.0
128.00	762.0
129.00	3579.0
130.00	300.0
135.00	322.0
141.00	546.0
147.00	313.0
148.00	596.0
155.00	312.0
156.00	445.0
167.00	1099.0
168.00	590.0
175.00	519.0
179.00	773.0
180.10	607.0
185.00	316.0
186.10	3121.0
187.00	844.0
196.00	602.0
198.00	22664.0
199.00	1371.0
204.10	897.0
205.10	1421.0
206.10	5999.0
207.10	813.0
217.00	1562.0
221.10	943.0
223.00	372.0
224.10	3505.0
225.10	834.0
227.00	1335.0
244.10	2649.0
245.00	375.0
246.00	517.0
255.10	14308.0
256.10	1991.0
258.00	794.0
265.00	320.0
273.10	419.0
274.10	1146.0
275.10	6554.0
276.10	865.0
277.00	487.0
296.10	1921.0
323.10	708.0
334.10	419.0
365.10	866.0
423.10	1344.0
424.10	361.0
441.10	4000.0
442.10	25192.0
443.10	4751.0
444.20	448.0

Instrument :
BNA_M
ClientSampleId :
DFTPP48

m/z Abundance

Instrument :
BNA_M
ClientSampleId :
DFTPP48