
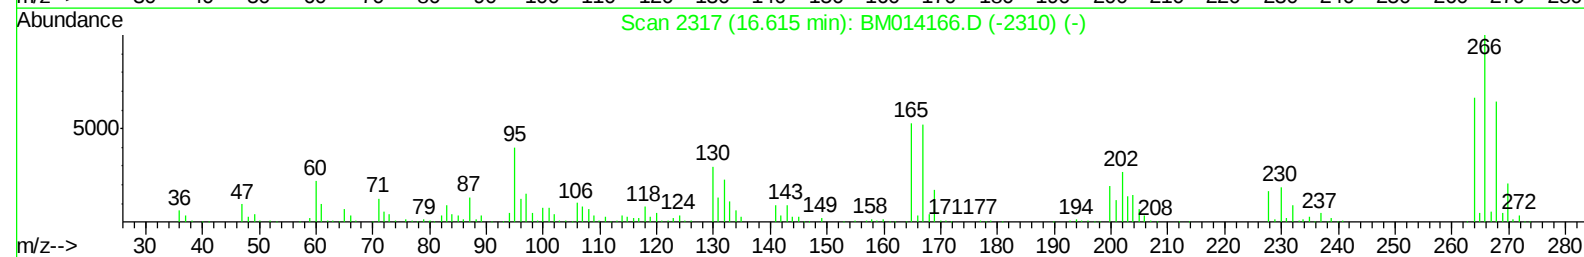
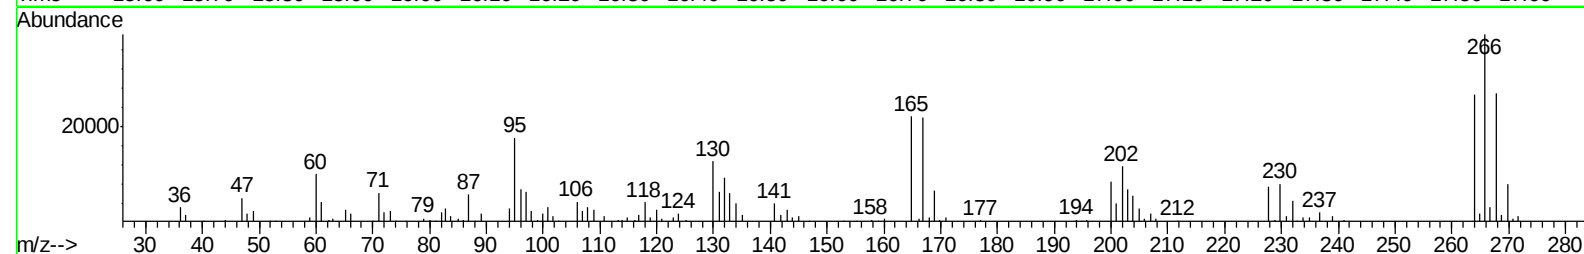


Data Path : Z:\HPCHEM1\BNA M\DATA\BM020818\
Data File : BM014182.D
Acq On : 08 Feb 2018 07:50
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 06:04:06 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 07 17:16:49 2018
Response via : Initial Calibration

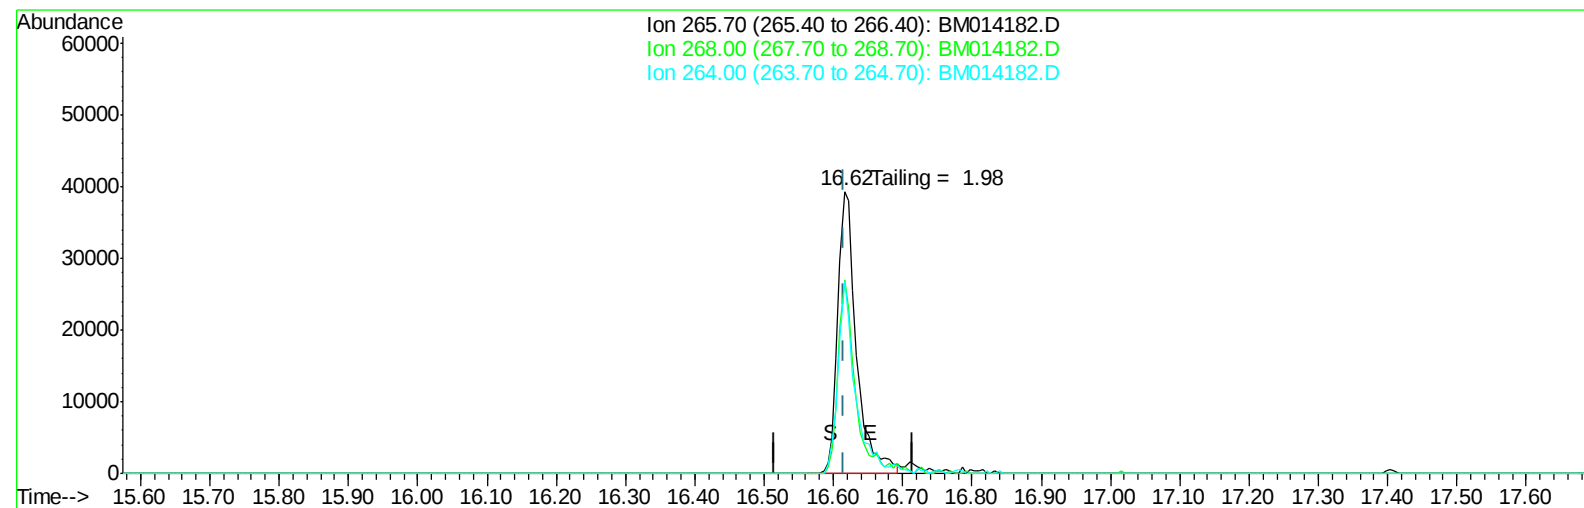

TIC: BM014182.D

(69) Pentachlorophenol (C)




16.616min (+0.001) 0.00ng

response 73407

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	68.48
264.00	61.20	68.25
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020818\
Data File : BM014182.D
Acq On : 08 Feb 2018 07:50
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 06:04:06 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 07 17:16:49 2018
Response via : Initial Calibration

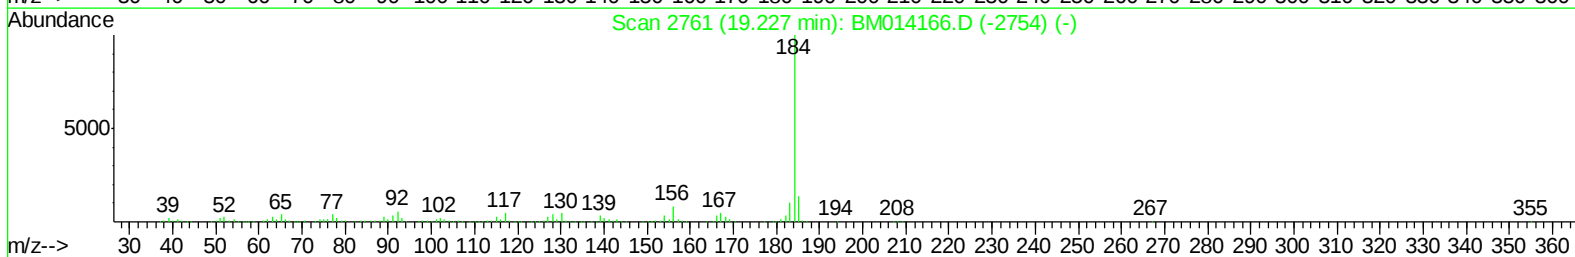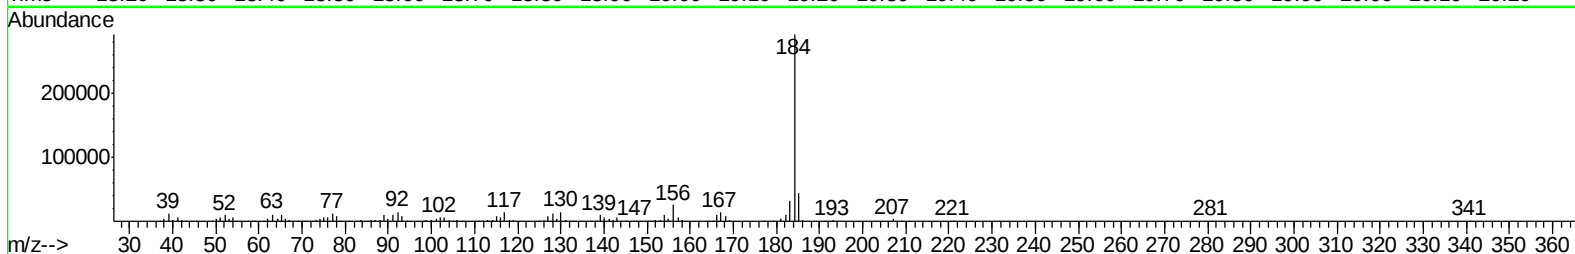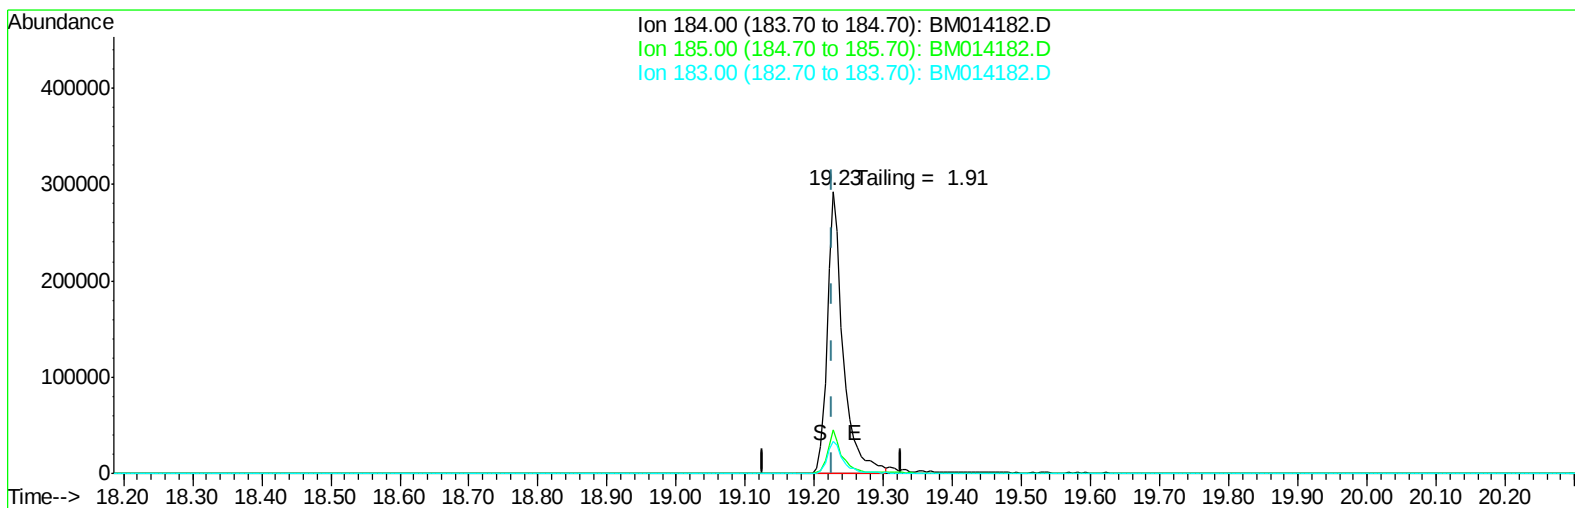

TIC: BM014182.D

(76) Benzidine

19.227min (+0.000) 0.00ng

response 464113

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	15.26
183.00	11.10	11.32
0.00	0.00	0.00