

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020818\
 Data File : BM014207.D
 Acq On : 08 Feb 2018 23:32
 Operator : SJ/JU
 Sample : PB106402BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB106402BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM020718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.163	364	370	386	rBV	2268093	3118626	57.89%	9.327%
2	6.734	630	637	651	rBV	2196890	3350469	62.19%	10.020%
3	7.081	688	696	708	rBV	2299251	3556499	66.01%	10.636%
4	7.540	768	774	784	rVB	378037	604933	11.23%	1.809%
5	7.851	820	827	839	rBV	1762794	2750736	51.06%	8.227%
6	8.698	964	971	990	rBV	1218891	2163147	40.15%	6.469%
7	10.310	1238	1245	1263	rBV	365603	742277	13.78%	2.220%
8	12.804	1662	1669	1686	rBV	3113714	4658689	86.47%	13.933%
9	14.198	1899	1906	1921	rBV2	555865	982769	18.24%	2.939%
10	15.698	2154	2161	2182	rBV	2192901	3397860	63.07%	10.162%
11	16.957	2369	2375	2389	rBV	640956	1056095	19.60%	3.158%
12	19.598	2818	2824	2838	rBV	4359240	5387561	100.00%	16.112%
13	21.162	3085	3090	3099	rBV	609828	883947	16.41%	2.644%
14	23.339	3454	3460	3468	rBV	391414	783774	14.55%	2.344%


Sum of corrected areas: 33437382

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020818\
Data File : BM014207.D
Acq On : 08 Feb 2018 23:32
Operator : SJ/JU
Sample : PB106402BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB106402BL

Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

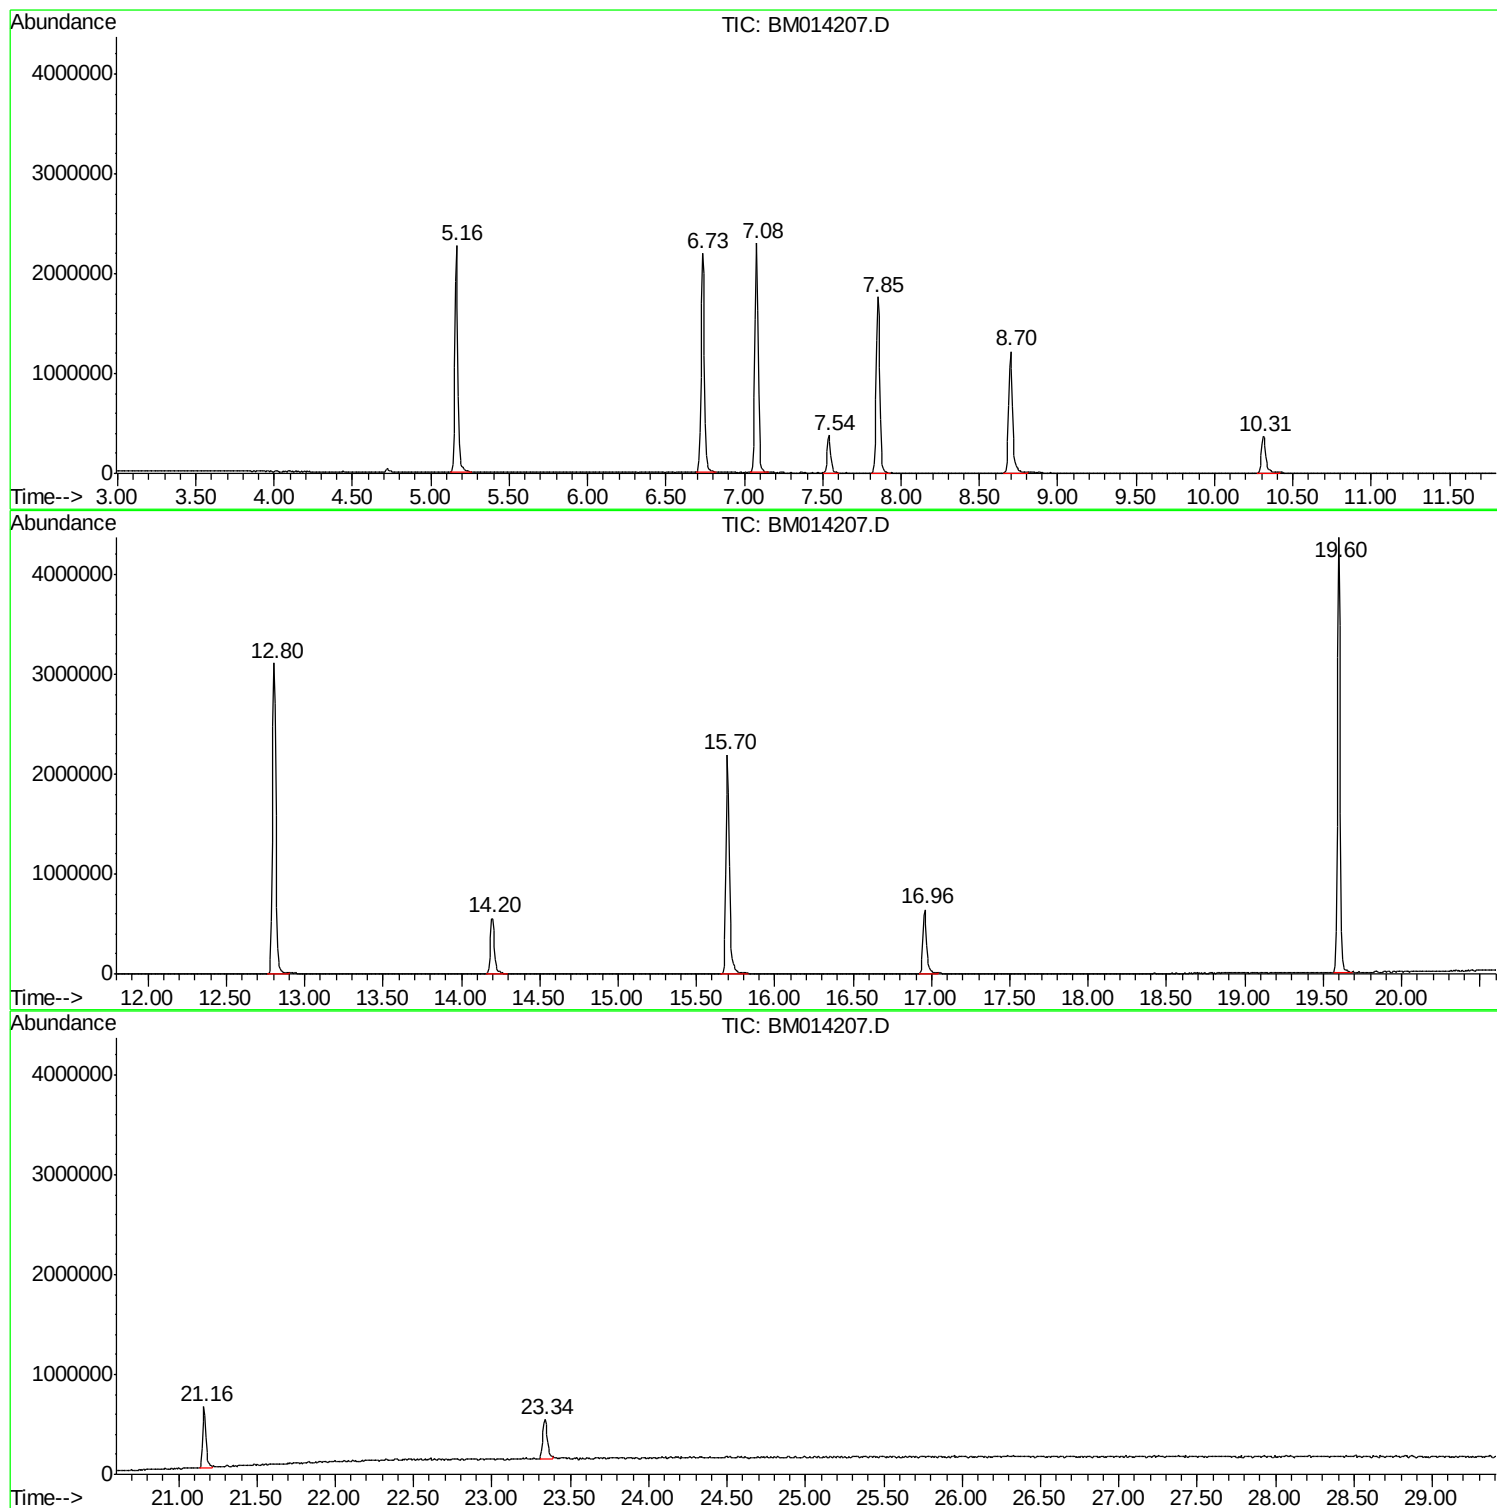

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020818\
Data File : BM014207.D
Acq On : 08 Feb 2018 23:32
Operator : SJ/JU
Sample : PB106402BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB106402BL










Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.08 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.08	117.58 ng	3556500	1,4-Dichlorobenzene-d4	7.54

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	14
2		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	14
3		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	14
4		1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	12
5		3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	10

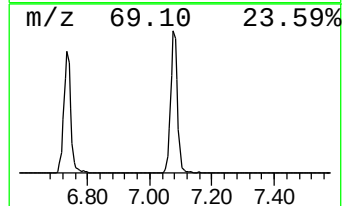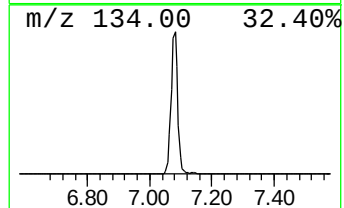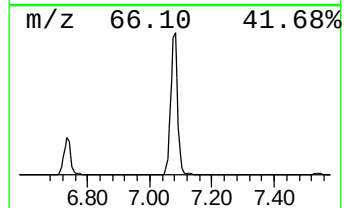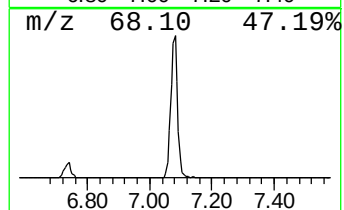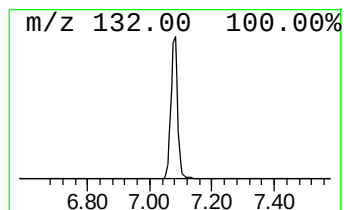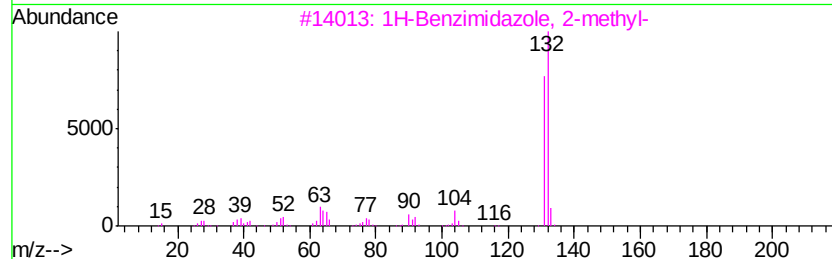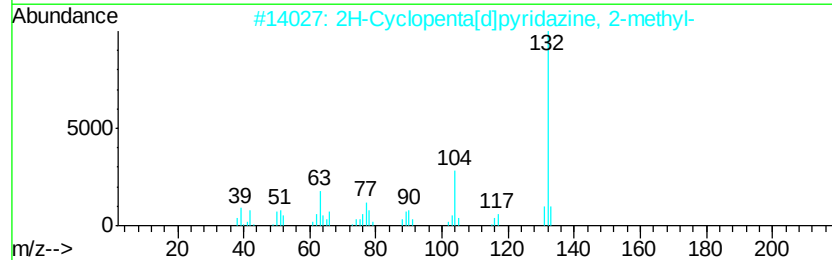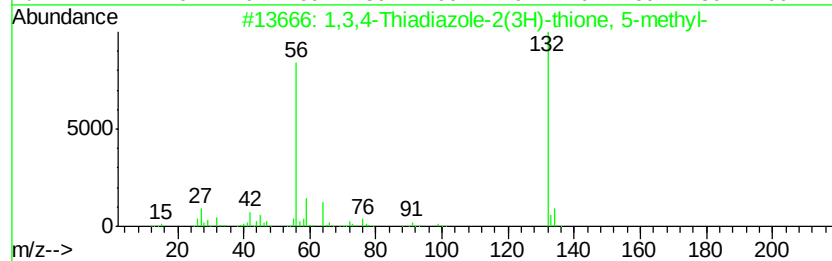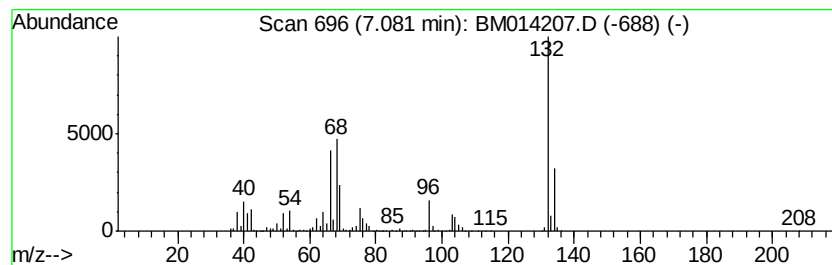

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020818\
Data File : BM014207.D
Acq On : 08 Feb 2018 23:32
Operator : SJ/JU
Sample : PB106402BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB106402BL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.08	7.08	117.6	ng	3556500	1	7.54	604933	20.0