


Data Path : Z:\HPCHEM1\BNA M\Data\BM020818\
 Data File : BM014190.D
 Acq On : 08 Feb 2018 13:23
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM020718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 07 17:16:49 2018

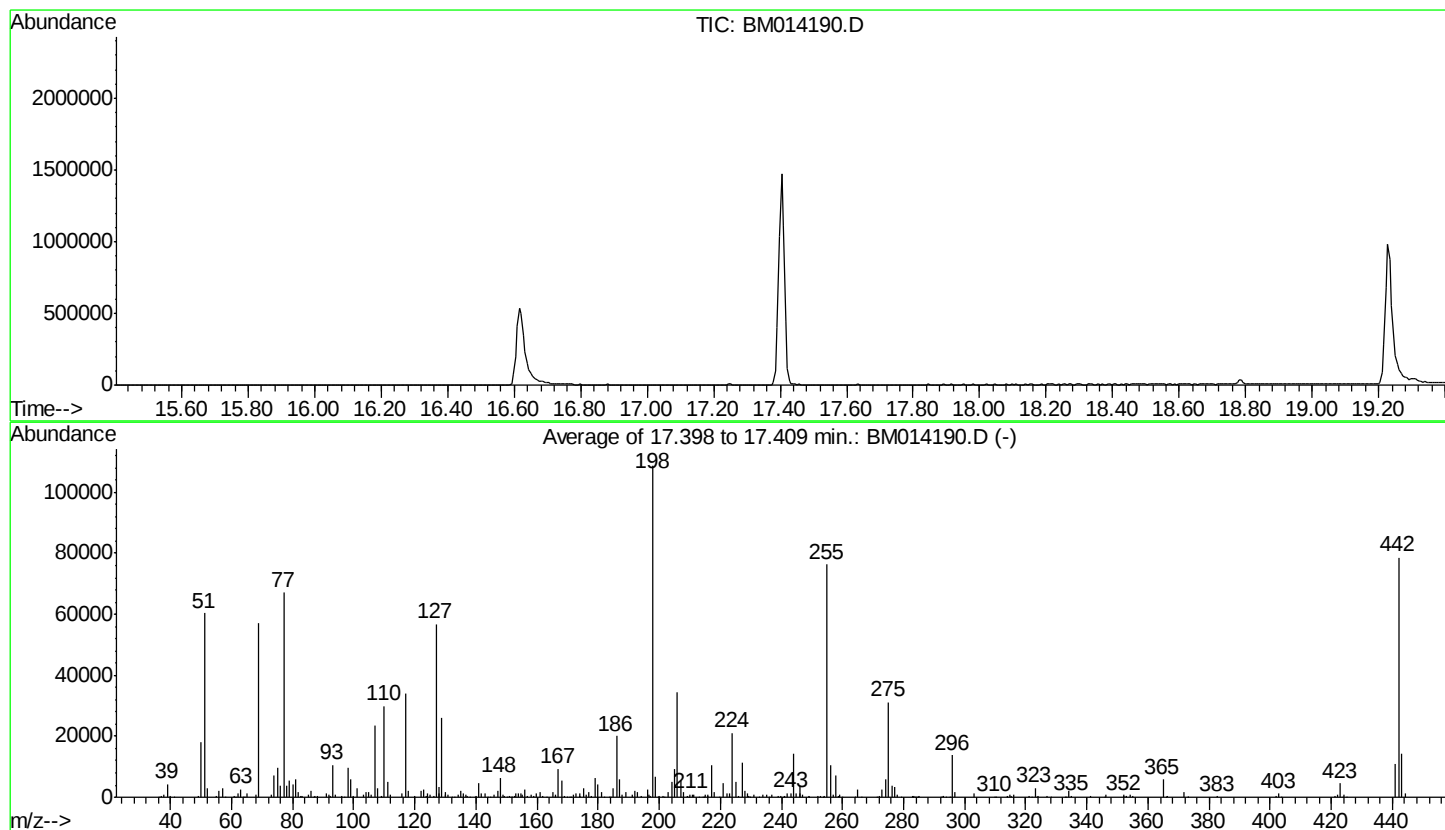

AutoFind: Scans 2450, 2451, 2452; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.4	60306	PASS
68	69	0.00	2	1.4	814	PASS
69	198	0.00	100	52.4	57032	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.3	56885	PASS
197	198	0.00	2	0.6	659	PASS
198	198	100	100	100.0	108760	PASS
199	198	5	9	6.1	6644	PASS
275	198	10	60	28.6	31072	PASS
365	198	1	100	5.4	5833	PASS
441	443	0.01	100	77.3	10958	PASS
442	198	50	100	72.3	78626	PASS
443	442	15	24	18.0	14173	PASS