
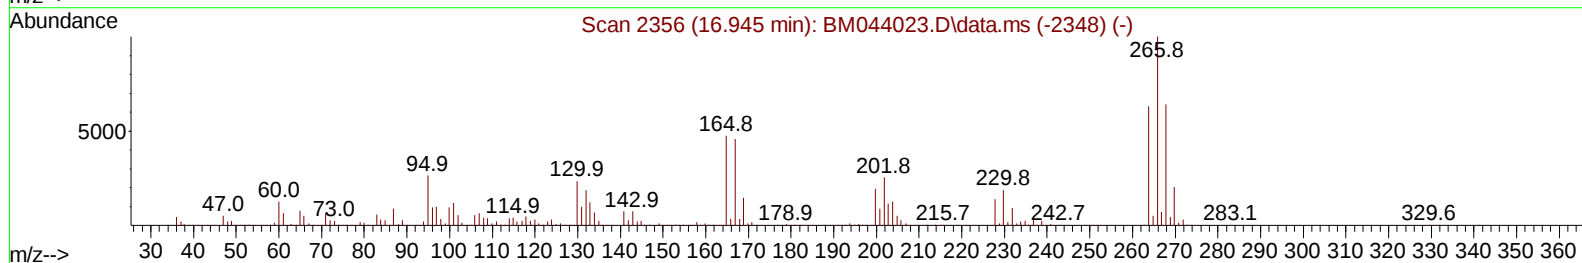
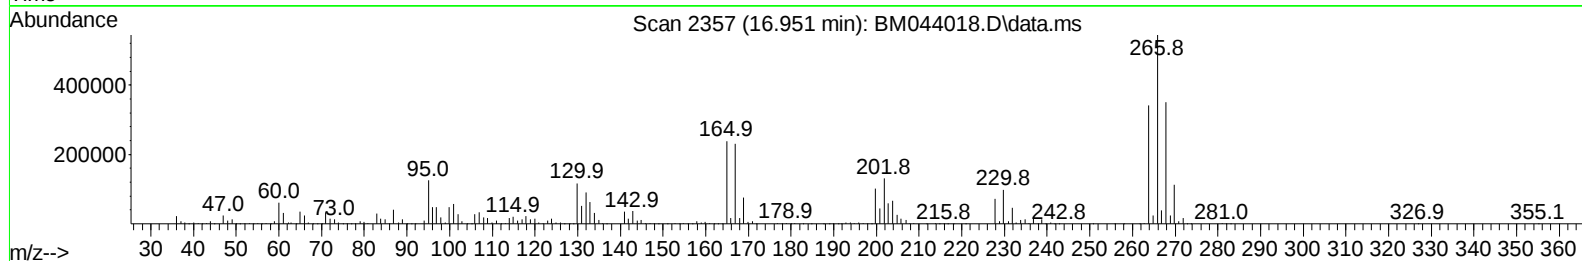


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020824\
Data File : BM044018.D
Acq On : 08 Feb 2024 12:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 02:49:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 02:42:01 2024
Response via : Initial Calibration

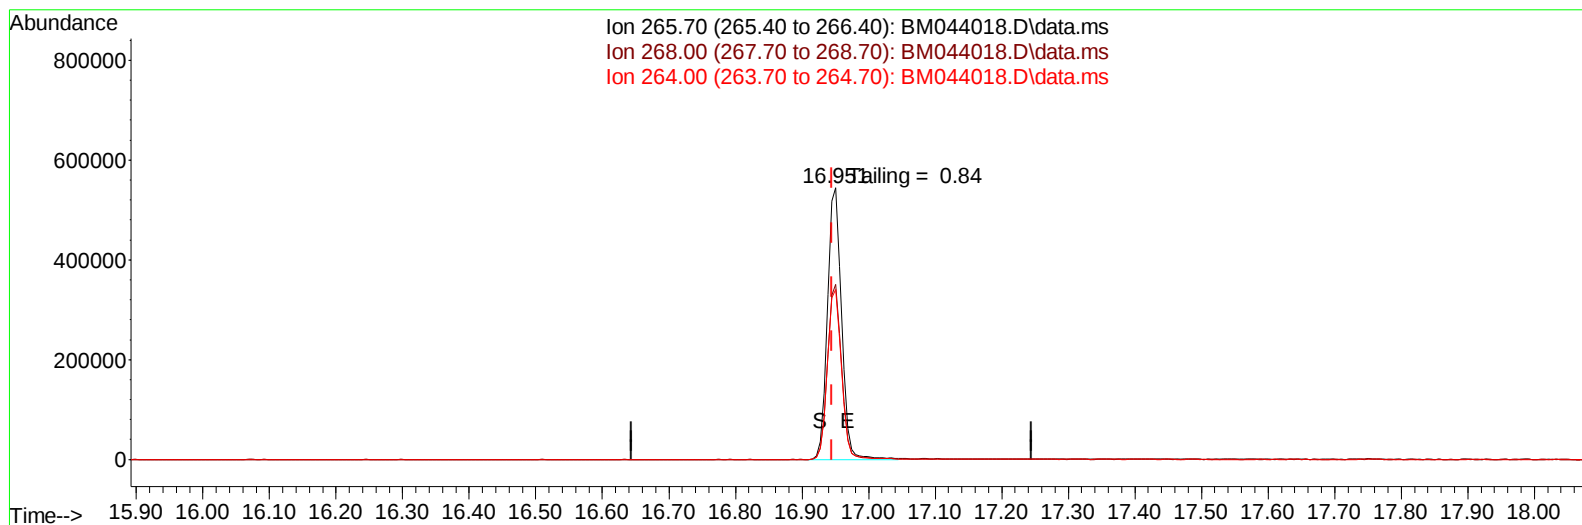

TIC: BM044018.D\data.ms

(70) Pentachlorophenol (C)




16.951min (+ 0.006) 0.00 ng

response 804760

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	64.51
264.00	63.10	62.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020824\
Data File : BM044018.D
Acq On : 08 Feb 2024 12:43
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 02:49:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 02:42:01 2024
Response via : Initial Calibration

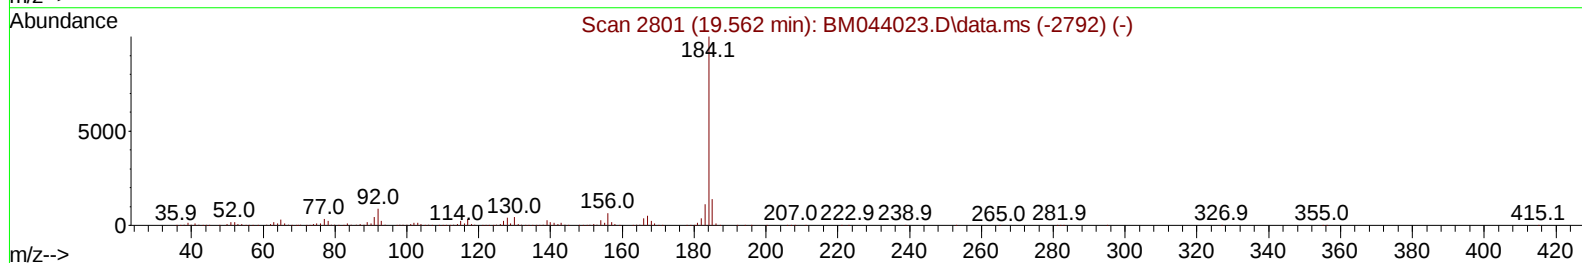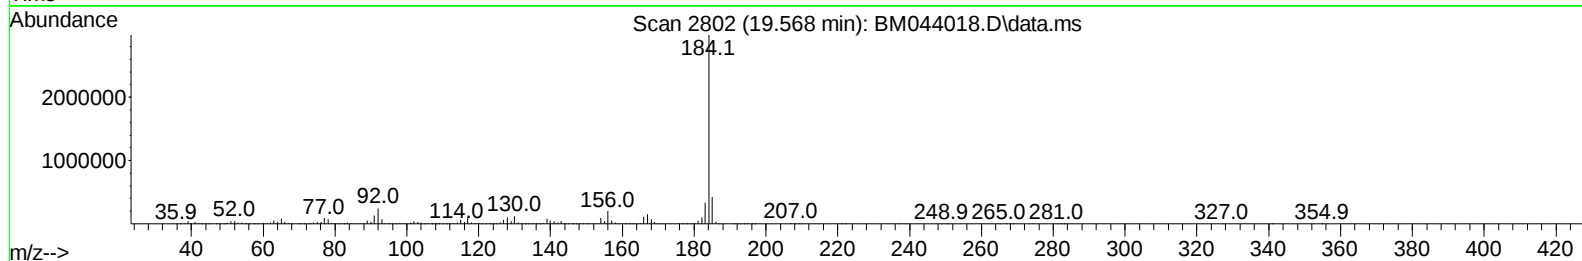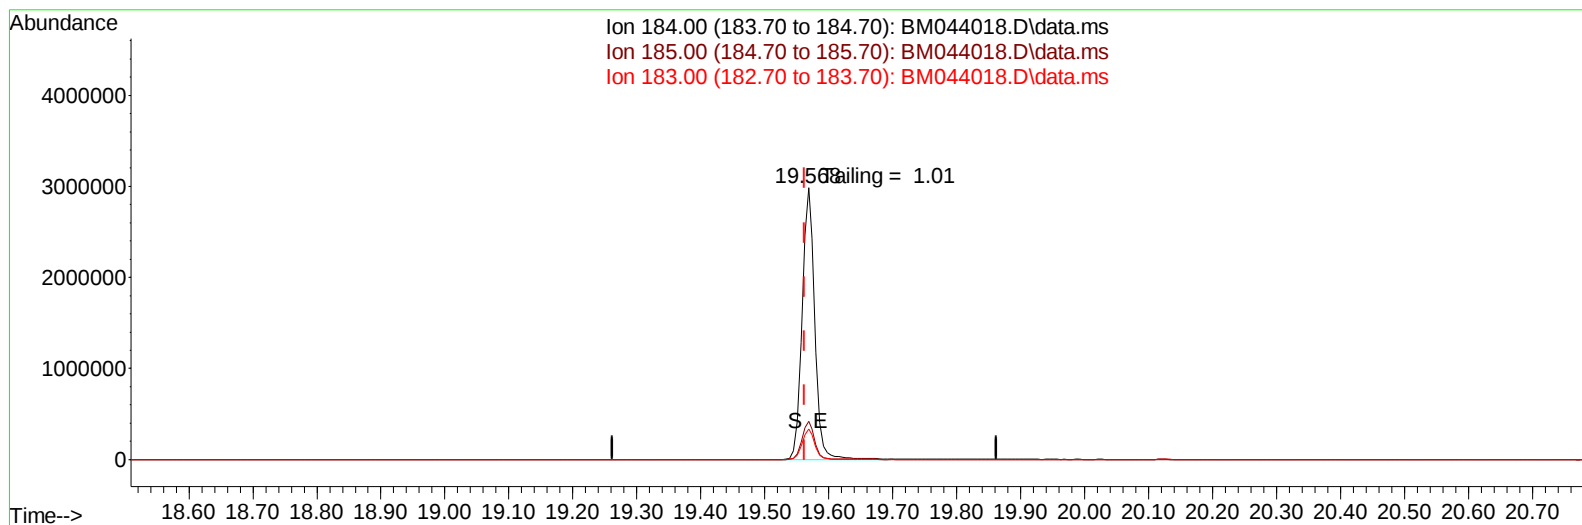

TIC: BM044018.D\data.ms

(77) Benzidine**19.568min (+ 0.006) 229712.77 ng****response 4165989**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.12
183.00	11.20	11.17
0.00	0.00	0.00