
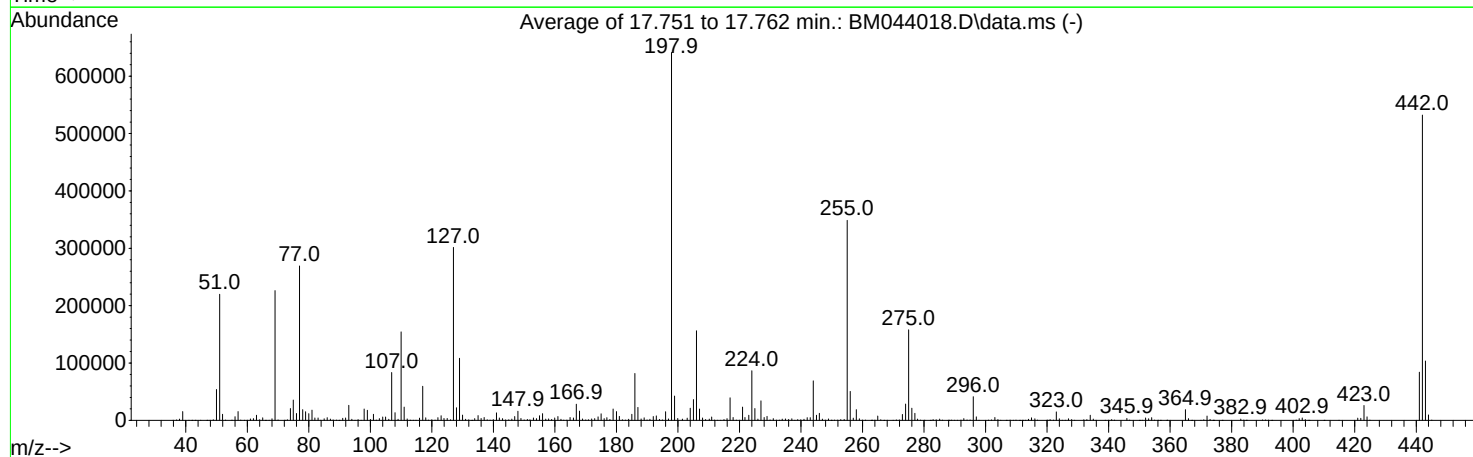


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM020824\  
Data File : BM044018.D  
Acq On : 08 Feb 2024 12:43  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM020824.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Fri Feb 09 02:42:01 2024

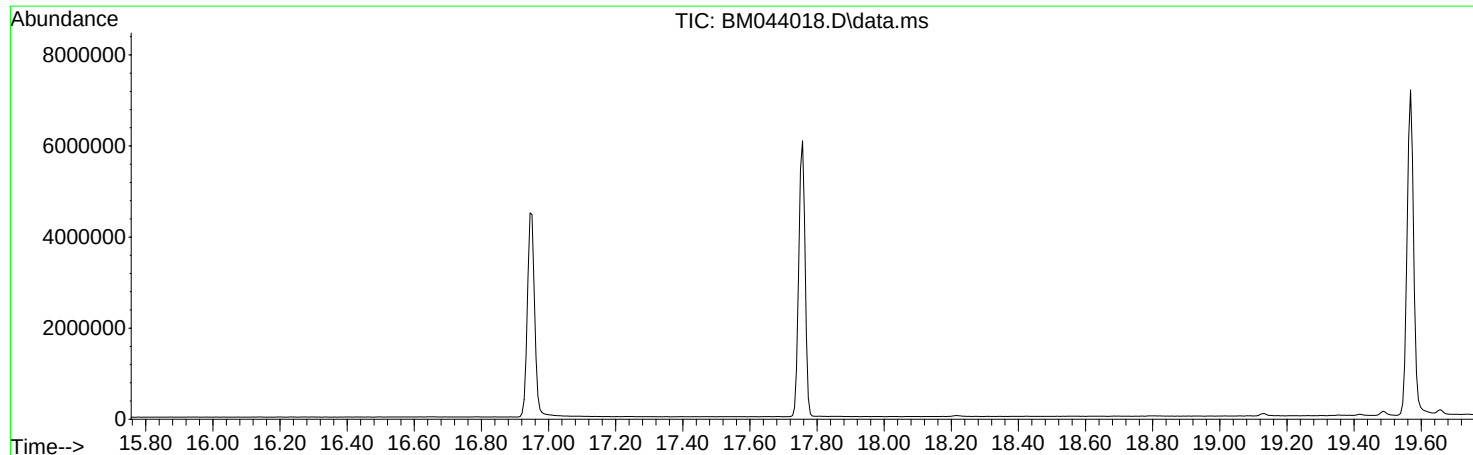




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2485

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 34.3         | 219873     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.3          | 2935       | PASS                |
| 69             | 198             | 0.00            | 100             | 35.3         | 226142     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.4          | 966        | PASS                |
| 127            | 198             | 10              | 80              | 47.0         | 301483     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.4          | 2524       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 641280     | PASS                |
| 199            | 198             | 5               | 9               | 6.6          | 42331      | PASS                |
| 275            | 198             | 10              | 60              | 24.6         | 157867     | PASS                |
| 365            | 198             | 1               | 100             | 2.9          | 18664      | PASS                |
| 441            | 198             | 0.01            | 100             | 13.1         | 84024      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 532117     | PASS                |
| 443            | 442             | 15              | 24              | 19.4         | 103475     | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM020824\  
Data File : BM044018.D  
Acq On : 08 Feb 2024 12:43  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Feb 09 02:49:42 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM020824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Feb 09 02:42:01 2024  
Response via : Initial Calibration

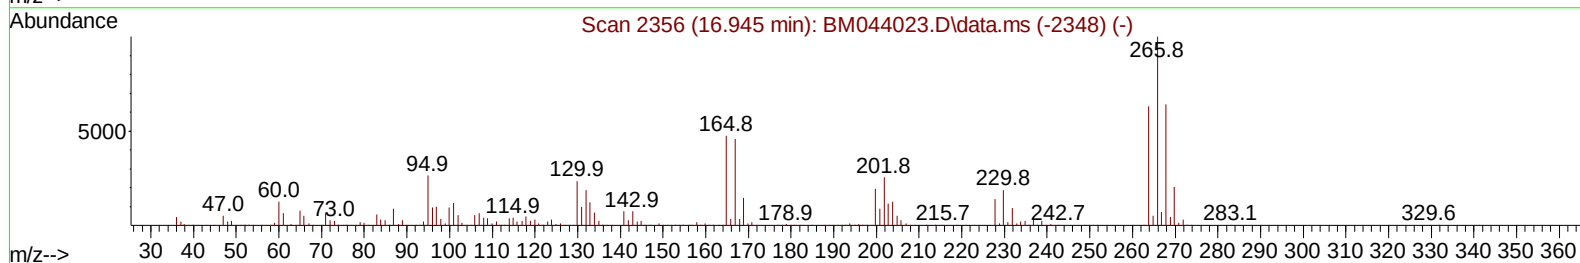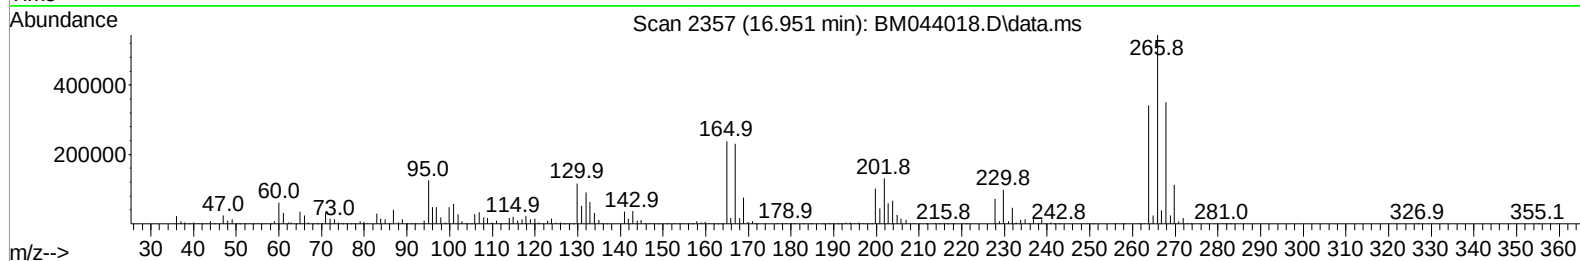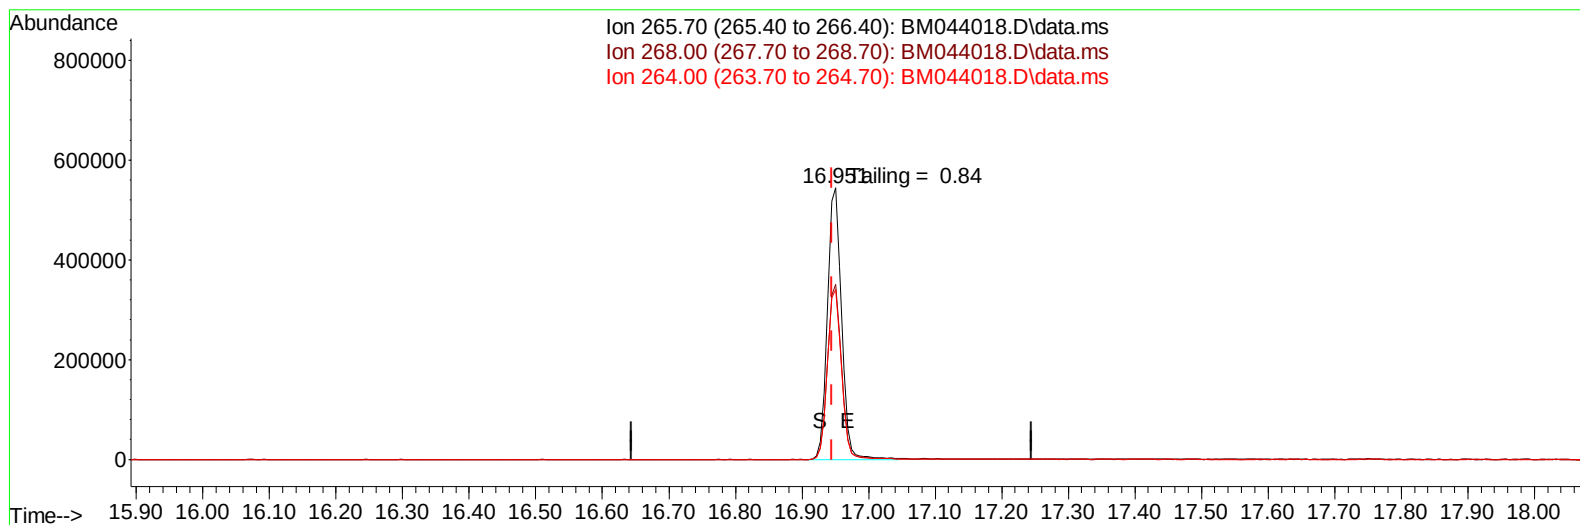

TIC: BM044018.D\data.ms

**(70) Pentachlorophenol (C)**

**16.951min (+ 0.006) 0.00 ng**




**response 804760**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.90  | 64.51  |
| 264.00 | 63.10  | 62.66  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM020824\  
Data File : BM044018.D  
Acq On : 08 Feb 2024 12:43  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Feb 09 02:49:42 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM020824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Feb 09 02:42:01 2024  
Response via : Initial Calibration

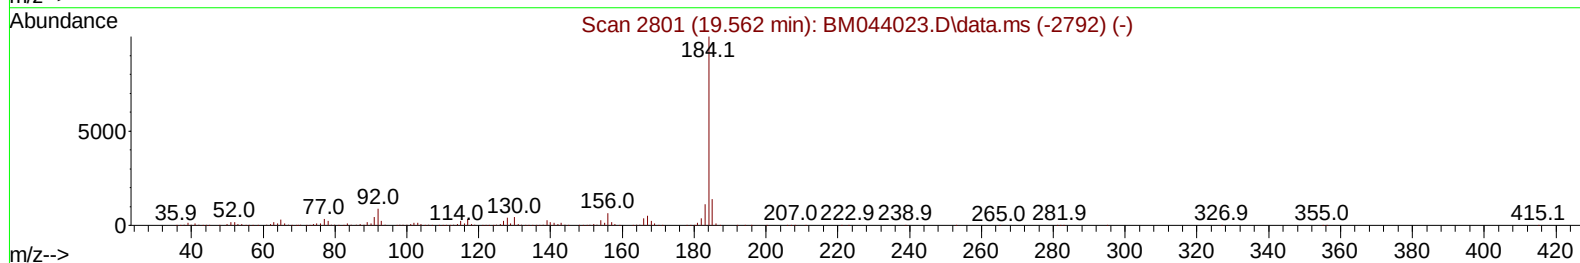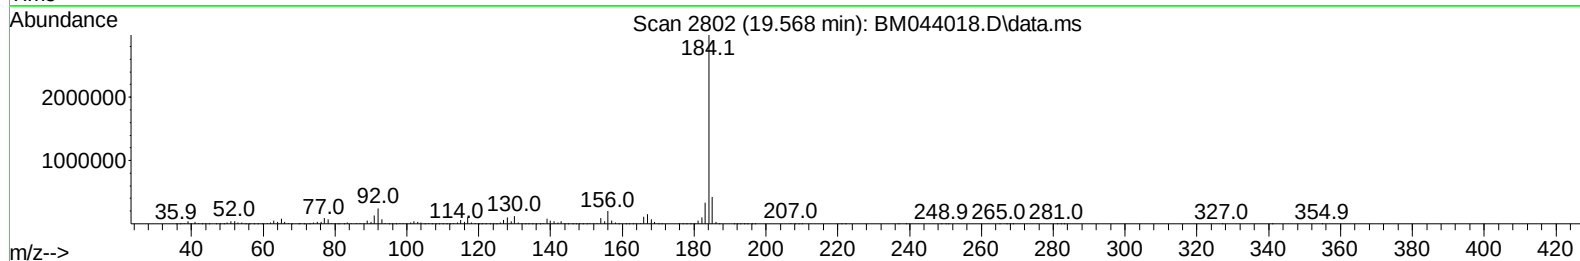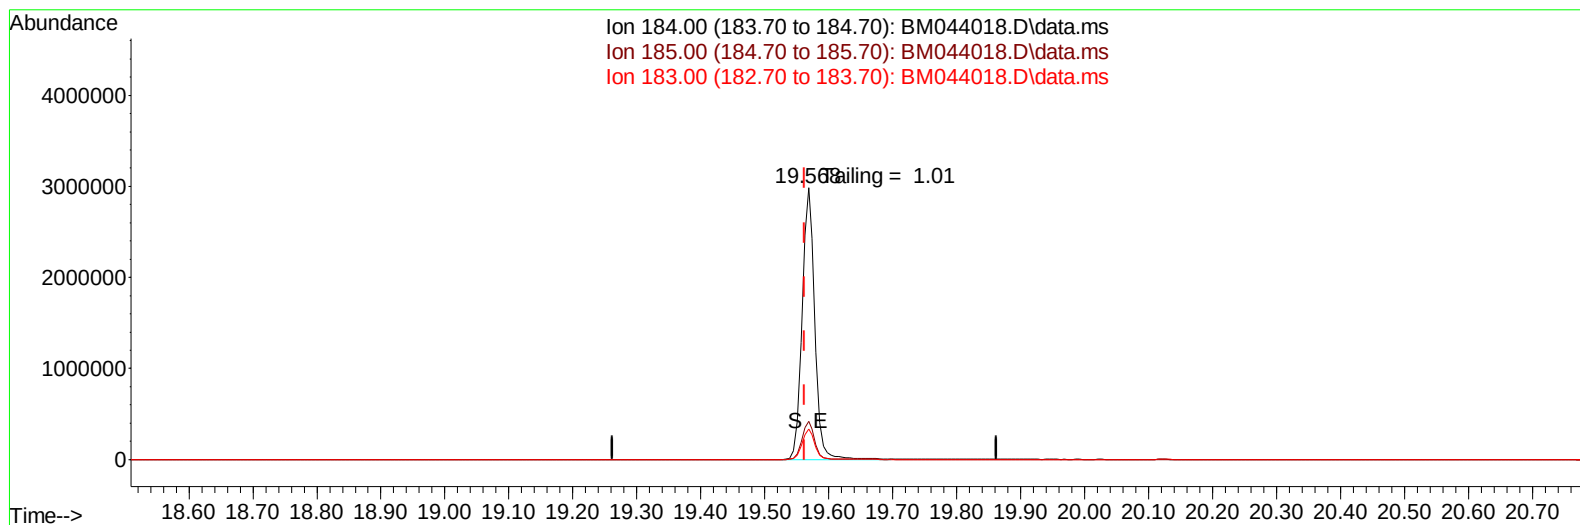

TIC: BM044018.D\data.ms

(77) Benzidine

19.568min (+ 0.006) 229712.77 ng

response 4165989

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.80  | 14.12  |
| 183.00 | 11.20  | 11.17  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 2/8/2024      | BNA_M            | <u>BM044018.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 1992602          | 20.803             |
| DDD           | 35566            | 20.362             |
| DDE           | 1295             | 19.851             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 36861         | 2029463          | 1.82               |
|               |                  |                    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP