

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020915\
 Data File : BM000456.D
 Acq On : 10 Feb 2015 07:44
 Operator : TP/IZ
 Sample : G1249-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4FL4

Quant Time: Feb 10 10:44:41 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM020615.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 10 05:48:08 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	186941	20.00	ng/ul	0.00
18) Naphthalene-d8	10.51	136	760914	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.37	164	462131	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.12	188	1042065	20.00	ng/ul	0.00
75) Chrysene-d12	21.31	240	1114372	20.00	ng/ul	0.00
83) Perylene-d12	23.56	264	1037987	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	6.89	99	70531	5.68	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	212169	27.78	ng/ul	0.00
9) 2-Chlorophenol-d4	7.26	132	239968	22.22	ng/ul	0.00
13) 4-Methylphenol-d8	8.43	113	138705	13.48	ng/ul	0.00
19) Nitrobenzene-d5	8.88	128	141676	29.72	ng/ul	0.00
22) 2-Nitrophenol-d4	9.60	143	158747	29.46	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.13	165	279577	24.09	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	1300	0.12	ng/ul	-0.13
43) Dimethylphthalate-d6	13.78	166	990023	31.09	ng/ul	0.00
46) Acenaphthylene-d8	14.06	160	1235754	28.40	ng/ul	0.00
51) 4-Nitrophenol-d4	14.57	143	18447	3.54	ng/ul	0.00
57) Fluorene-d10	15.37	176	904798	28.23	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.49	200	134480	24.39	ng/ul	0.00
70) Anthracene-d10	17.22	188	1354483	28.58	ng/ul	0.00
76) Pyrene-d10	19.52	212	1487273	28.32	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.42	264	1278330	27.57	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) 2,6-Dinitrotoluene	13.79	165	8336	1.35	ng/ul#	38


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020915\
Data File : BM000456.D
Acq On : 10 Feb 2015 07:44
Operator : TP/IZ
Sample : G1249-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4FL4

Quant Time: Feb 10 10:44:41 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM020615.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 10 05:48:08 2015
Response via : Initial Calibration

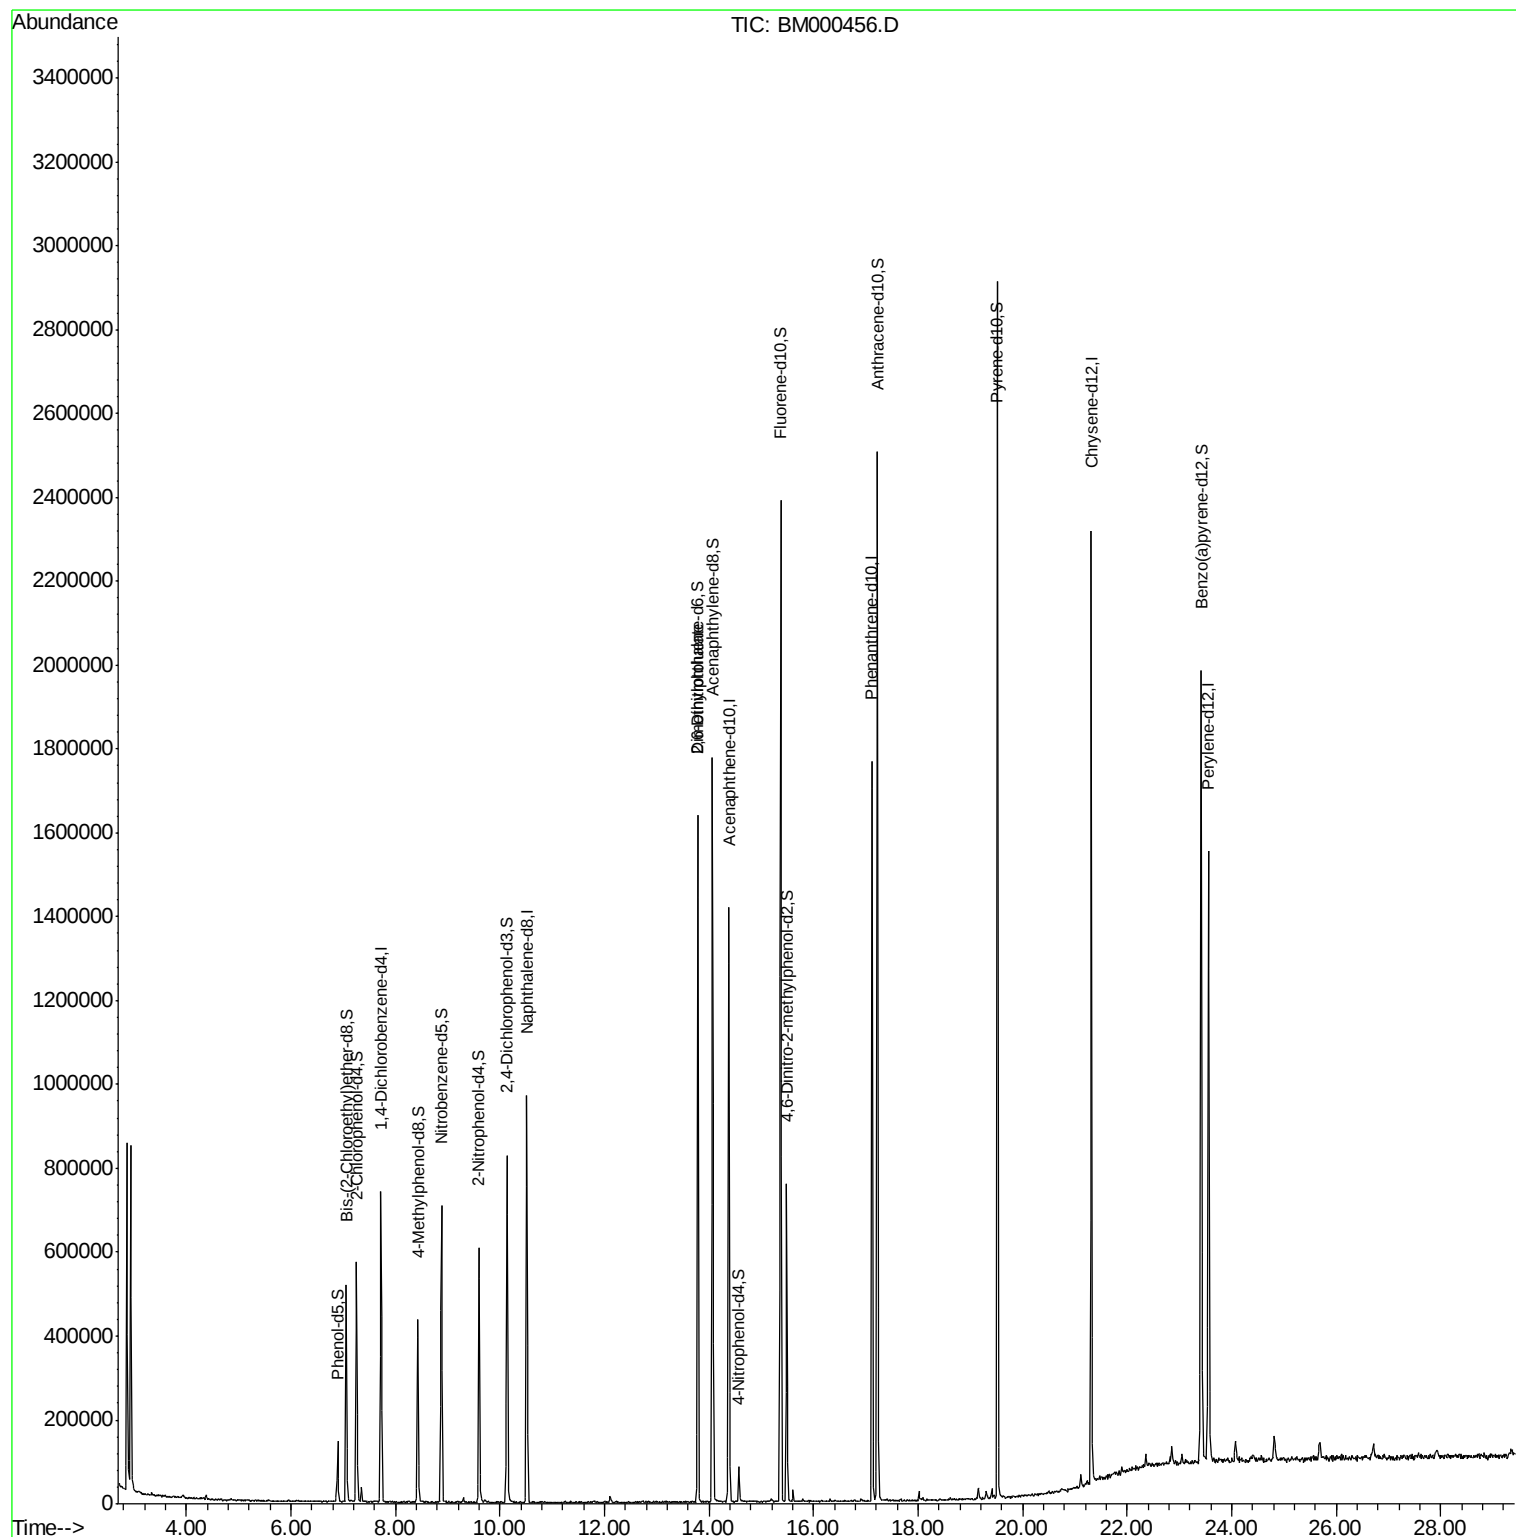

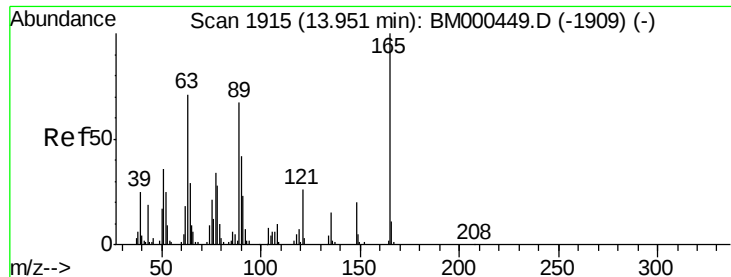

#45

2,6-Dinitrotoluene

Concen: 1.35 ng/ul

RT: 13.79 min Scan# 1887

Delta R.T. -0.16 min

Lab File: BM000456.D

Acq: 10 Feb 2015 07:44

Instrument :

BNA_M

ClientSampleId :

A4FL4



Tot Ion:165 Resp: 8336

Ion Ratio Lower Upper

165 100

89 0.0 50.2 75.2#

121 18.9 17.1 25.7

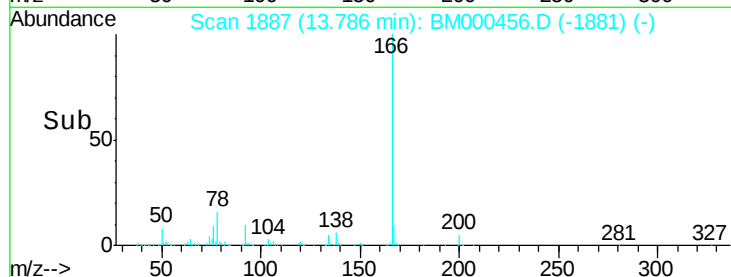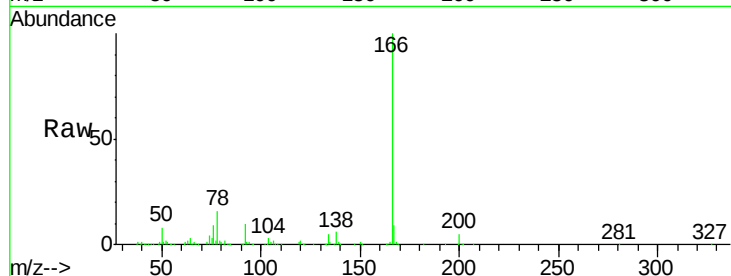

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

