

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020915\
 Data File : BM000460.D
 Acq On : 10 Feb 2015 10:06
 Operator : TP/IZ
 Sample : G1249-15
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4FM7

Quant Time: Feb 10 10:54:53 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM020615.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 10 05:48:08 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	193609	20.00	ng/ul	0.00
18) Naphthalene-d8	10.52	136	810557	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.37	164	533404	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.12	188	1217139	20.00	ng/ul	0.00
75) Chrysene-d12	21.32	240	1312137	20.00	ng/ul	0.00
83) Perylene-d12	23.56	264	1218667	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	6.89	99	73554	5.72	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	199370	25.20	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	239565	21.42	ng/ul	0.00
13) 4-Methylphenol-d8	8.43	113	143024	13.42	ng/ul	0.00
19) Nitrobenzene-d5	8.88	128	128662	25.34	ng/ul	0.00
22) 2-Nitrophenol-d4	9.60	143	148329	25.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.13	165	278109	22.49	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	11375	1.00	ng/ul	0.00
43) Dimethylphthalate-d6	13.78	166	954964	25.98	ng/ul	0.00
46) Acenaphthylene-d8	14.06	160	1150979	22.92	ng/ul	0.00
51) 4-Nitrophenol-d4	14.57	143	21610	3.59	ng/ul	0.00
57) Fluorene-d10	15.37	176	870304	23.53	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.49	200	130543	20.27	ng/ul	0.00
70) Anthracene-d10	17.22	188	1331990	24.06	ng/ul	0.00
76) Pyrene-d10	19.52	212	1493821	24.15	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.42	264	1188682	21.84	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) 2,6-Dinitrotoluene	13.79	165	7413	1.04	ng/ul#	38




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020915\
Data File : BM000460.D
Acq On : 10 Feb 2015 10:06
Operator : TP/IZ
Sample : G1249-15
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4FM7

Quant Time: Feb 10 10:54:53 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM01.2-EPA-BM020615.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 10 05:48:08 2015
Response via : Initial Calibration

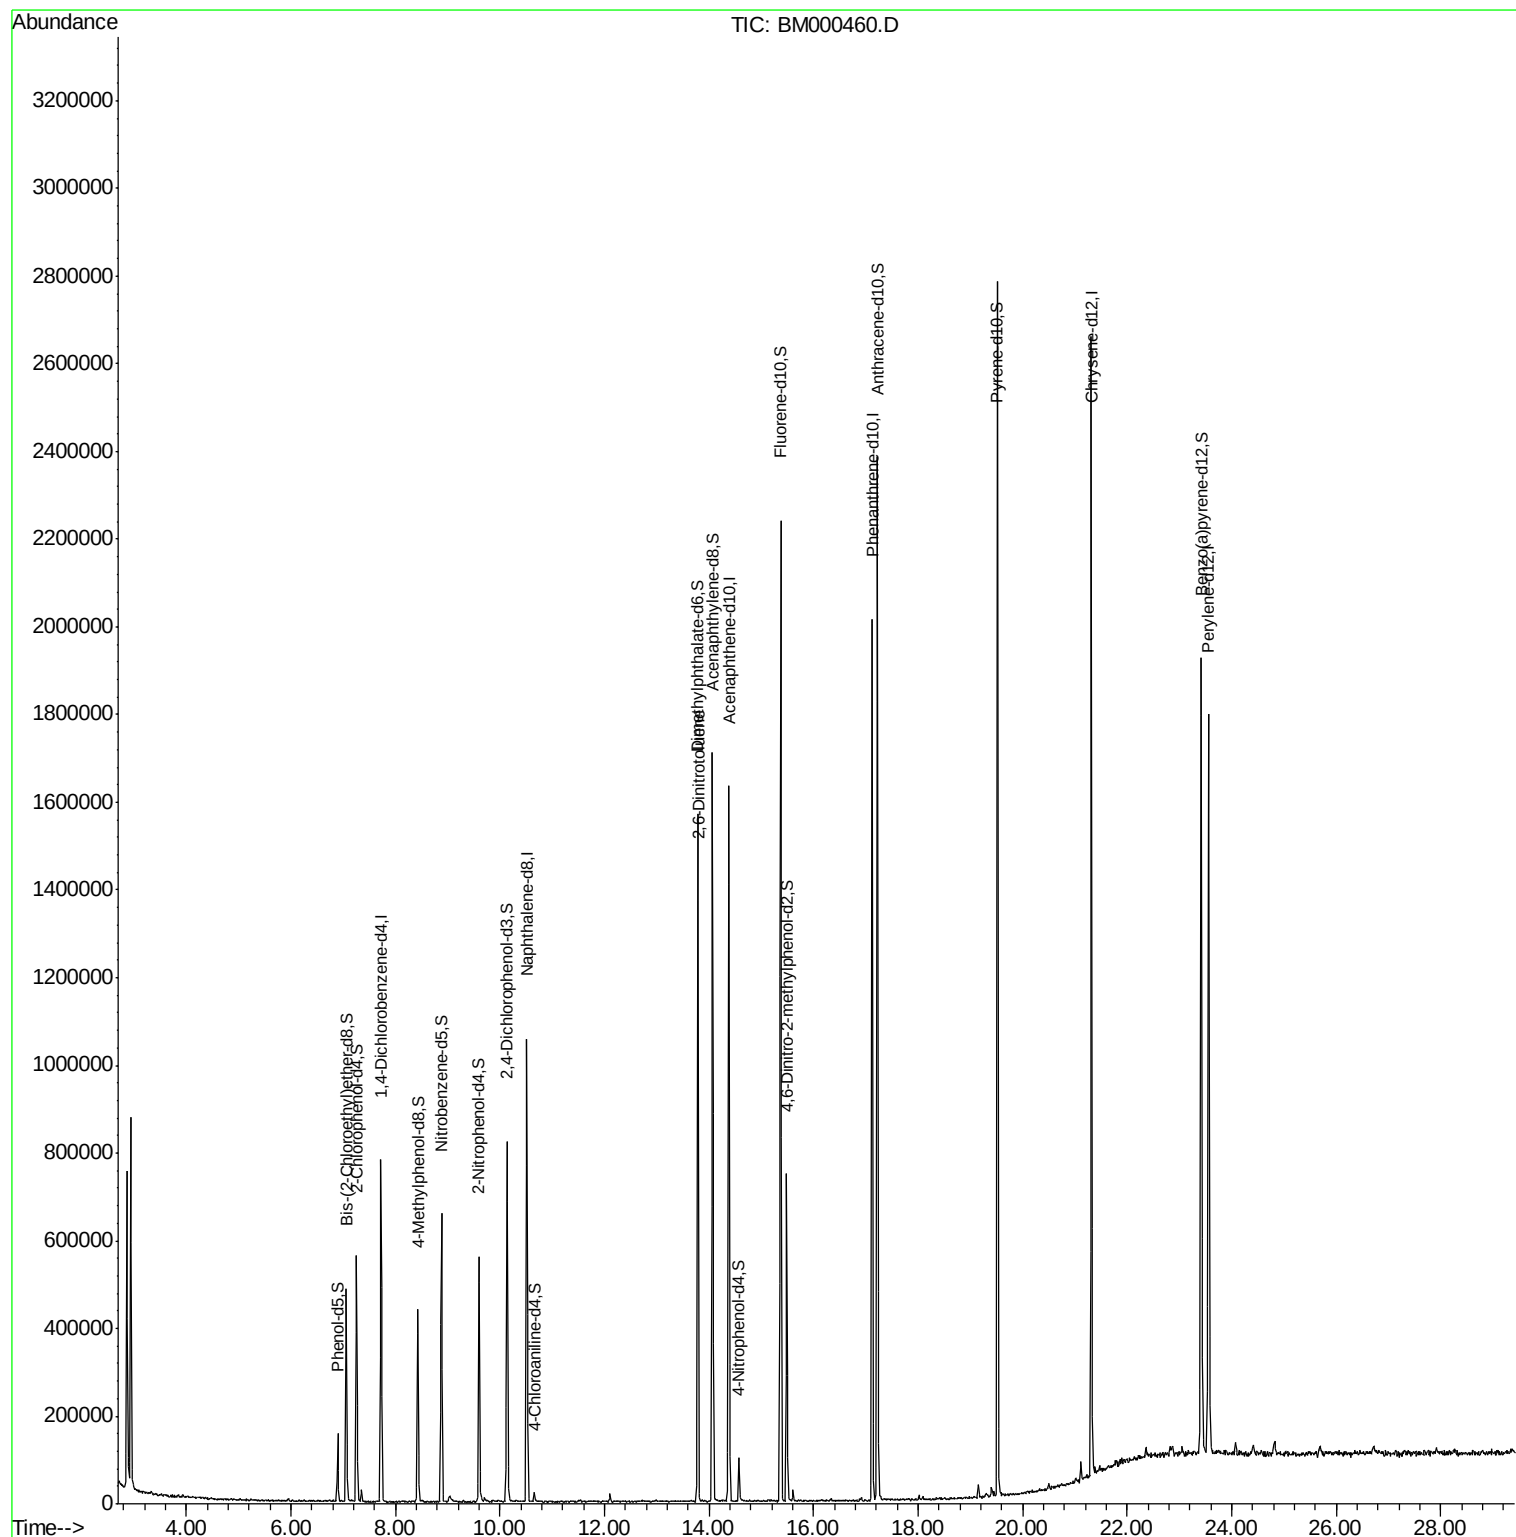

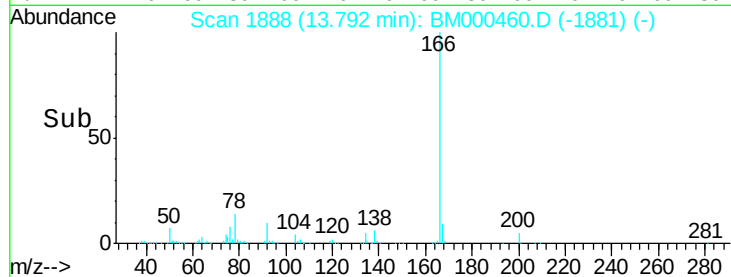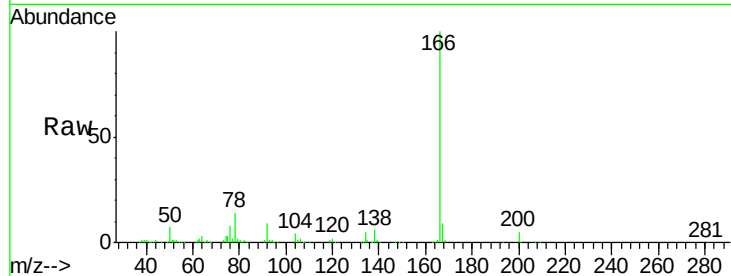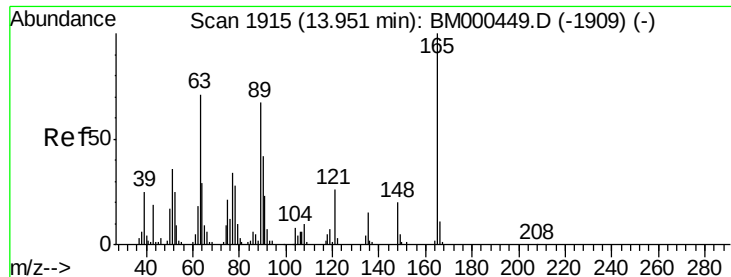

#45

2,6-Dinitrotoluene

Concen: 1.04 ng/ul

RT: 13.79 min Scan# 1888

Delta R.T. -0.16 min

Lab File: BM000460.D

Acq: 10 Feb 2015 10:06

Instrument :

BNA_M

ClientSampleId :

A4FM7

Tot Ion:165 Resp: 7413

Ion Ratio Lower Upper

165 100

89 0.0 50.2 75.2#

121 18.0 17.1 25.7

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

