

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020915\
 Data File : BM000466.D
 Acq On : 10 Feb 2015 20:20
 Operator : TP/IZ
 Sample : PB81660BL
 Misc : SBLK18
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK18

Quant Time: Feb 11 04:12:28 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM020615.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 11 04:03:52 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	100029	20.00	ng/ul	0.00
18) Naphthalene-d8	10.52	136	398974	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.37	164	244270	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.12	188	536397	20.00	ng/ul	0.00
75) Chrysene-d12	21.31	240	566306	20.00	ng/ul	0.00
83) Perylene-d12	23.56	264	525428	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	6.89	99	203673	30.66	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	125989	30.82	ng/ul	0.00
9) 2-Chlorophenol-d4	7.26	132	177378	30.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.43	113	165428	30.05	ng/ul	0.00
19) Nitrobenzene-d5	8.88	128	82542	33.03	ng/ul	0.00
22) 2-Nitrophenol-d4	9.60	143	89161	31.56	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.13	165	170001	27.93	ng/ul	0.00
29) 4-Chloroaniline-d4	10.65	131	227073	40.60	ng/ul	0.00
43) Dimethylphthalate-d6	13.78	166	549825	32.67	ng/ul	0.00
46) Acenaphthylene-d8	14.06	160	684325	29.76	ng/ul	0.00
51) 4-Nitrophenol-d4	14.57	143	68301	24.80	ng/ul	0.00
57) Fluorene-d10	15.37	176	498873	29.45	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.49	200	69998	24.66	ng/ul	0.00
70) Anthracene-d10	17.22	188	755063	30.95	ng/ul	0.00
76) Pyrene-d10	19.52	212	819609	30.71	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.41	264	730298	31.12	ng/ul	0.00


Target Compounds					Qvalue
45) 2,6-Dinitrotoluene	13.79	165	3964	1.21 ng/ul#	34


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020915\
Data File : BM000466.D
Acq On : 10 Feb 2015 20:20
Operator : TP/IZ
Sample : PB81660BL
Misc : SBLK18
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK18

Quant Time: Feb 11 04:12:28 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM020615.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 11 04:03:52 2015
Response via : Initial Calibration

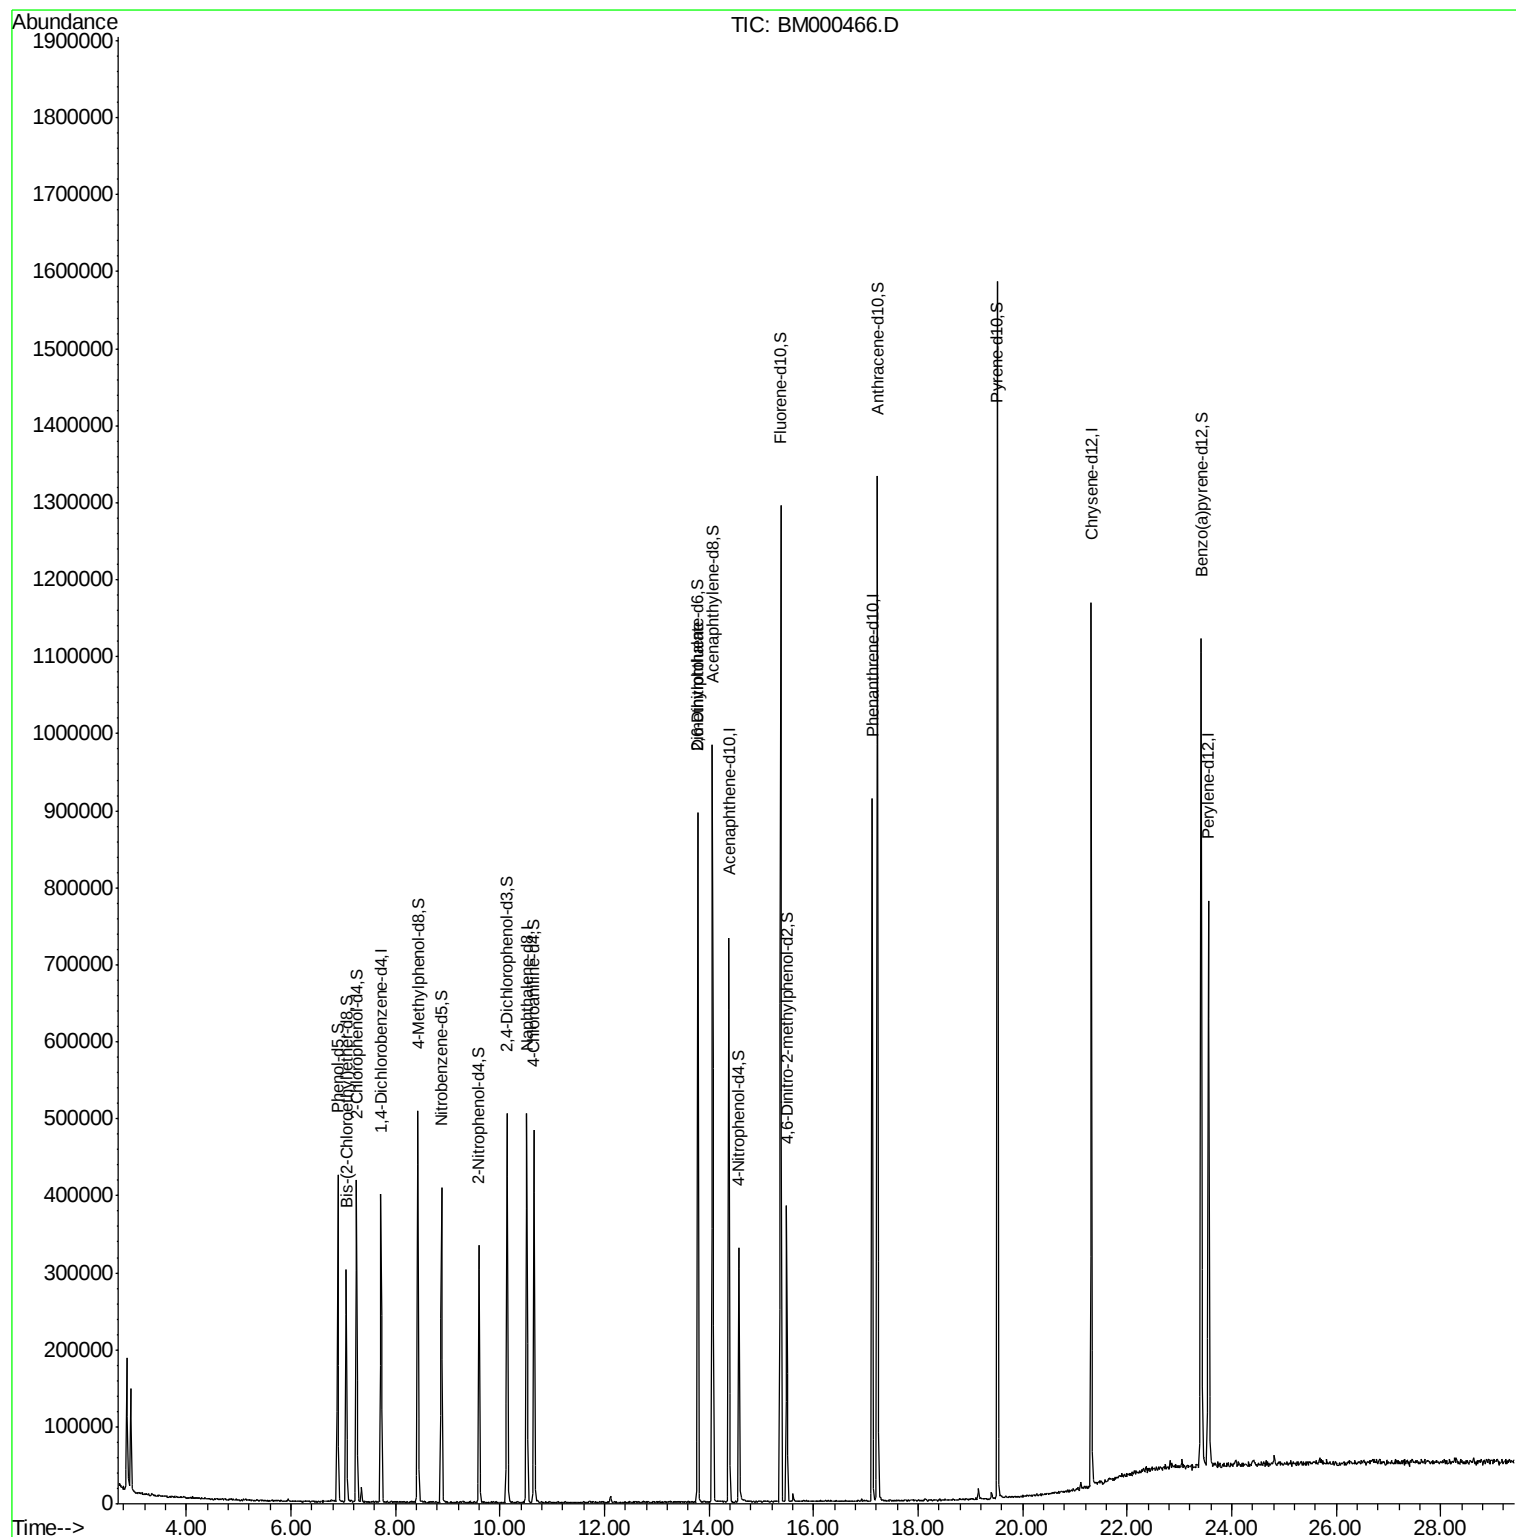

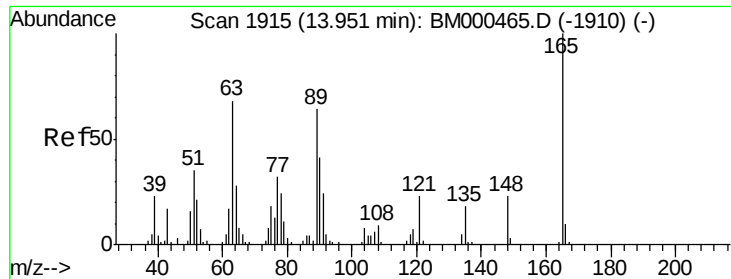

#45

2,6-Dinitrotoluene

Concen: 1.21 ng/ul

RT: 13.79 min Scan# 1887

Delta R.T. -0.16 min

Lab File: BM000466.D

Acq: 10 Feb 2015 20:20

Instrument :

BNA_M

ClientSampleId :

SBLK18


Tgt Ion:165 Resp: 3964

Ion Ratio Lower Upper

165 100

89 0.0 50.2 75.2#

121 31.3 17.1 25.7#

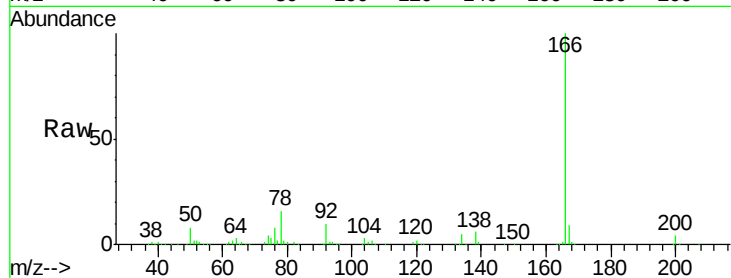

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

