

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020915\
 Data File : BM000471.D
 Acq On : 10 Feb 2015 23:18
 Operator : TP/IZ
 Sample : G1249-23
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4FN6

Quant Time: Feb 11 04:12:58 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM020615.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 11 04:03:52 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	103915	20.00	ng/ul	0.00
18) Naphthalene-d8	10.51	136	421125	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.37	164	258112	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.12	188	569905	20.00	ng/ul	0.00
75) Chrysene-d12	21.31	240	586005	20.00	ng/ul	0.00
83) Perylene-d12	23.55	264	549144	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	6.89	99	35973	5.21	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.06	67	105786	24.91	ng/ul	0.00
9) 2-Chlorophenol-d4	7.26	132	120012	19.99	ng/ul	0.00
13) 4-Methylphenol-d8	8.43	113	69041	12.07	ng/ul	0.00
19) Nitrobenzene-d5	8.88	128	68782	26.07	ng/ul	0.00
22) 2-Nitrophenol-d4	9.60	143	75224	25.22	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.13	165	142202	22.14	ng/ul	0.00
29) 4-Chloroaniline-d4	10.66	131	2220	0.38	ng/ul	0.00
43) Dimethylphthalate-d6	13.78	166	499224	28.07	ng/ul	0.00
46) Acenaphthylene-d8	14.06	160	612995	25.23	ng/ul	0.00
51) 4-Nitrophenol-d4	14.57	143	9520	3.27	ng/ul	0.00
57) Fluorene-d10	15.37	176	448526	25.06	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.49	200	68713	22.78	ng/ul	0.00
70) Anthracene-d10	17.22	188	703773	27.15	ng/ul	0.00
76) Pyrene-d10	19.52	212	775920	28.09	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.41	264	633430	25.82	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) 2,6-Dinitrotoluene	13.79	165	3888	1.12	ng/ul#	37


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020915\
Data File : BM000471.D
Acq On : 10 Feb 2015 23:18
Operator : TP/IZ
Sample : G1249-23
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4FN6

Quant Time: Feb 11 04:12:58 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM020615.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 11 04:03:52 2015
Response via : Initial Calibration

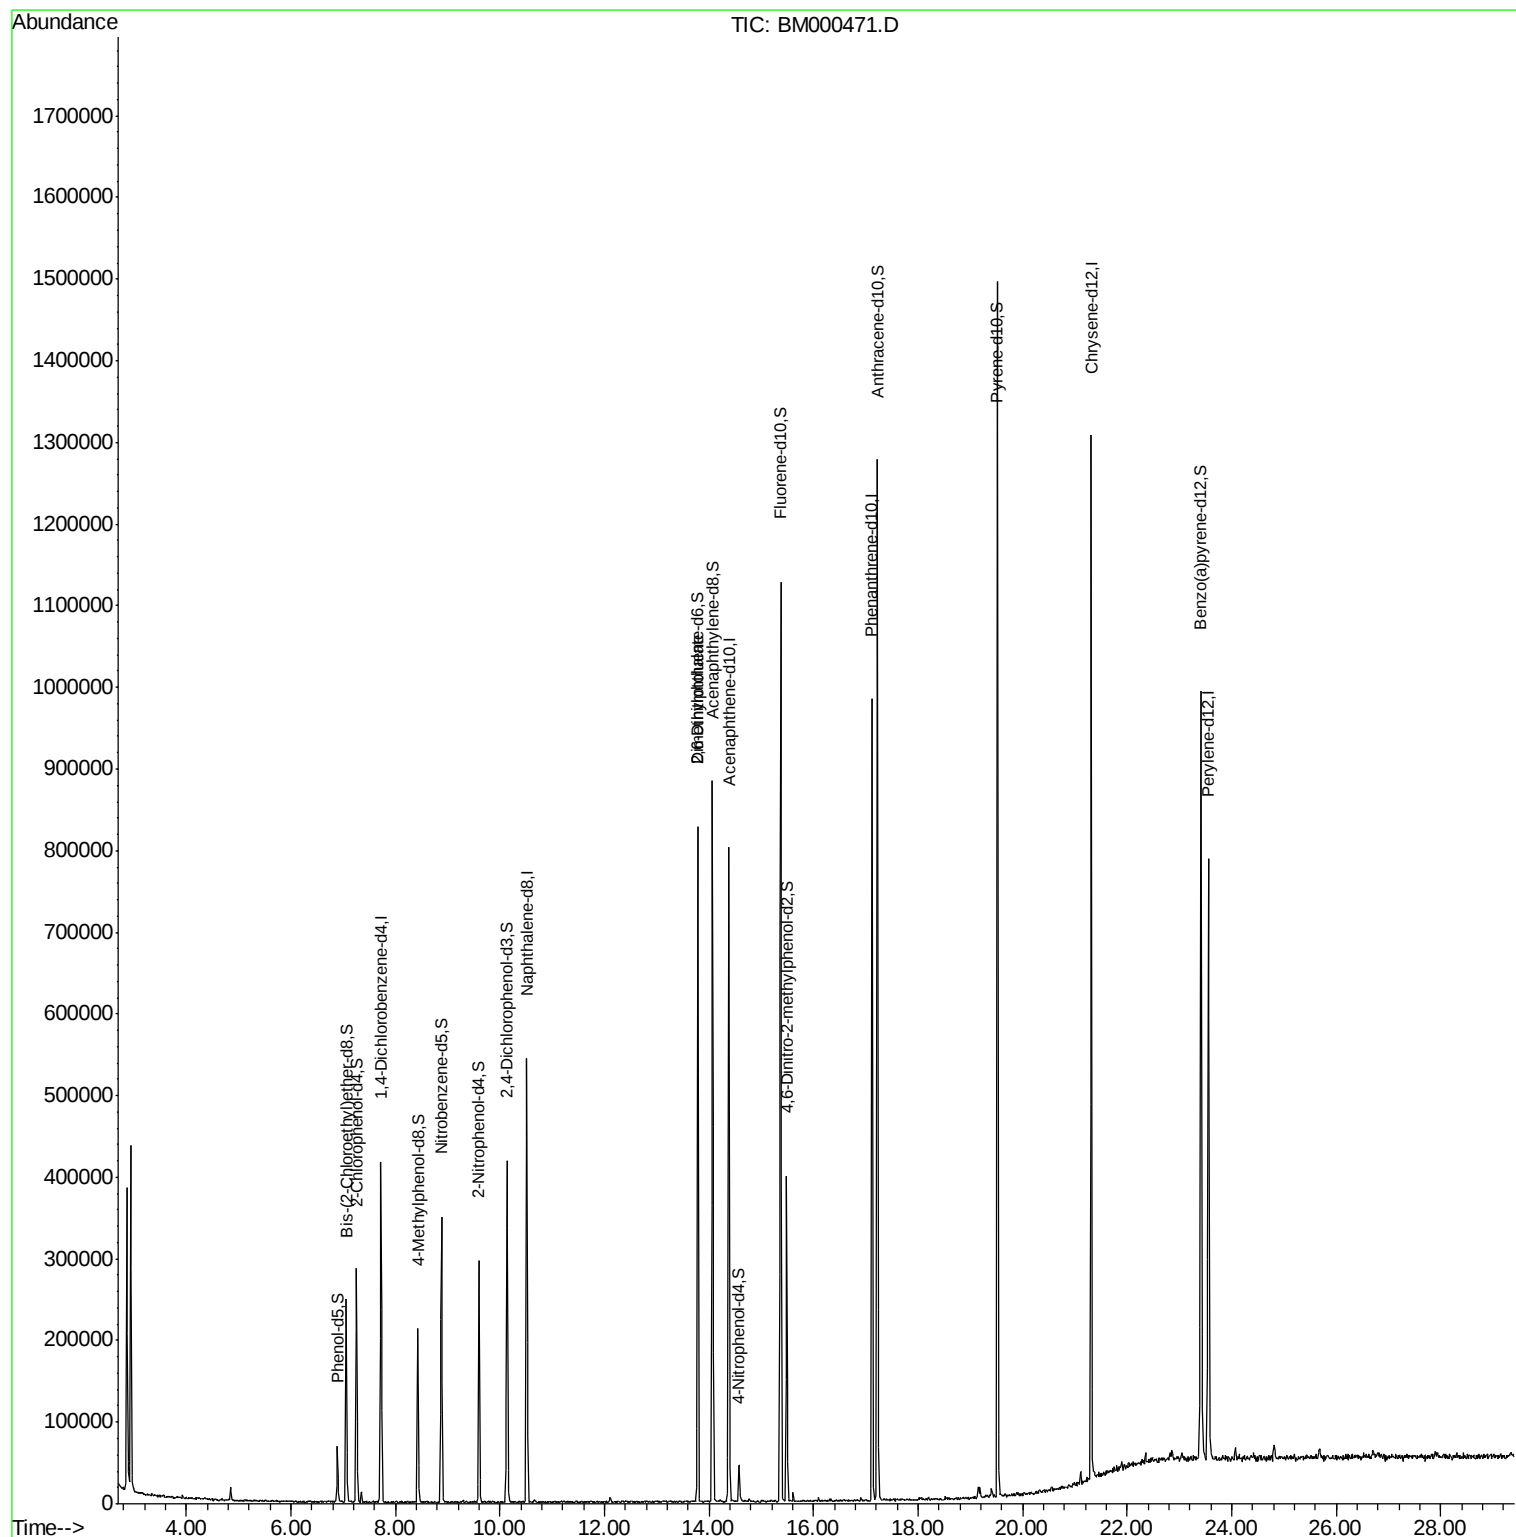

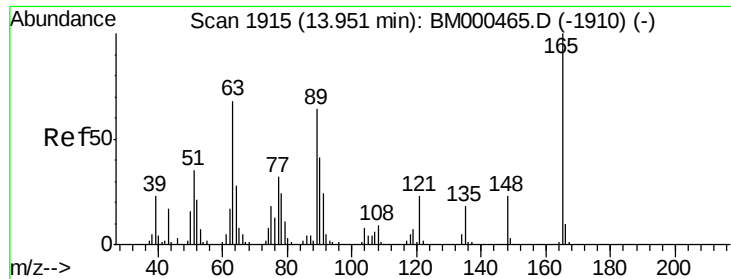

#45
 2,6-Dinitrotoluene
 Concen: 1.12 ng/ul
 RT: 13.79 min Scan# 1887
 Delta R.T. -0.16 min
 Lab File: BM000471.D
 Acq: 10 Feb 2015 23:18

Instrument :
 BNA_M
 ClientSampleId :
 A4FN6

Tgt Ion	Ratio	Lower	Upper
165	100		
89	0.0	50.2	75.2#
121	26.8	17.1	25.7#

