


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020915\
 Data File : BM000448.D
 Acq On : 10 Feb 2015 03:00
 Operator : TP/IZ
 Sample : DFTPP20
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP20

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-BM020615.M
 Title : SVOA CALIBRATION
 Last Update : Tue Feb 10 05:48:08 2015

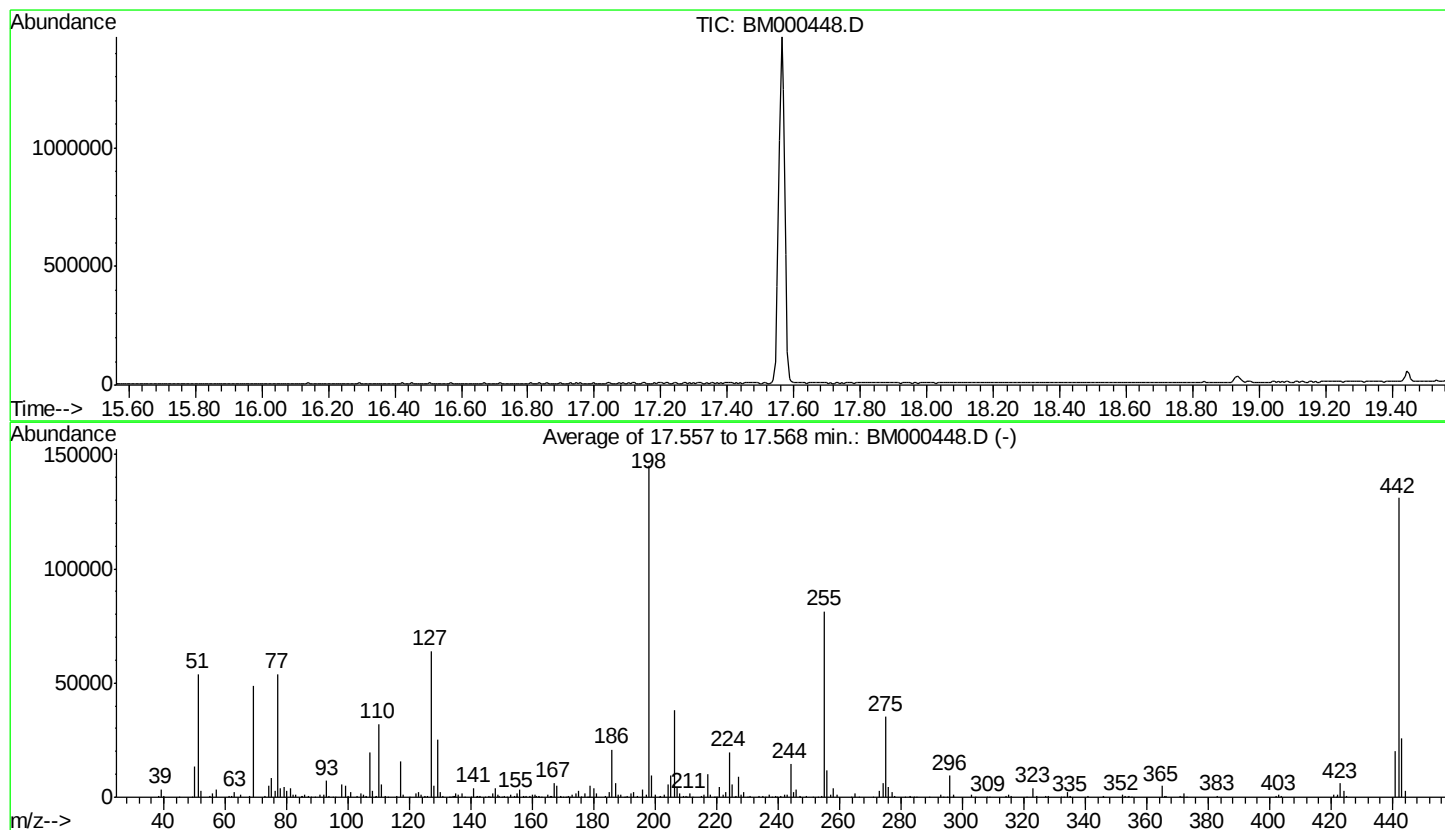

AutoFind: Scans 2528, 2529, 2530; Background Corrected with Scan 2523

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	54058	PASS
68	69	0.00	2	1.6	790	PASS
69	198	0.00	100	33.5	48568	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.0	63898	PASS
197	198	0.00	2	0.8	1117	PASS
198	198	100	100	100.0	145178	PASS
199	198	5	9	6.6	9522	PASS
275	198	10	60	24.2	35197	PASS
365	198	1	100	3.3	4830	PASS
441	443	0.01	100	77.9	19990	PASS
442	198	50	100	90.2	131018	PASS
443	442	15	24	19.6	25666	PASS

m/z	Abundance
38.10	478.0
39.10	3428.0
40.00	1103.0
44.00	3788.0
49.20	467.0
50.00	13293.0
51.10	52984.0
52.10	2930.0
55.10	512.0
56.00	1314.0
57.10	3273.0
61.10	995.0
62.10	730.0
63.10	2281.0
65.00	1019.0
68.10	1051.0
69.00	45032.0
73.10	1256.0
74.10	4556.0
75.00	10021.0
76.00	2470.0
77.10	49920.0
78.00	3735.0
79.00	4112.0
80.00	3109.0
81.00	3668.0
82.10	1111.0
83.10	1033.0
84.80	525.0
85.20	537.0
86.00	1178.0
87.00	621.0
89.00	310.0
91.00	944.0
92.00	1199.0
93.00	6299.0
94.00	528.0
98.00	5567.0
99.00	5618.0
100.00	351.0
101.00	2228.0
102.90	662.0
104.00	1625.0
105.00	1369.0
105.70	394.0
107.00	17104.0
108.10	2544.0
108.80	560.0
110.00	27744.0
111.00	4325.0
112.10	434.0
116.00	688.0
117.00	14547.0
118.10	1073.0
122.10	1443.0
123.10	1754.0
124.00	963.0
125.00	1048.0
126.00	316.0
127.00	57552.0
128.00	4488.0
129.00	22032.0
130.10	2046.0
134.00	888.0
134.80	988.0
135.20	1096.0
136.20	588.0
137.00	1504.0
138.00	353.0
141.00	3882.0
142.00	1119.0
143.00	922.0
146.00	477.0
147.00	2353.0
148.00	3770.0
149.00	1220.0
149.90	370.0
150.90	534.0
151.80	486.0
153.00	983.0
154.10	510.0
154.90	1417.0
155.20	1305.0
156.00	2949.0
157.00	482.0
158.00	608.0
159.10	585.0
160.00	972.0
160.90	1178.0
161.90	660.0
164.80	1067.0

Instrument :
BNA_M
ClientSampleId :
DFTPP20

165.90	883.0
167.00	5821.0
168.00	4859.0
169.00	912.0
171.90	644.0
173.00	781.0
174.00	1885.0
175.00	2330.0
176.00	428.0
177.00	1375.0
178.00	380.0
179.00	3993.0
180.00	3964.0
181.00	1696.0
184.00	664.0
185.10	2102.0
186.00	16280.0
187.10	4933.0
188.10	1334.0
188.90	938.0
190.90	670.0
192.00	1481.0
193.10	1609.0
194.00	301.0
196.10	2910.0
197.10	861.0
198.00	120208.0
199.00	8322.0
199.90	567.0
201.70	415.0
202.90	934.0
204.00	4722.0
205.10	8309.0
206.10	30944.0
207.10	5314.0
208.00	1167.0
209.00	656.0
210.40	405.0
211.10	1218.0
212.00	372.0
215.90	671.0
217.00	7602.0
218.00	994.0
219.90	403.0
221.00	3702.0
222.00	1089.0
223.00	2326.0
224.10	16464.0
225.00	4010.0
225.90	574.0
227.00	7870.0
228.00	1343.0
228.90	1511.0
230.20	351.0
231.00	696.0
234.00	539.0
234.90	528.0
237.00	1068.0
239.00	346.0
239.80	384.0
240.70	472.0
242.20	969.0
243.10	911.0
244.10	12465.0
245.10	2214.0
245.90	2081.0
247.00	541.0
249.00	509.0
254.10	550.0
255.00	64536.0
256.00	9813.0
257.00	1147.0
258.10	2404.0
259.00	563.0
264.90	1219.0
270.90	323.0
273.10	1734.0
274.10	4573.0
275.10	25368.0
276.10	3529.0
277.00	1672.0
278.10	416.0
282.80	631.0
293.00	814.0
293.90	374.0
296.00	7521.0
296.90	941.0
303.20	832.0
304.10	301.0
308.00	321.0
315.00	815.0
316.10	639.0
323.00	3851.0
323.90	496.0
327.00	338.0

Instrument :
BNA_M
ClientSampleId :
DFTPP20

332.10	339.0
334.20	1429.0
335.20	638.0
352.10	397.0
353.00	505.0
354.00	1069.0
365.00	3635.0
365.90	501.0
371.00	447.0
372.10	1323.0
383.10	372.0
402.00	732.0
403.10	639.0
403.90	302.0
421.10	824.0
422.10	621.0
423.10	3662.0
424.00	1877.0
425.00	419.0
441.10	13178.0
442.00	80416.0
443.10	16632.0
444.00	1710.0

Instrument :
BNA_M
ClientSampleId :
DFTPP20

m/z	Abundance
38.10	885.0
39.10	3717.0
40.00	1393.0
44.00	3448.0
50.10	16352.0
51.10	63240.0
52.10	3607.0
55.00	411.0
56.00	2107.0
57.00	3831.0
61.00	675.0
61.90	798.0
63.00	2857.0
65.10	1079.0
67.90	811.0
69.00	58224.0
73.10	931.0
74.00	5558.0
75.10	7578.0
76.10	2994.0
77.10	63712.0
78.10	4898.0
79.00	5640.0
80.00	3538.0
81.10	4587.0
82.00	1301.0
83.10	971.0
85.10	414.0
86.00	1666.0
87.00	839.0
87.90	334.0
91.00	1194.0
92.00	1333.0
93.00	9164.0
93.80	1292.0
96.00	442.0
98.00	6352.0
99.00	6773.0
100.00	522.0
101.10	2786.0
102.90	697.0
104.00	2054.0
104.80	1404.0
106.00	720.0
107.00	22176.0
108.00	3302.0
109.10	861.0
110.00	39080.0
111.00	6557.0
112.20	569.0
116.00	1231.0
117.00	18256.0
118.10	2202.0
120.00	324.0
121.90	2084.0
123.00	3262.0
123.90	1126.0
124.90	894.0
126.10	400.0
127.00	75792.0
128.00	5791.0
129.00	29848.0
130.00	2524.0
131.00	709.0
132.80	348.0
133.20	429.0
133.90	803.0
135.10	2535.0
136.00	1350.0
137.00	1351.0
140.10	729.0
141.00	4574.0
142.10	1245.0
142.80	771.0
143.10	694.0
144.80	313.0
145.80	449.0
146.30	593.0
147.00	1645.0
148.00	3678.0
148.90	1500.0
151.00	711.0
153.00	1471.0
154.00	1312.0
154.90	1957.0
156.00	3794.0
157.20	832.0
158.00	835.0
159.00	696.0
159.90	1621.0
161.10	2374.0

Instrument :
BNA_M
ClientSampleId :
DFTPP20

162.10	598.0
163.10	412.0
164.90	1467.0
166.10	1054.0
167.10	7840.0
168.00	6234.0
169.20	558.0
170.00	389.0
170.90	547.0
171.70	762.0
172.90	1274.0
174.00	2459.0
175.10	3414.0
176.10	467.0
177.00	1709.0
178.20	580.0
179.00	5754.0
180.00	5586.0
181.00	1793.0
183.80	663.0
184.90	3259.0
186.00	25136.0
187.10	7466.0
188.00	1505.0
189.00	1440.0
190.00	615.0
190.80	703.0
192.10	1817.0
193.00	2318.0
194.10	394.0
196.10	4729.0
197.10	1455.0
198.00	174528.0
199.00	12337.0
200.00	917.0
201.80	765.0
203.00	1080.0
204.00	6933.0
205.00	9776.0
206.10	45296.0
207.00	7698.0
208.10	2063.0
209.10	977.0
210.00	662.0
211.10	1762.0
215.00	516.0
216.00	970.0
217.00	12793.0
218.10	1411.0
219.00	416.0
219.40	395.0
219.90	425.0
221.10	3953.0
222.00	1161.0
222.90	2224.0
224.10	22128.0
225.10	6179.0
226.20	1085.0
227.00	9392.0
227.90	1373.0
229.00	2706.0
230.00	380.0
230.90	803.0
233.90	938.0
234.90	841.0
236.00	477.0
237.10	1316.0
239.00	432.0
240.80	332.0
242.00	1410.0
243.10	1169.0
244.10	15952.0
245.10	2038.0
246.00	4405.0
247.20	863.0
249.00	598.0
254.20	732.0
255.00	94704.0
256.10	13410.0
257.10	917.0
258.00	5695.0
259.00	1386.0
265.00	2567.0
266.10	313.0
273.00	2955.0
274.00	8055.0
275.10	42176.0
276.00	4658.0
277.00	2752.0
278.10	1177.0
283.10	432.0
285.00	418.0
289.10	394.0
292.90	796.0
295.10	333.0

Instrument :
BNA_M
ClientSampleId :
DFTPP20

296.00	10526.0
297.10	2164.0
303.00	1630.0
308.70	433.0
314.00	821.0
315.10	858.0
315.90	775.0
320.90	338.0
323.10	4220.0
324.00	706.0
327.10	642.0
327.90	354.0
332.20	549.0
333.10	361.0
334.00	2511.0
335.10	643.0
341.10	799.0
346.00	757.0
352.00	1064.0
352.90	528.0
354.10	1006.0
365.00	5577.0
366.10	934.0
371.00	497.0
372.10	1334.0
372.90	341.0
382.90	725.0
402.10	987.0
403.00	1257.0
403.90	438.0
421.00	1314.0
422.00	1625.0
423.00	6913.0
424.00	3585.0
425.10	599.0
441.10	22896.0
442.10	153920.0
443.00	29064.0
444.10	3126.0

Instrument :
BNA_M
ClientSampleId :
DFTPP20

m/z	Abundance
38.20	525.0
39.00	3657.0
40.00	1643.0
44.00	3526.0
44.80	450.0
49.00	358.0
50.10	11054.0
51.10	45952.0
52.10	2711.0
56.00	1245.0
57.00	2956.0
61.10	517.0
62.00	627.0
63.00	1917.0
64.90	946.0
68.00	508.0
69.00	42448.0
73.00	935.0
74.10	4854.0
75.10	7135.0
76.10	2288.0
77.10	48200.0
78.10	3311.0
79.10	4027.0
79.90	2487.0
81.00	3366.0
82.00	521.0
83.10	690.0
84.80	669.0
86.10	1323.0
86.90	725.0
91.00	1139.0
92.10	1196.0
93.00	6248.0
93.90	384.0
95.10	318.0
97.90	5105.0
98.90	3445.0
100.10	468.0
100.90	2020.0
103.00	787.0
104.00	1231.0
105.20	1749.0
106.00	328.0
107.00	18864.0
108.00	2583.0
109.10	326.0
110.00	29736.0
111.00	5373.0
112.00	356.0
112.80	395.0
116.10	481.0
117.00	14908.0
118.10	872.0
122.00	1589.0
123.00	2318.0
123.90	902.0
124.90	573.0
126.10	381.0
127.00	58352.0
128.00	4336.0
129.00	23120.0
130.10	1868.0
131.00	348.0
132.90	337.0
134.10	830.0
135.10	1701.0
136.00	818.0
137.10	1558.0
140.90	3591.0
141.80	910.0
142.70	554.0
146.00	614.0
147.00	1719.0
148.00	4059.0
149.20	1071.0
151.10	439.0
151.70	338.0
153.00	1183.0
154.10	733.0
155.00	2170.0
156.00	2963.0
157.10	349.0
158.10	622.0
159.00	788.0
160.00	1476.0
160.90	1556.0
162.20	415.0
163.10	316.0
165.00	1186.0
165.90	744.0

Instrument :
BNA_M
ClientSampleId :
DFTPP20

166.90	5248.0
168.00	4189.0
169.00	678.0
171.80	505.0
172.10	552.0
173.00	714.0
174.00	1266.0
175.10	2908.0
175.80	449.0
177.10	1255.0
178.00	300.0
178.90	5129.0
179.90	3105.0
181.00	1811.0
184.00	520.0
185.00	2205.0
186.10	21248.0
187.00	5543.0
187.90	808.0
189.00	1444.0
190.80	764.0
192.10	1746.0
193.10	2505.0
194.00	413.0
196.00	2976.0
197.10	1037.0
198.00	140800.0
198.90	7908.0
200.00	1511.0
201.30	713.0
201.90	515.0
203.00	1154.0
204.10	4714.0
205.00	10498.0
206.10	38648.0
207.10	6845.0
208.10	1131.0
209.00	632.0
210.10	601.0
211.10	1541.0
212.00	339.0
215.10	431.0
216.00	1117.0
217.00	9618.0
218.00	996.0
221.00	5318.0
222.10	1063.0
223.00	2319.0
224.10	20488.0
225.00	5943.0
227.00	9557.0
228.00	1351.0
229.00	2587.0
230.90	377.0
234.00	841.0
234.90	1157.0
236.10	426.0
236.90	1358.0
238.00	304.0
239.00	426.0
240.80	819.0
242.00	1087.0
243.10	1262.0
244.10	16112.0
245.10	2645.0
246.00	2843.0
247.00	696.0
249.10	676.0
251.10	364.0
253.00	515.0
254.20	1120.0
255.10	84752.0
256.00	11613.0
257.10	966.0
258.00	4543.0
259.10	839.0
263.90	350.0
265.10	1962.0
273.00	2981.0
274.00	5360.0
275.00	38048.0
276.00	5021.0
276.90	2955.0
278.00	846.0
281.10	312.0
283.00	500.0
284.10	349.0
285.10	412.0
293.00	1195.0
296.00	10034.0
297.00	1487.0
303.10	1449.0
314.10	508.0
314.90	1172.0
315.10	1179.0

Instrument :

BNA_M

ClientSampleId :

DFTPP20

316.00	846.0
320.90	350.0
323.00	3811.0
324.10	1167.0
326.90	726.0
328.00	711.0
333.10	432.0
334.10	2432.0
334.90	735.0
341.00	640.0
345.70	333.0
346.10	416.0
352.10	1453.0
353.00	899.0
353.80	656.0
355.00	396.0
365.00	5278.0
365.90	808.0
371.20	307.0
372.10	2197.0
373.00	414.0
383.10	659.0
402.00	836.0
403.10	890.0
403.90	421.0
421.00	1005.0
421.80	858.0
422.20	708.0
423.10	7775.0
424.10	3190.0
424.90	628.0
441.00	23896.0
442.00	158720.0
443.00	31304.0
444.00	3152.0

Instrument :
BNA_M
ClientSampleId :
DFTPP20

Scan 2523 (17.527 min): BM000448.D
DFTPP20

m/z	Abundance
40.00	965.0
41.10	336.0
44.00	4186.0
73.00	441.0
191.00	363.0
207.10	1923.0

Instrument :
BNA_M
ClientSampleId :
DFTPP20