

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020916\
 Data File : BM004218.D
 Acq On : 09 Feb 2016 11:37
 Operator : SJ/IZ
 Sample : H1340-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04J9

Quant Time: Feb 10 01:39:39 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 10 01:35:45 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	21780	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	109299	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.32	164	69374	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.07	188	168540	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	205075	20.00	ng/ul	0.00
86) Perylene-d12	23.51	264	186220	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	1453	3.53	ng/uL	0.00
5) Phenol-d5	6.83	99	42916	20.20	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	22428	19.83	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	37401	22.61	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	38746	21.25	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	18394	22.71	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	20292	22.57	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	38155	22.84	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	51255	24.10	ng/ul	0.00
44) Dimethylphthalate-d6	13.73	166	134827	22.59	ng/ul	0.00
47) Acenaphthylene-d8	14.00	160	167572	24.11	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	18019	15.08	ng/ul	0.00
58) Fluorene-d10	15.31	176	123410	24.10	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.45	200	13475	12.97	ng/ul	0.00
71) Anthracene-d10	17.17	188	203270	24.79	ng/ul	0.00
79) Pyrene-d10	19.47	212	241827	26.32	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.37	264	248784	25.61	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.77	163	49925	7.94	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020916\
Data File : BM004218.D
Acq On : 09 Feb 2016 11:37
Operator : SJ/IZ
Sample : H1340-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04J9

Quant Time: Feb 10 01:39:39 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 10 01:35:45 2016
Response via : Initial Calibration

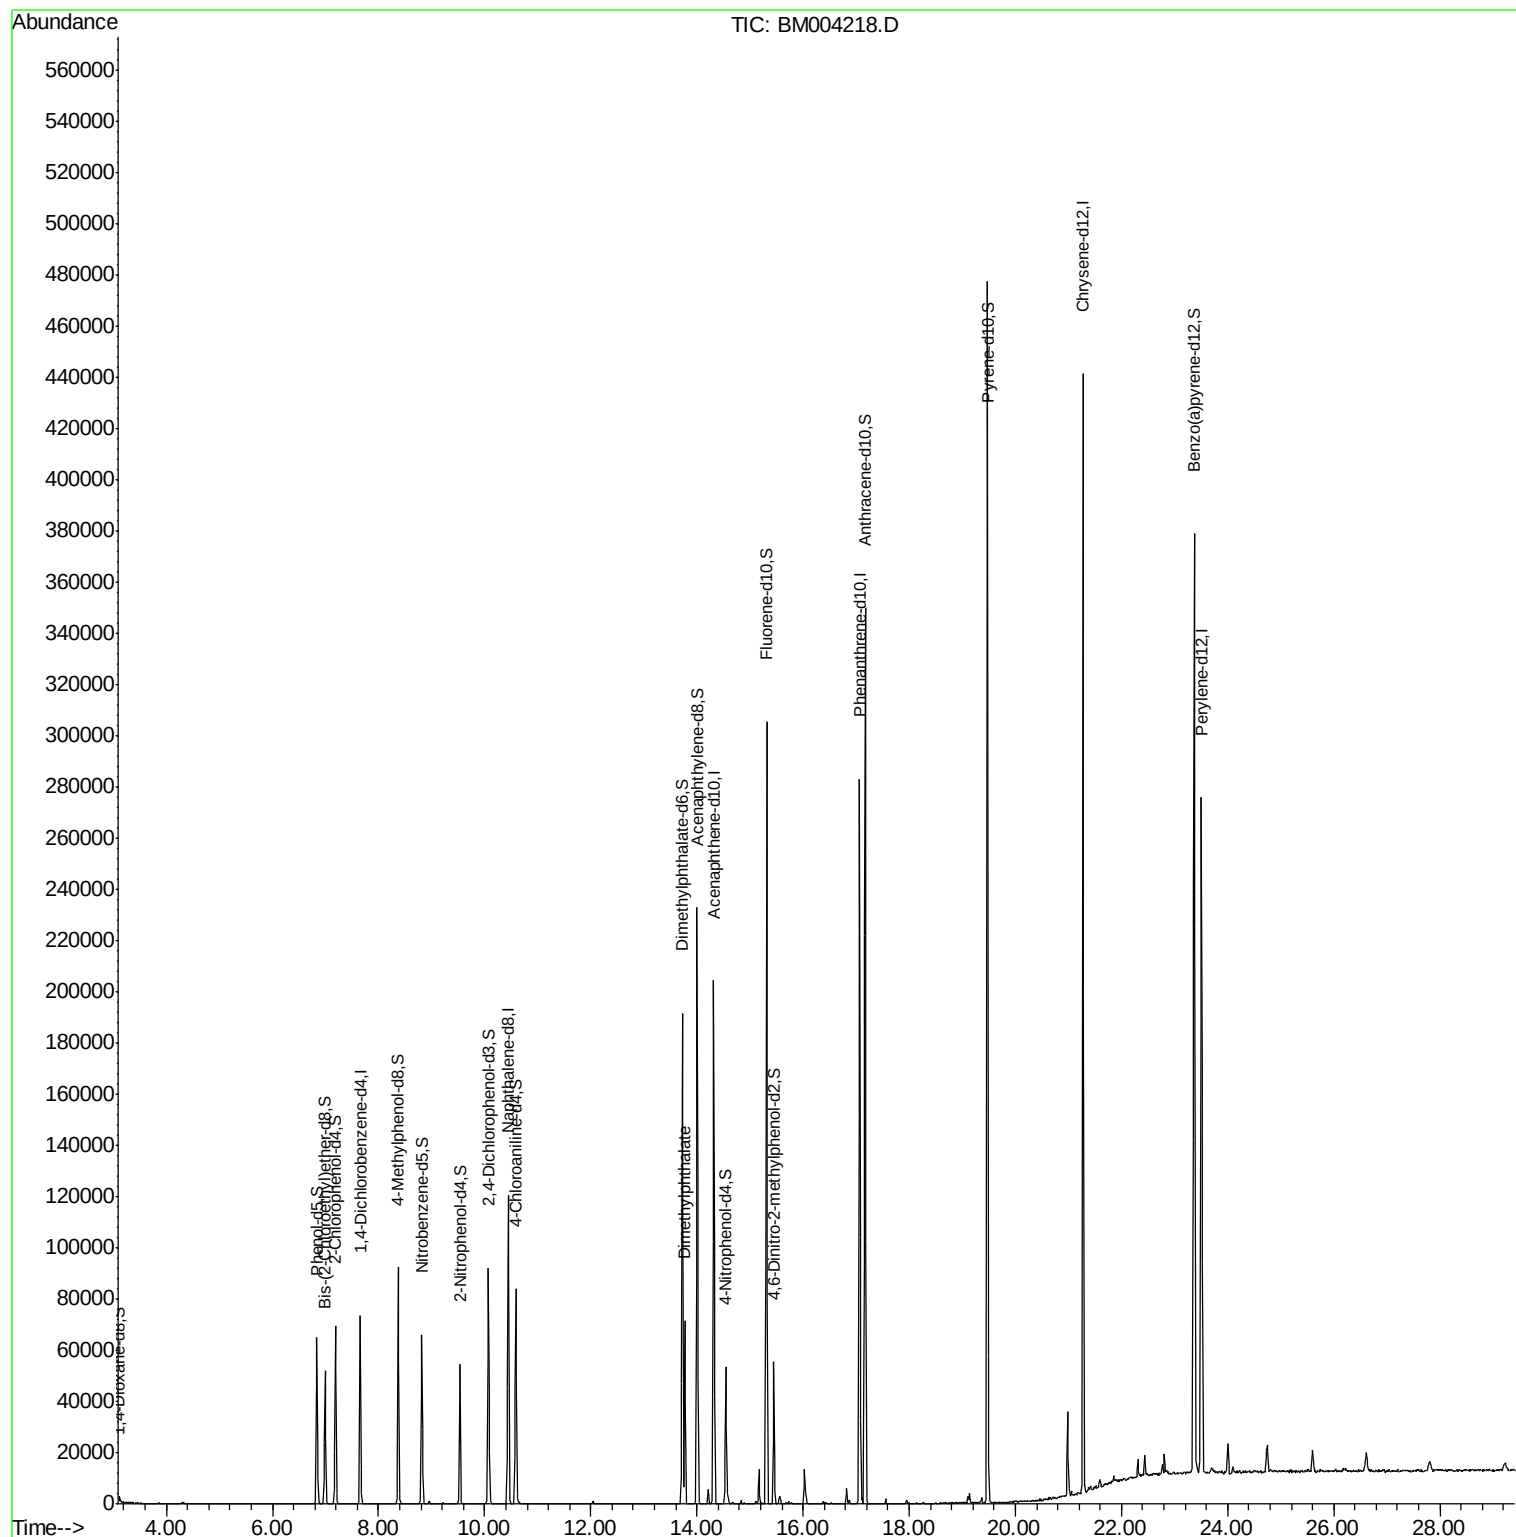

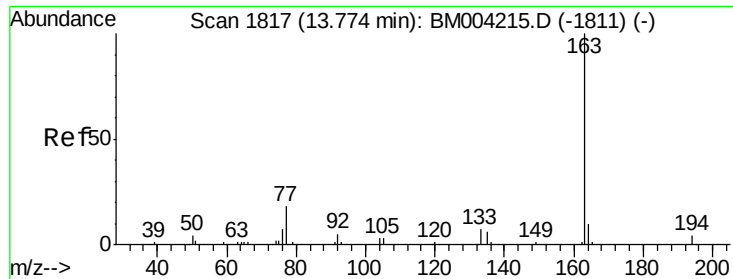

#45

Dimethylphthalate

Concen: 7.94 ng/ul

RT: 13.77 min Scan# 1816

Delta R.T. -0.01 min

Lab File: BM004218.D


Acq: 09 Feb 2016 11:37

Instrument :

BNA_M

ClientSampleId :

C04J9

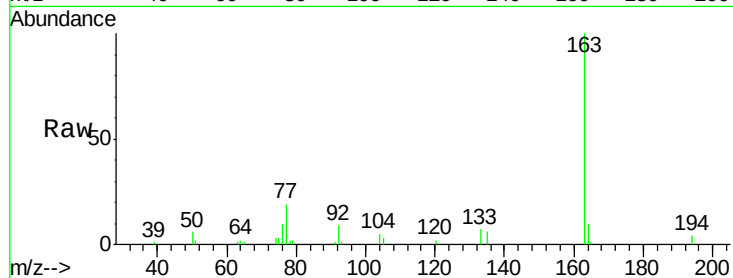


Tgt Ion:163 Resp: 49925

Ion Ratio Lower Upper

163 100

194 4.1 3.2 4.8

164 9.8 7.8 11.8

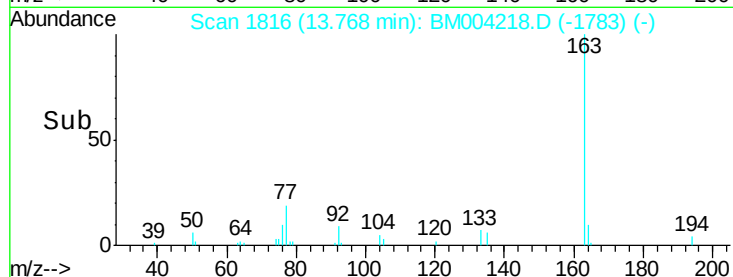

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

