

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020916\
 Data File : BM004220.D
 Acq On : 09 Feb 2016 12:49
 Operator : SJ/IZ
 Sample : H1340-21
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04K8

Manual Integrations
 APPROVED

Sohil
 2/10/2016 1:47:46 PM

Quant Time: Feb 10 02:54:45 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM012016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 10 01:35:45 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	21183	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	105604	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.32	164	67100	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.07	188	160811	20.00	ng/ul	0.00
78) Chrysene-d12	21.27	240	193772	20.00	ng/ul	0.00
86) Perylene-d12	23.51	264	176164	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	2296m	5.73	ng/uL	0.00
5) Phenol-d5	6.83	99	64391	31.16	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	34525	31.39	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	55349	34.40	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	57998	32.71	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	28796	36.79	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	32481	37.40	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	57026	35.32	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	86116	41.91	ng/ul	0.00
44) Dimethylphthalate-d6	13.73	166	199400	34.54	ng/ul	0.00
47) Acenaphthylene-d8	14.00	160	246211	36.63	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	31700	27.43	ng/ul	0.00
58) Fluorene-d10	15.31	176	177275	35.79	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.45	200	23954	24.17	ng/ul	0.00
71) Anthracene-d10	17.17	188	287798	36.79	ng/ul	0.00
79) Pyrene-d10	19.47	212	339150	39.07	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.37	264	351154	38.22	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.77	163	87804	14.44	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM020916\
Data File : BM004220.D
Acq On : 09 Feb 2016 12:49
Operator : SJ/IZ
Sample : H1340-21
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C04K8

Manual Integrations
APPROVED

Sohil
2/10/2016 1:47:46 PM

Quant Time: Feb 10 02:54:45 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM012016.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 10 01:35:45 2016
Response via : Initial Calibration

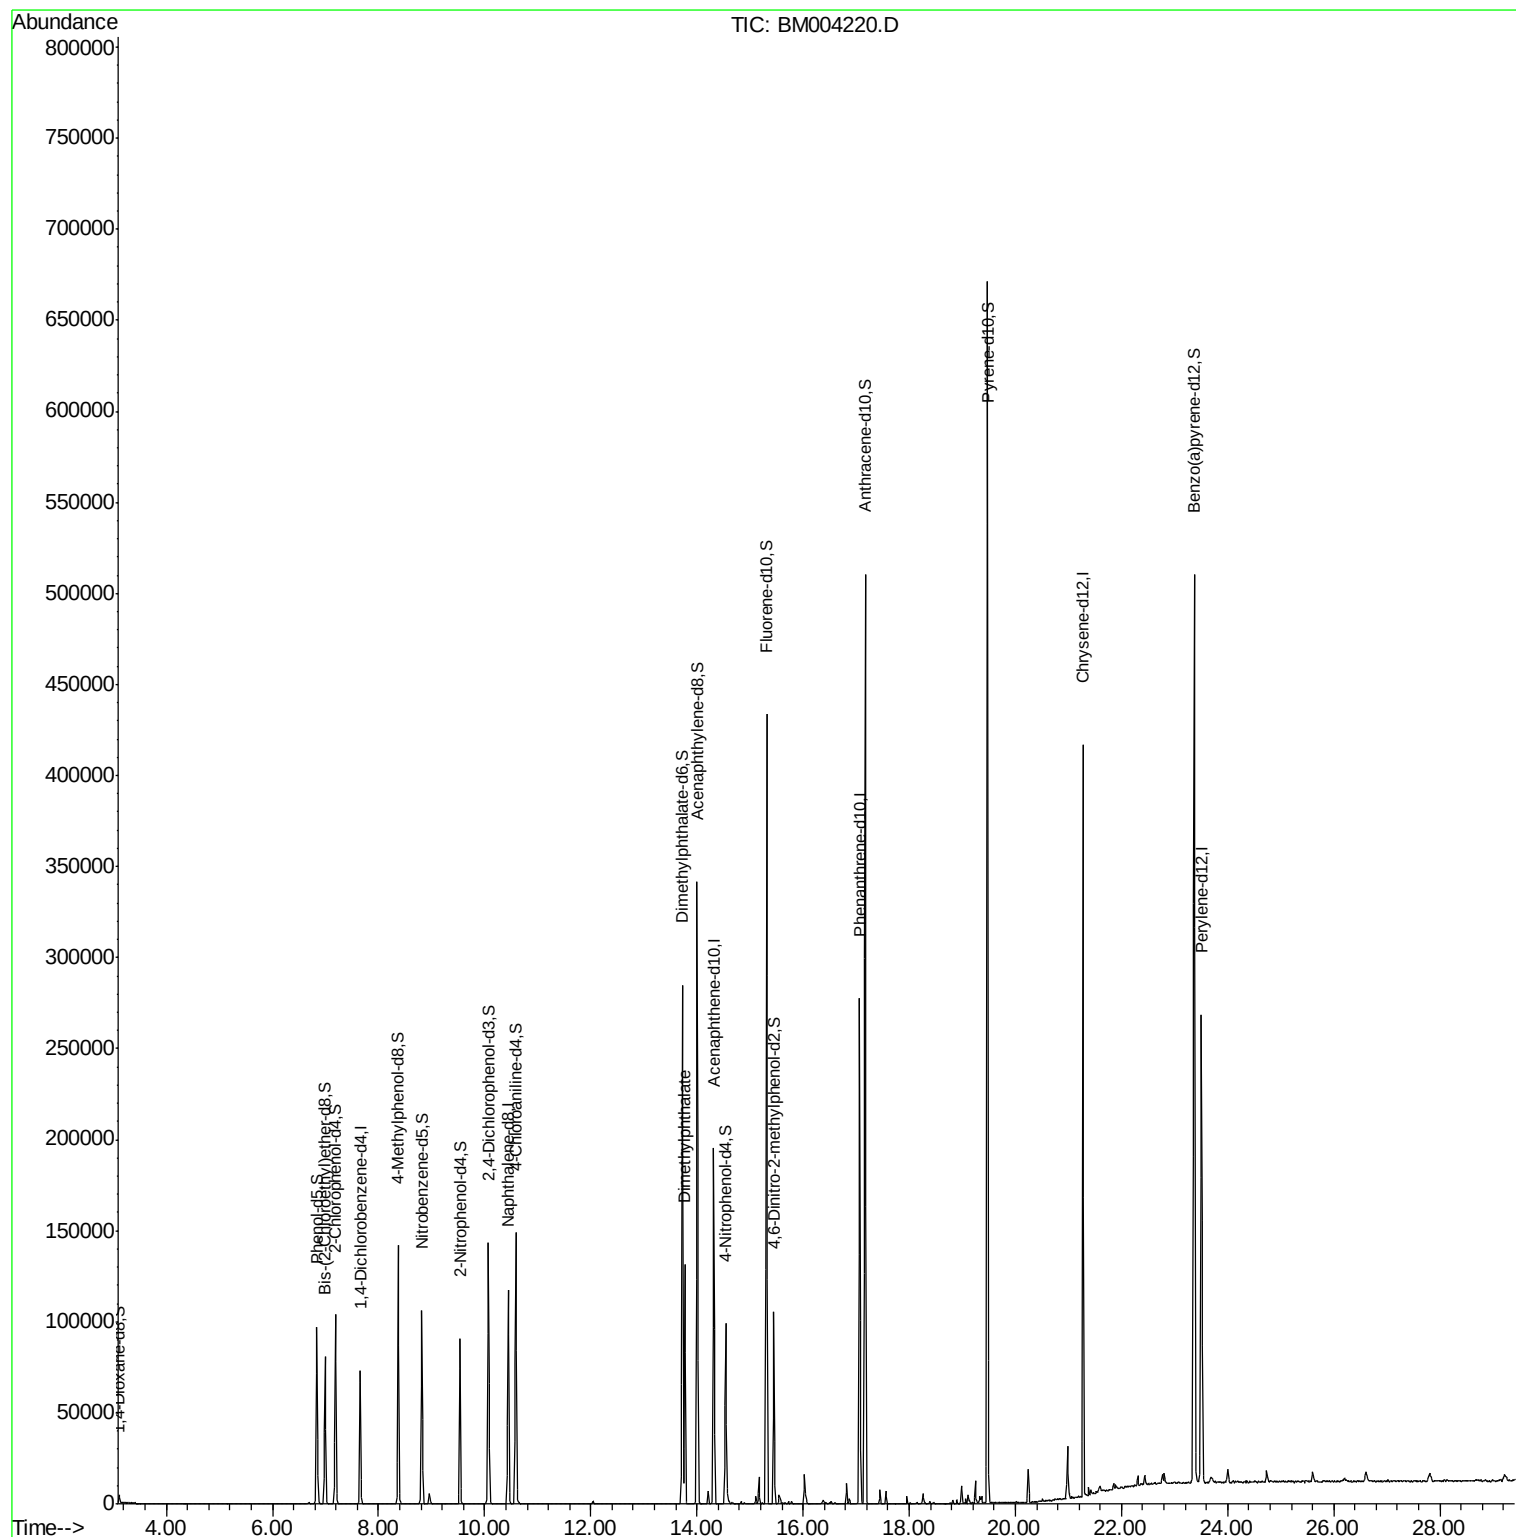

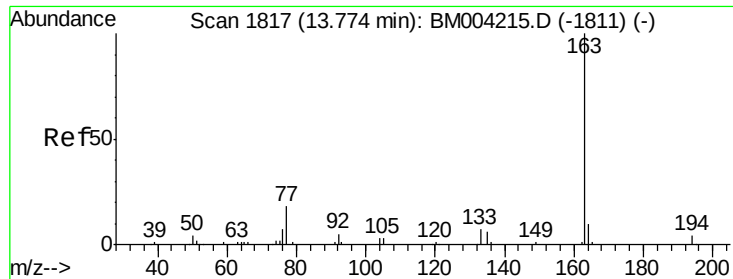


#45
 Dimethylphthalate
 Concen: 14.44 ng/ul
 RT: 13.77 min Scan# 1817
 Delta R.T. 0.00 min
 Lab File: BM004220.D
 Acq: 09 Feb 2016 12:49

Instrument :
 BNA_M
 ClientSampleId :
 C04K8

Tot Ion	Ratio	Resp	Lower	Upper
163	100	87804		
194	3.9		3.2	4.8
164	9.8		7.8	11.8

Manual Integrations
 APPROVED

Sohil
 2/10/2016 1:47:46 PM

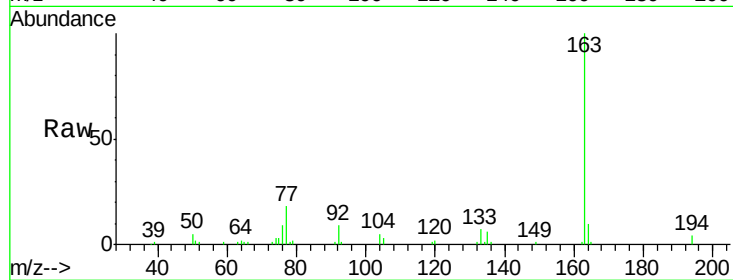

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

