

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020916\
 Data File : BM004218.D
 Acq On : 09 Feb 2016 11:37
 Operator : SJ/IZ
 Sample : H1340-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04J9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	3	5	13	rVB	2088	2568	0.40%	0.041%
2	6.834	632	637	647	rBB	64879	101488	15.94%	1.633%
3	6.992	659	664	672	rBB	51869	77286	12.14%	1.243%
4	7.192	692	698	705	rBB	69285	107640	16.91%	1.731%
5	7.657	771	777	784	rBB	73670	112647	17.70%	1.812%
6	8.369	893	898	908	rBB	92517	144401	22.68%	2.323%
7	8.816	968	974	982	rBB	65951	104596	16.43%	1.683%
8	8.957	995	998	1001	rBB	995	1340	0.21%	0.022%
9	9.533	1091	1096	1103	rBB	54728	82601	12.98%	1.329%
10	10.075	1182	1188	1198	rBB	92260	147710	23.20%	2.376%
11	10.445	1244	1251	1259	rBB	120729	200740	31.53%	3.229%
12	10.586	1269	1275	1289	rBB	83838	137827	21.65%	2.217%
13	12.045	1521	1523	1525	rBB	839	709	0.11%	0.011%
14	13.727	1803	1809	1813	rBV	191779	263406	41.38%	4.237%
15	13.768	1813	1816	1822	rVB	71538	94696	14.88%	1.523%
16	14.004	1850	1856	1866	rBB	232986	328020	51.53%	5.276%
17	14.210	1888	1891	1895	rBB	5708	6806	1.07%	0.109%
18	14.316	1903	1909	1915	rBB2	204422	301876	47.42%	4.856%
19	14.539	1943	1947	1959	rBV	53464	85568	13.44%	1.376%
20	14.833	1994	1997	1999	rBB	1560	1176	0.18%	0.019%
21	15.115	2042	2045	2049	rBB	1172	1267	0.20%	0.020%
22	15.168	2050	2054	2058	rBB	13322	15345	2.41%	0.247%
23	15.310	2073	2078	2085	rBB	305610	431941	67.85%	6.948%
24	15.451	2098	2102	2108	rBB	55575	69531	10.92%	1.118%
25	15.557	2116	2120	2126	rBB2	3283	6872	1.08%	0.111%
26	15.721	2146	2148	2150	rBB	1244	961	0.15%	0.015%
27	16.033	2197	2201	2204	rBV	13744	19002	2.99%	0.306%
28	16.374	2257	2259	2262	rBV	1222	1361	0.21%	0.022%
29	16.821	2332	2335	2339	rBV	5848	7293	1.15%	0.117%
30	16.874	2342	2344	2347	rVB	1300	1296	0.20%	0.021%
31	17.068	2371	2377	2382	rBV	283312	394638	61.99%	6.348%
32	17.109	2382	2384	2388	rVV	2292	2469	0.39%	0.040%
33	17.168	2388	2394	2404	rVB	349876	497699	78.18%	8.006%
34	17.562	2459	2461	2463	rBB	1856	1263	0.20%	0.020%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020916\
 Data File : BM004218.D
 Acq On : 09 Feb 2016 11:37
 Operator : SJ/IZ
 Sample : H1340-10
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04J9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
 Title : SVOA CALIBRATION

35	17.962	2527	2529	2531	rBB	1782	1034	0.16%	0.017%
36	18.268	2578	2581	2583	rBB	745	784	0.12%	0.013%
37	18.874	2681	2684	2687	rBV	388	764	0.12%	0.012%
38	19.103	2720	2723	2726	rBV	2581	3195	0.50%	0.051%
39	19.139	2726	2729	2733	rVB	3569	4124	0.65%	0.066%
40	19.362	2762	2767	2770	rBV	2019	2311	0.36%	0.037%
41	19.474	2780	2786	2794	rBV	477075	634721	99.71%	10.210%
42	20.633	2980	2983	2984	rVB	1079	917	0.14%	0.015%
43	20.703	2991	2995	2996	rBV	714	992	0.16%	0.016%
44	20.980	3039	3042	3051	rVB	32778	47005	7.38%	0.756%
45	21.050	3051	3054	3058	rBV	1755	2147	0.34%	0.035%
46	21.192	3075	3078	3080	rBV2	978	930	0.15%	0.015%
47	21.274	3087	3092	3097	rBV	437795	543539	85.38%	8.743%
48	21.315	3097	3099	3101	rVB	2781	2662	0.42%	0.043%
49	21.386	3109	3111	3113	rBV2	1405	1180	0.19%	0.019%
50	21.421	3115	3117	3120	rVB2	1410	1087	0.17%	0.017%
51	21.592	3142	3146	3152	rVB3	2860	6125	0.96%	0.099%
52	21.850	3188	3190	3194	rBV	2302	2310	0.36%	0.037%
53	22.309	3265	3268	3272	rBV2	6975	8241	1.29%	0.133%
54	22.439	3286	3290	3295	rBV	7521	9186	1.44%	0.148%
55	22.809	3350	3353	3357	rBV2	7433	8869	1.39%	0.143%
56	23.368	3441	3448	3456	rBV	365640	636581	100.00%	10.240%
57	23.509	3464	3472	3480	rBV	263898	481970	75.71%	7.753%
58	24.009	3552	3557	3562	rVB	11966	22555	3.54%	0.363%
59	24.750	3676	3683	3689	rBV2	10369	22366	3.51%	0.360%
60	25.603	3824	3828	3836	rVB4	8314	16995	2.67%	0.273%


Sum of corrected areas: 6216629

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020916\
Data File : BM004218.D
Acq On : 09 Feb 2016 11:37
Operator : SJ/IZ
Sample : H1340-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04J9

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM012016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

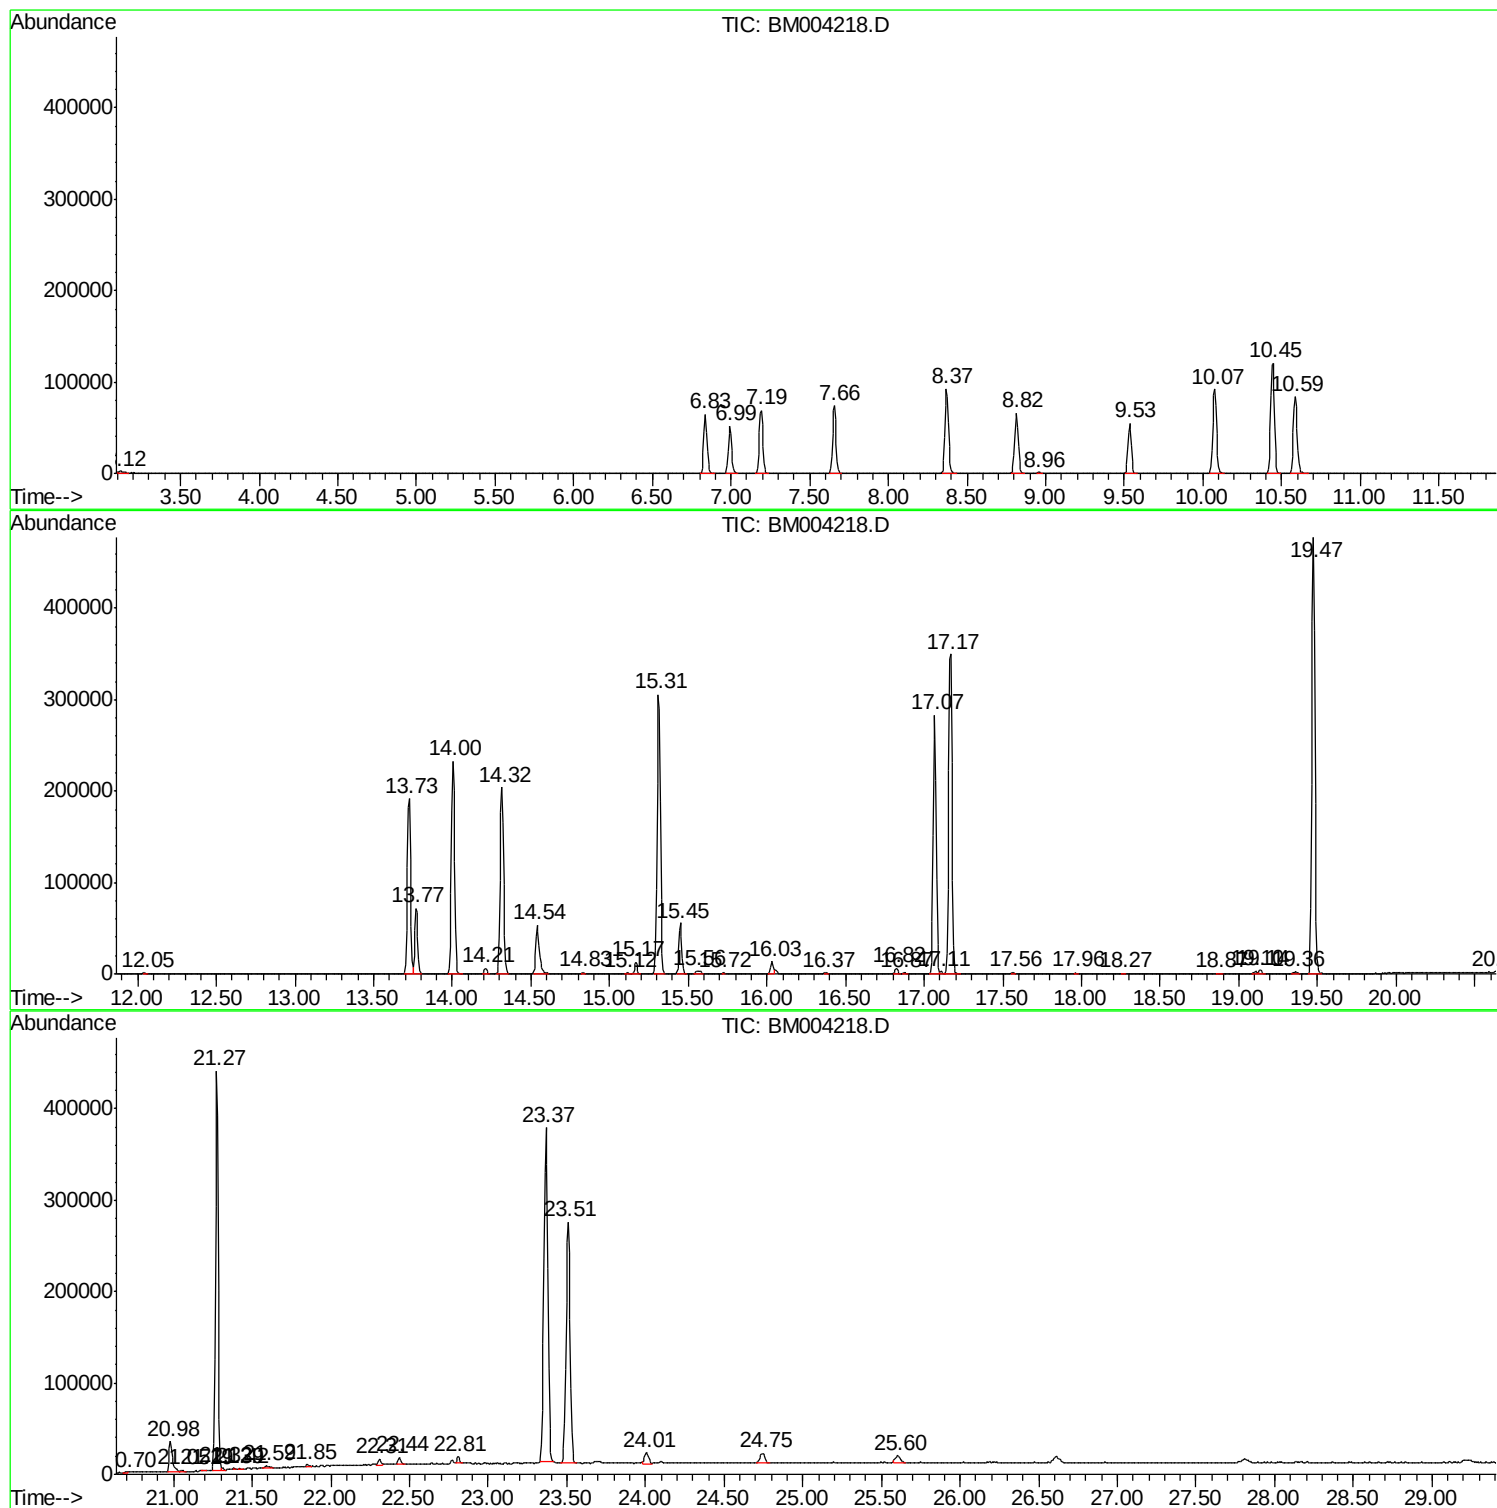

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020916\
Data File : BM004218.D
Acq On : 09 Feb 2016 11:37
Operator : SJ/IJ
Sample : H1340-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04J9

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020916\
Data File : BM004218.D
Acq On : 09 Feb 2016 11:37
Operator : SJ/IZ
Sample : H1340-10
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04J9

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc