

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020916\
 Data File : BM004220.D
 Acq On : 09 Feb 2016 12:49
 Operator : SJ/IZ
 Sample : H1340-21
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04K8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	3	5	10	rVB	3972	4035	0.45%	0.049%
2	6.687	610	612	617	rBB	772	1038	0.11%	0.013%
3	6.834	632	637	647	rBB	97302	156110	17.29%	1.902%
4	6.993	658	664	672	rBB	80958	121168	13.42%	1.476%
5	7.193	692	698	706	rBB	103863	165408	18.32%	2.015%
6	7.657	771	777	783	rBB	73021	110604	12.25%	1.347%
7	8.369	893	898	908	rBB	141858	223097	24.70%	2.718%
8	8.816	968	974	982	rBB	105974	165045	18.28%	2.010%
9	8.957	994	998	1006	rBB	5562	9792	1.08%	0.119%
10	9.534	1090	1096	1103	rBB	90540	139620	15.46%	1.701%
11	10.075	1182	1188	1198	rBB	143283	232146	25.71%	2.828%
12	10.445	1244	1251	1258	rBB	117679	194044	21.49%	2.364%
13	10.586	1269	1275	1290	rBB	148707	242057	26.80%	2.948%
14	12.039	1520	1522	1526	rBB	1281	1666	0.18%	0.020%
15	13.727	1803	1809	1813	rBV	285028	395177	43.76%	4.814%
16	13.774	1813	1817	1823	rVB	131477	172939	19.15%	2.107%
17	14.004	1850	1856	1866	rBV	341766	487168	53.95%	5.934%
18	14.210	1888	1891	1895	rBB	6836	7797	0.86%	0.095%
19	14.316	1903	1909	1915	rBB2	195363	289701	32.08%	3.529%
20	14.539	1942	1947	1962	rBB	98862	158109	17.51%	1.926%
21	14.833	1994	1997	1999	rBB	1672	1395	0.15%	0.017%
22	15.116	2041	2045	2049	rBB	4398	5411	0.60%	0.066%
23	15.168	2050	2054	2058	rBB	14647	16828	1.86%	0.205%
24	15.310	2072	2078	2085	rBB	433825	629313	69.69%	7.666%
25	15.451	2097	2102	2108	rBB	105671	132908	14.72%	1.619%
26	15.551	2116	2119	2122	rBV3	4944	6851	0.76%	0.083%
27	15.721	2146	2148	2151	rBB	1242	1235	0.14%	0.015%
28	15.792	2157	2160	2162	rBB	1207	970	0.11%	0.012%
29	16.033	2197	2201	2204	rBV	16181	21731	2.41%	0.265%
30	16.374	2256	2259	2263	rBV	1940	2766	0.31%	0.034%
31	16.821	2332	2335	2339	rBV	11634	13524	1.50%	0.165%
32	16.874	2339	2344	2348	rVB2	3197	4765	0.53%	0.058%
33	17.068	2371	2377	2382	rBV	277508	374353	41.45%	4.560%
34	17.104	2382	2383	2387	rVV	1242	1348	0.15%	0.016%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020916\
 Data File : BM004220.D
 Acq On : 09 Feb 2016 12:49
 Operator : SJ/IZ
 Sample : H1340-21
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C04K8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
 Title : SVOA CALIBRATION

35	17.168	2387	2394	2404	rVB	510722	716985	79.39%	8.734%
36	17.451	2439	2442	2448	rBB	7874	9614	1.06%	0.117%
37	17.562	2458	2461	2464	rBB	6850	7508	0.83%	0.091%
38	17.962	2526	2529	2532	rBB	3990	3663	0.41%	0.045%
39	18.145	2558	2560	2563	rBB	864	930	0.10%	0.011%
40	18.262	2576	2580	2584	rBV2	6005	8042	0.89%	0.098%
41	18.456	2611	2613	2616	rBB	1044	981	0.11%	0.012%
42	18.821	2671	2675	2678	rBB2	2078	3105	0.34%	0.038%
43	18.898	2685	2688	2692	rVB2	2297	2439	0.27%	0.030%
44	18.986	2699	2703	2709	rVB	9294	10330	1.14%	0.126%
45	19.062	2714	2716	2720	rVB	2207	2462	0.27%	0.030%
46	19.104	2720	2723	2727	rBV	4841	5794	0.64%	0.071%
47	19.139	2727	2729	2732	rVB	1808	1635	0.18%	0.020%
48	19.245	2743	2747	2755	rBV	12626	14726	1.63%	0.179%
49	19.333	2757	2762	2764	rVV	3530	4349	0.48%	0.053%
50	19.362	2764	2767	2771	rVB	3740	4036	0.45%	0.049%
51	19.474	2780	2786	2795	rBV2	670910	893438	98.93%	10.883%
52	20.239	2912	2916	2922	rBV	18432	33596	3.72%	0.409%
53	20.515	2961	2963	2965	rBV2	2019	1438	0.16%	0.018%
54	20.633	2980	2983	2987	rBV2	873	1230	0.14%	0.015%
55	20.980	3038	3042	3052	rBV	29061	39692	4.40%	0.483%
56	21.056	3052	3055	3056	rVV3	1180	1159	0.13%	0.014%
57	21.192	3075	3078	3079	rBV	1120	1091	0.12%	0.013%
58	21.274	3087	3092	3098	rBV	412796	508350	56.29%	6.192%
59	21.315	3098	3099	3102	rVB2	1292	1069	0.12%	0.013%
60	21.386	3108	3111	3113	rBV2	5210	4852	0.54%	0.059%
61	21.421	3113	3117	3119	rVV2	3014	3903	0.43%	0.048%
62	21.597	3140	3147	3152	rBV2	3659	9082	1.01%	0.111%
63	21.850	3187	3190	3194	rBV4	3494	4885	0.54%	0.060%
64	22.309	3264	3268	3271	rVB	5182	6228	0.69%	0.076%
65	22.439	3286	3290	3294	rBV	4764	6635	0.73%	0.081%
66	22.768	3344	3346	3350	rVV2	3682	4482	0.50%	0.055%
67	22.809	3350	3353	3357	rVB	4933	5716	0.63%	0.070%
68	23.368	3440	3448	3460	rVV	498322	903071	100.00%	11.000%
69	23.509	3464	3472	3481	rVB	257120	456151	50.51%	5.556%
70	24.003	3552	3556	3563	rVB	7270	12916	1.43%	0.157%
71	24.738	3678	3681	3687	rVB4	6126	11148	1.23%	0.136%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020916\
Data File : BM004220.D
Acq On : 09 Feb 2016 12:49
Operator : SJ/IZ
Sample : H1340-21
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04K8

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
Title : SVOA CALIBRATION

72	25.609	3823	3829	3834	rBV6	5366	12664	1.40%	0.154%
----	--------	------	------	------	------	------	-------	-------	--------


Sum of corrected areas: 8209514

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020916\
Data File : BM004220.D
Acq On : 09 Feb 2016 12:49
Operator : SJ/IZ
Sample : H1340-21
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04K8

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM012016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

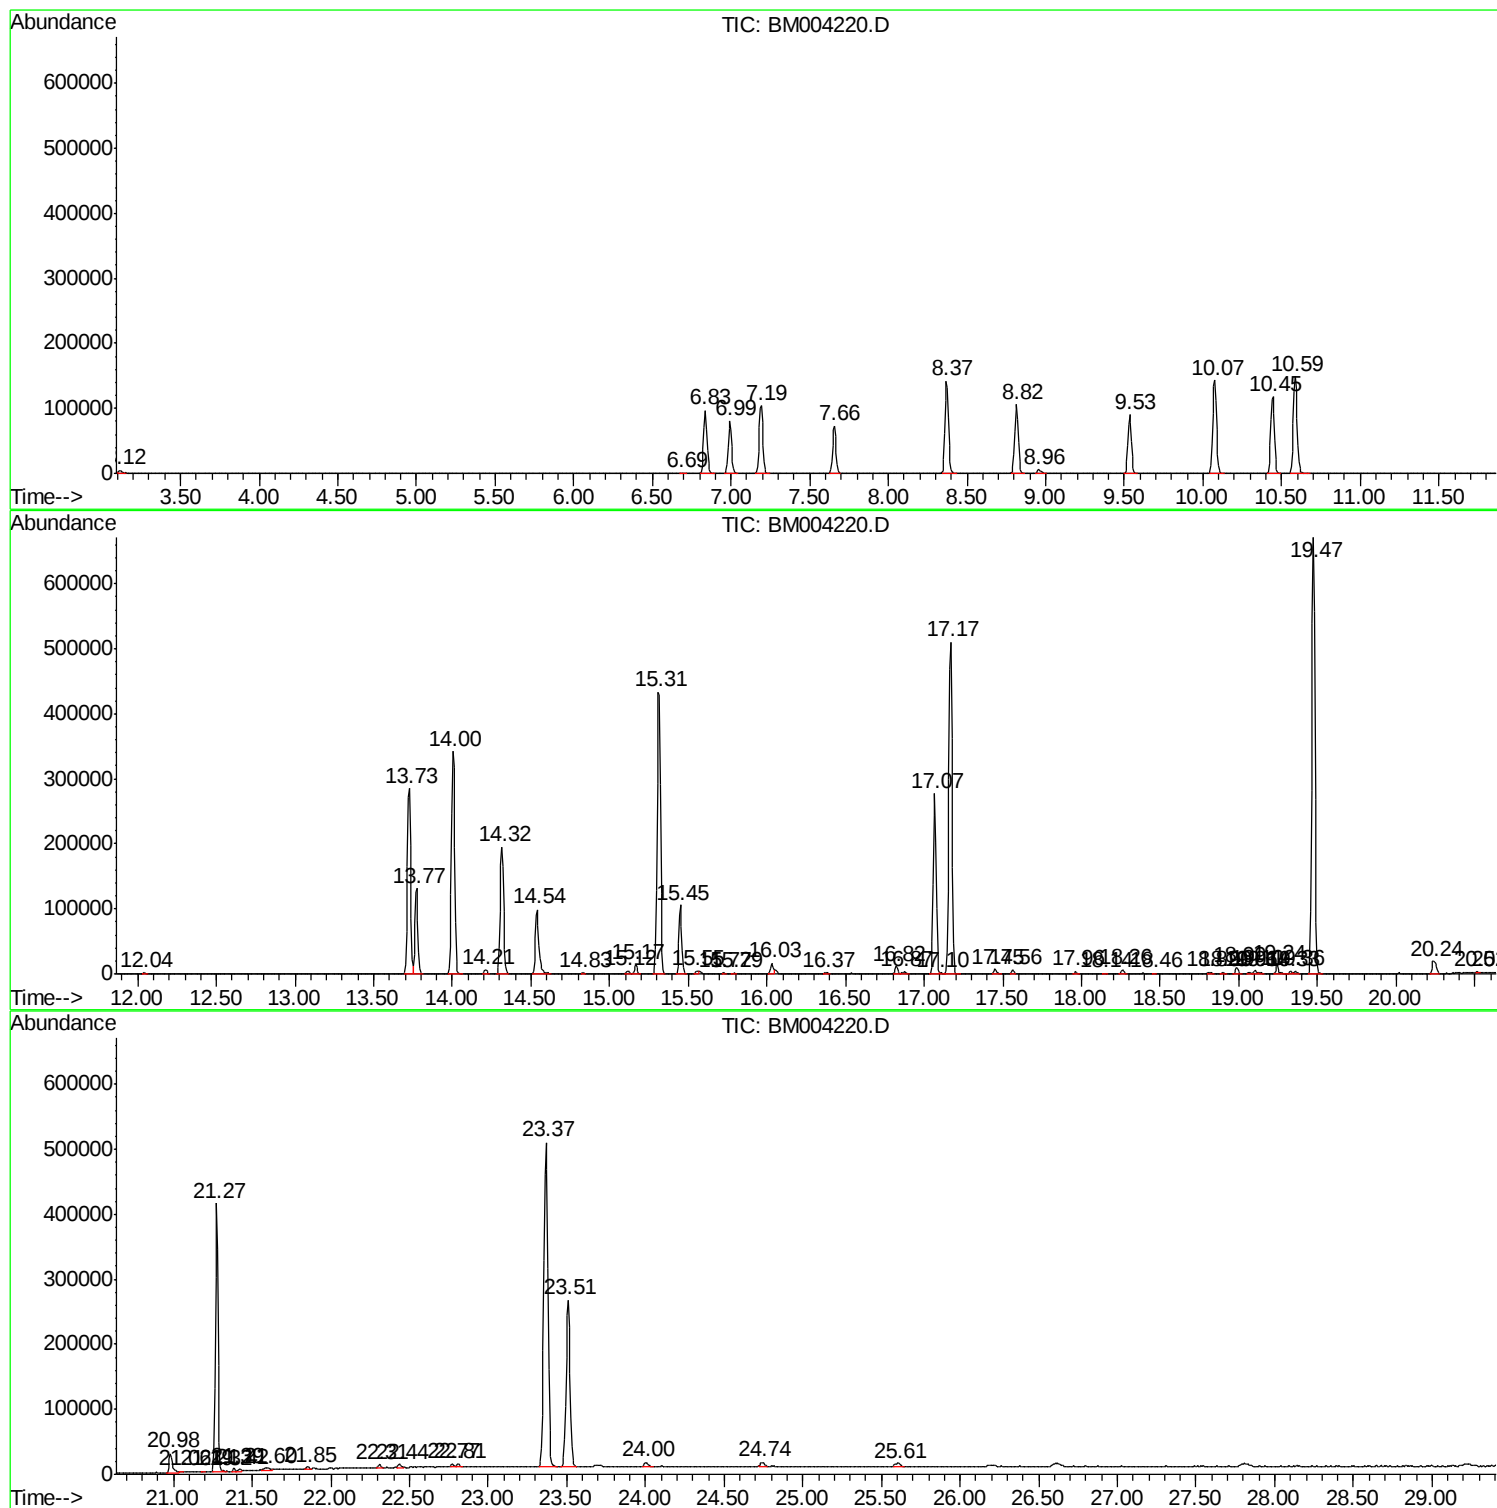

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020916\
Data File : BM004220.D
Acq On : 09 Feb 2016 12:49
Operator : SJ/IZ
Sample : H1340-21
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04K8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020916\
Data File : BM004220.D
Acq On : 09 Feb 2016 12:49
Operator : SJ/IZ
Sample : H1340-21
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C04K8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc