


Data Path : Z:\HPCHEM1\BNA M\DATA\BM020916\
Data File : BM004214.D
Acq On : 09 Feb 2016 09:03
Operator : SJ/IZ
Sample : DFTPP49
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP49

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM012016.M
Title : SVOA CALIBRATION
Last Update : Wed Feb 10 01:35:45 2016

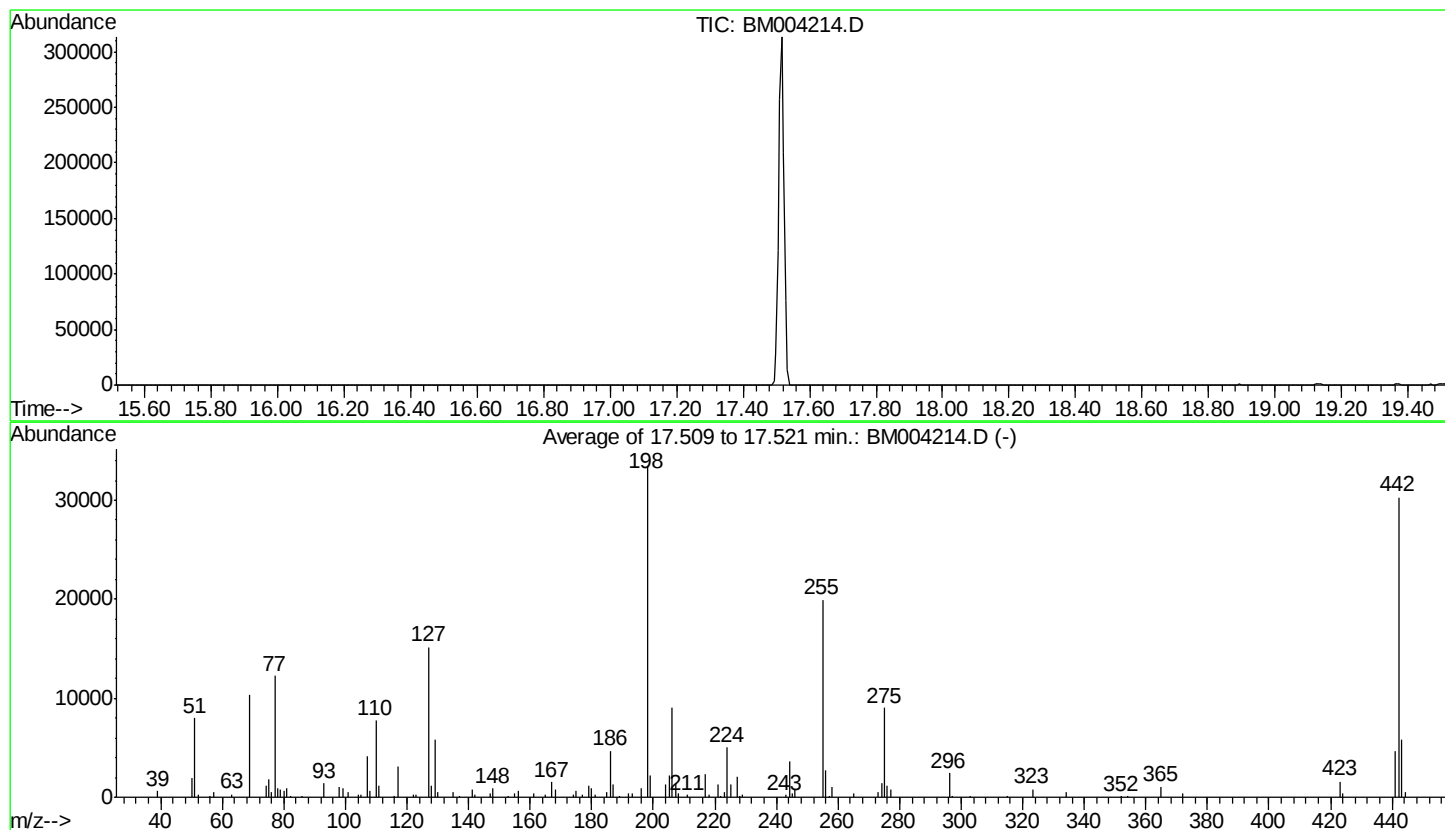

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.9	8015	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.8	10331	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.3	15178	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	33496	PASS
199	198	5	9	6.7	2233	PASS
275	198	10	60	26.9	9026	PASS
365	198	1	100	3.2	1072	PASS
441	443	0.01	100	78.2	4603	PASS
442	198	50	100	90.4	30272	PASS
443	442	15	24	19.4	5885	PASS

m/z	Abundance
39.10	739.0
50.10	2218.0
51.10	9060.0
52.10	434.0
57.00	651.0
63.00	420.0
69.00	11624.0
74.10	1329.0
75.00	1975.0
76.10	638.0
77.10	13674.0
78.10	926.0
79.00	920.0
80.00	616.0
81.00	1046.0
93.00	1569.0
98.00	1092.0
99.00	1100.0
101.00	524.0
104.00	378.0
105.00	390.0
107.00	4586.0
108.00	743.0
110.00	8260.0
111.00	1256.0
117.00	3421.0
121.90	321.0
123.00	417.0
127.10	16009.0
128.00	1251.0
129.00	6174.0
130.00	538.0
135.00	549.0
141.00	813.0
142.00	305.0
147.00	458.0
148.00	936.0
155.00	446.0
156.00	721.0
161.00	387.0
165.00	310.0
167.00	1538.0
168.00	917.0
174.00	365.0
175.10	682.0
177.00	319.0
179.00	1239.0
180.00	952.0
181.00	371.0
185.00	595.0
186.10	4784.0
187.00	1381.0
192.00	381.0
193.10	476.0
196.00	816.0
198.00	33752.0
199.00	2477.0
204.00	1227.0
205.10	2284.0
206.10	9051.0
207.10	1353.0
208.10	322.0
211.00	346.0
217.00	2403.0
218.00	310.0
221.10	1310.0
223.10	509.0
224.10	4979.0
225.10	1341.0
227.00	2089.0
229.00	385.0
243.00	338.0
244.10	3614.0
245.10	430.0
246.00	704.0
255.10	19416.0
256.10	2691.0
258.10	1030.0
265.00	395.0
273.10	528.0
274.10	1366.0
275.10	8215.0
276.10	1160.0
277.00	701.0
296.10	2273.0
323.10	719.0
334.10	444.0
365.00	840.0
372.00	350.0
423.10	1265.0
424.10	373.0
441.10	3534.0

Instrument :
BNA_M
ClientSampleId :
DFTPP49

442.20	23888.0
443.20	4681.0
444.10	432.0

Instrument :
BNA_M
ClientSampleId :
DFTPP49

m/z	Abundance
39.10	756.0
50.10	2374.0
51.10	9420.0
52.10	464.0
56.00	311.0
57.00	637.0
63.10	477.0
69.00	12390.0
74.10	1254.0
75.00	2073.0
76.10	675.0
77.10	14428.0
78.10	987.0
79.00	972.0
80.00	764.0
81.00	1132.0
82.00	315.0
86.00	349.0
93.00	1672.0
98.00	1254.0
99.00	1121.0
101.00	624.0
104.00	390.0
104.90	368.0
107.00	4953.0
108.00	744.0
110.00	9274.0
111.00	1490.0
116.00	324.0
117.00	3681.0
122.00	363.0
123.00	469.0
127.10	18088.0
128.00	1368.0
129.00	6781.0
130.00	524.0
135.00	599.0
137.10	314.0
141.00	971.0
142.00	302.0
147.00	562.0
148.00	1024.0
153.00	300.0
155.00	535.0
156.10	799.0
161.00	390.0
165.00	397.0
167.10	1910.0
168.00	946.0
174.00	443.0
175.00	742.0
177.10	315.0
179.00	1479.0
180.00	1094.0
181.00	439.0
185.00	673.0
186.10	5495.0
187.10	1613.0
189.00	361.0
192.10	469.0
193.00	505.0
196.00	1194.0
198.00	40168.0
199.00	2493.0
204.10	1469.0
205.10	2550.0
206.10	10947.0
207.10	1662.0
208.10	406.0
211.10	354.0
217.00	2833.0
218.00	395.0
221.10	1487.0
221.80	373.0
223.00	622.0
224.10	5903.0
225.10	1518.0
227.10	2464.0
228.10	376.0
229.10	551.0
243.00	301.0
244.10	4307.0
245.10	523.0
246.10	914.0
255.10	23576.0
256.10	3264.0
257.10	304.0
258.00	1330.0
265.10	453.0
273.00	692.0
274.10	1797.0
275.10	11005.0

Instrument :
BNA_M
ClientSampleId :
DFTPP49

276.10	1450.0
277.10	982.0
296.10	2865.0
297.10	432.0
303.00	328.0
315.00	324.0
323.10	929.0
334.10	629.0
352.10	307.0
354.10	330.0
365.10	1299.0
372.10	576.0
423.10	1844.0
424.10	446.0
441.10	5499.0
442.20	35352.0
443.10	6989.0
444.10	682.0

Instrument :
BNA_M
ClientSampleId :
DFTPP49

m/z	Abundance
39.00	372.0
50.10	1308.0
51.10	5565.0
57.00	425.0
69.00	6981.0
74.00	771.0
75.00	1245.0
76.10	404.0
77.10	8687.0
78.00	628.0
79.00	488.0
80.00	421.0
81.00	656.0
93.00	1008.0
98.00	738.0
99.00	662.0
101.00	419.0
107.00	3045.0
108.00	461.0
110.00	5669.0
111.00	876.0
117.00	2332.0
127.10	11437.0
128.00	792.0
129.00	4371.0
130.00	350.0
135.00	340.0
140.90	527.0
147.00	349.0
148.00	658.0
155.00	349.0
156.00	499.0
161.00	336.0
167.00	1132.0
168.00	657.0
175.00	491.0
179.00	906.0
180.00	727.0
185.00	488.0
186.10	3692.0
187.10	1047.0
192.00	337.0
193.10	339.0
196.00	750.0
198.00	26568.0
199.00	1729.0
204.00	1020.0
205.10	1794.0
206.10	7312.0
207.10	1100.0
208.00	324.0
217.00	1881.0
221.10	1086.0
223.00	399.0
224.10	4155.0
225.10	1058.0
227.10	1665.0
244.10	2992.0
245.10	361.0
246.00	604.0
255.10	16824.0
256.10	2373.0
258.00	920.0
265.00	358.0
273.10	513.0
274.10	1310.0
275.10	7860.0
276.00	1016.0
277.00	727.0
296.10	2155.0
323.10	704.0
334.10	514.0
365.00	1077.0
372.00	429.0
423.10	1574.0
424.10	400.0
441.10	4778.0
442.20	31576.0
443.10	5985.0
444.10	516.0

Instrument :
BNA_M
ClientSampleId :
DFTPP49

m/z

Abundance

Instrument :

BNA_M

ClientSampleId :

DFTPP49