
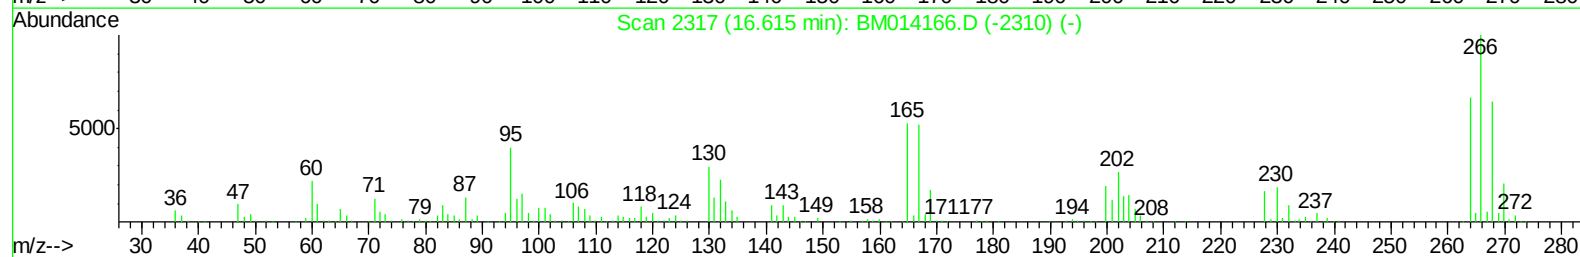
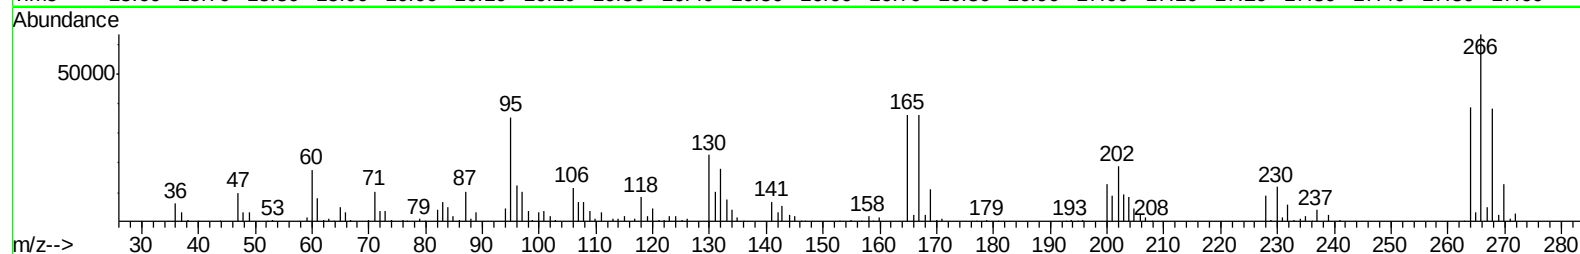


Data Path : Z:\HPCHEM1\BNA M\DATA\BM020918\
Data File : BM014208.D
Acq On : 09 Feb 2018 09:22
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 10 03:03:16 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 07 17:16:49 2018
Response via : Initial Calibration

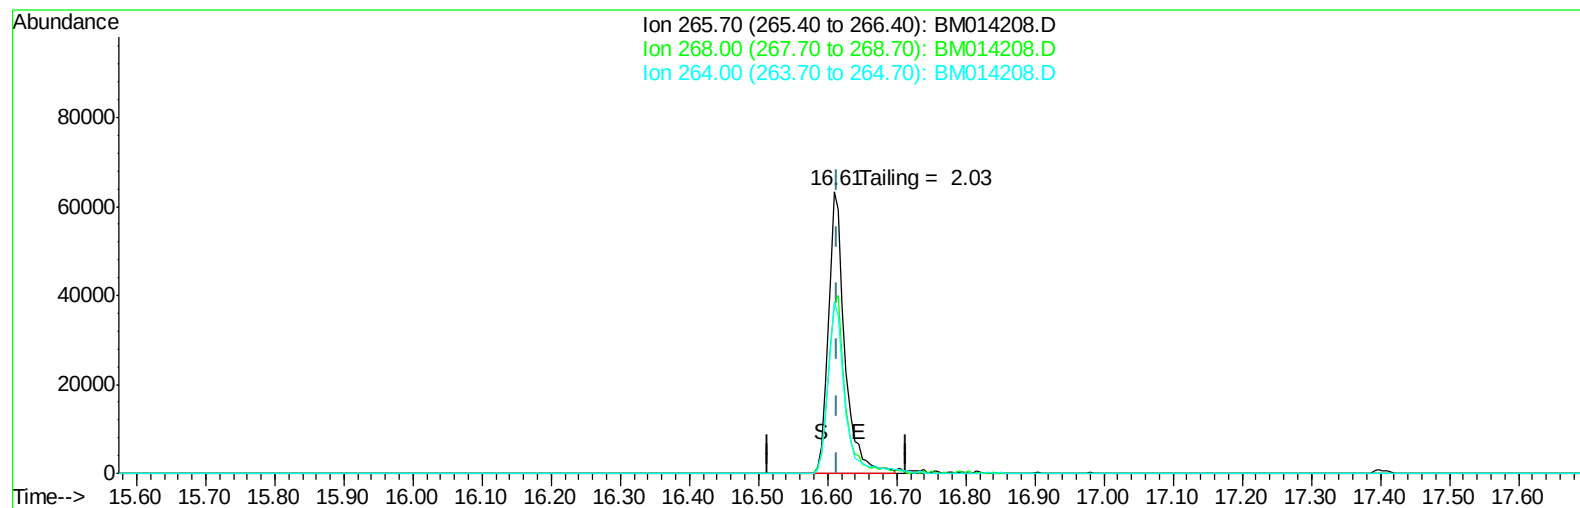

TIC: BM014208.D

(69) Pentachlorophenol (C)




16.609min (-0.006) 0.00ng

response 104075

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	60.21
264.00	61.20	61.10
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020918\
 Data File : BM014208.D
 Acq On : 09 Feb 2018 09:22
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 10 03:03:16 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM020718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 07 17:16:49 2018
 Response via : Initial Calibration

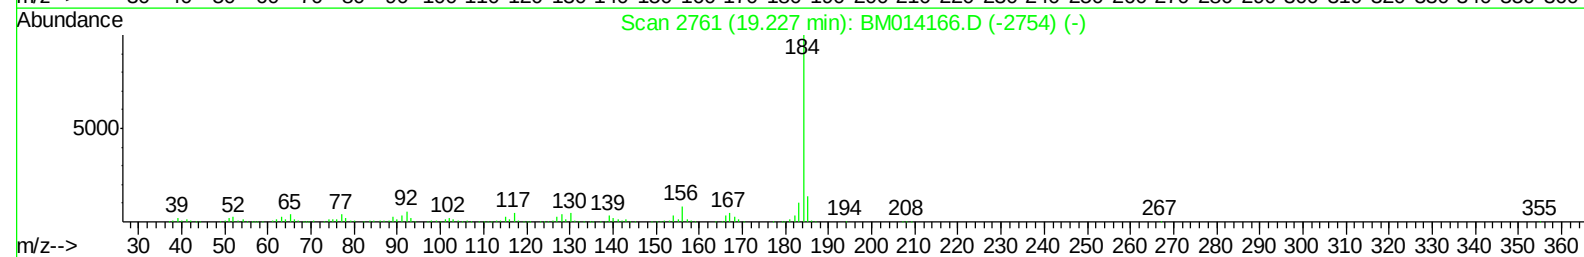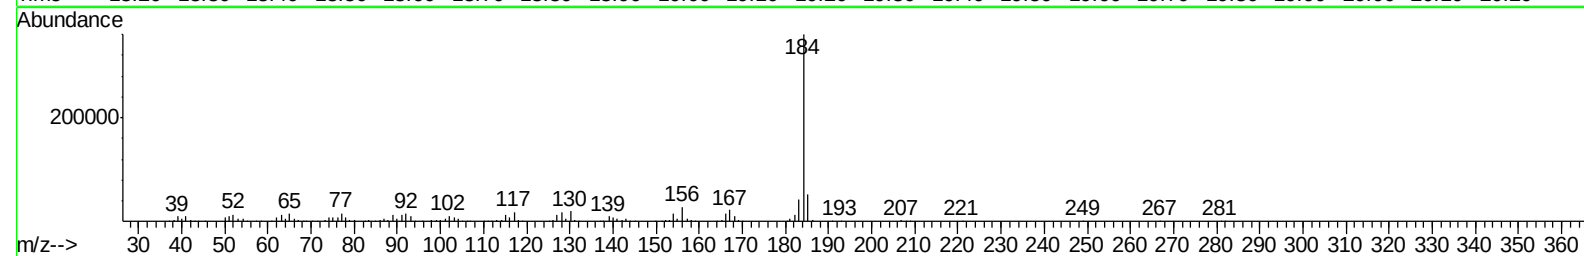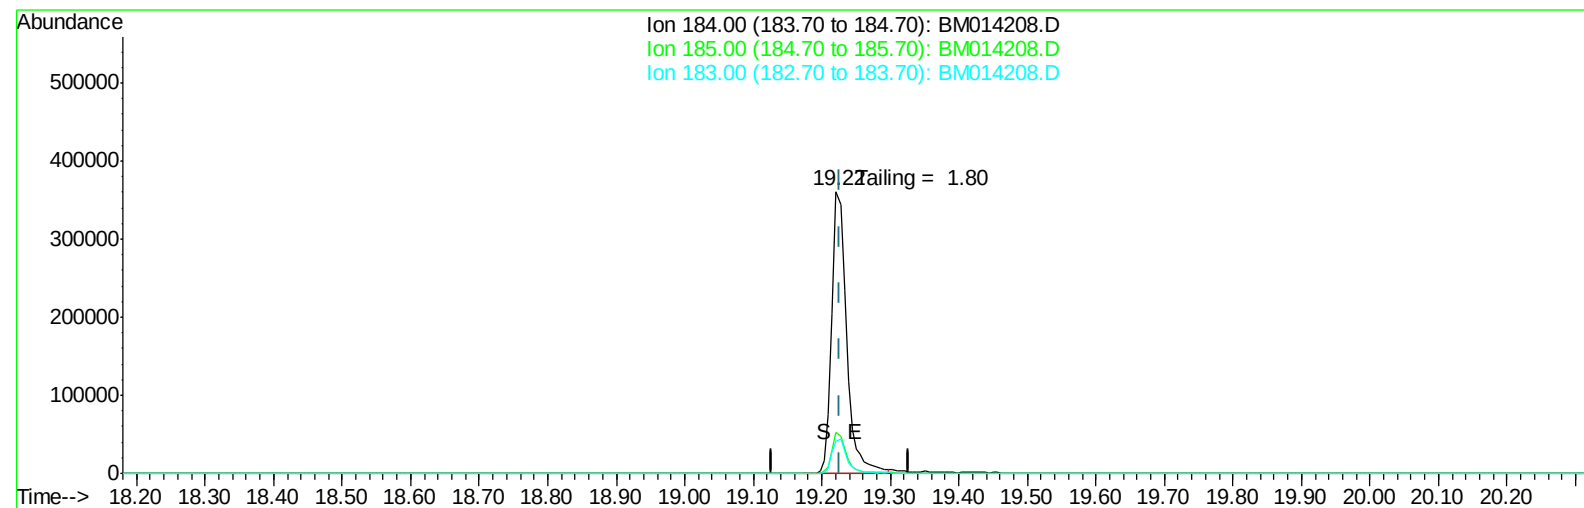

TIC: BM014208.D

(76) Benzidine

19.221min (-0.006) 169112.12ng

response 543924

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.51
183.00	11.10	11.52
0.00	0.00	0.00