

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020918\
 Data File : BM014210.D
 Acq On : 09 Feb 2018 10:34
 Operator : SJ/JU
 Sample : PB106402BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB106402BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM020718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.163	364	370	387	rBV	2204969	3080532	45.13%	8.398%
2	6.734	630	637	652	rBV	2218868	3382324	49.55%	9.221%
3	7.075	688	695	707	rBV	2318967	3562955	52.19%	9.713%
4	7.540	767	774	787	rVB	417312	675509	9.90%	1.842%
5	7.851	820	827	841	rVB	1682020	2688153	39.38%	7.328%
6	8.698	964	971	988	rBV	1189791	2116109	31.00%	5.769%
7	10.310	1236	1245	1262	rBV	417517	847081	12.41%	2.309%
8	12.804	1662	1669	1691	rBV	3275247	4902314	71.82%	13.365%
9	14.198	1900	1906	1924	rBV2	667279	1161715	17.02%	3.167%
10	15.698	2153	2161	2183	rBV	2493232	3786168	55.46%	10.322%
11	16.957	2367	2375	2389	rBV	788151	1342044	19.66%	3.659%
12	19.598	2818	2824	2836	rBV	5630306	6826268	100.00%	18.610%
13	21.162	3084	3090	3099	rBV	871211	1305690	19.13%	3.560%
14	23.333	3454	3459	3469	rBV	487663	1004088	14.71%	2.737%


Sum of corrected areas: 36680950

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020918\
Data File : BM014210.D
Acq On : 09 Feb 2018 10:34
Operator : SJ/JU
Sample : PB106402BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB106402BL

Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

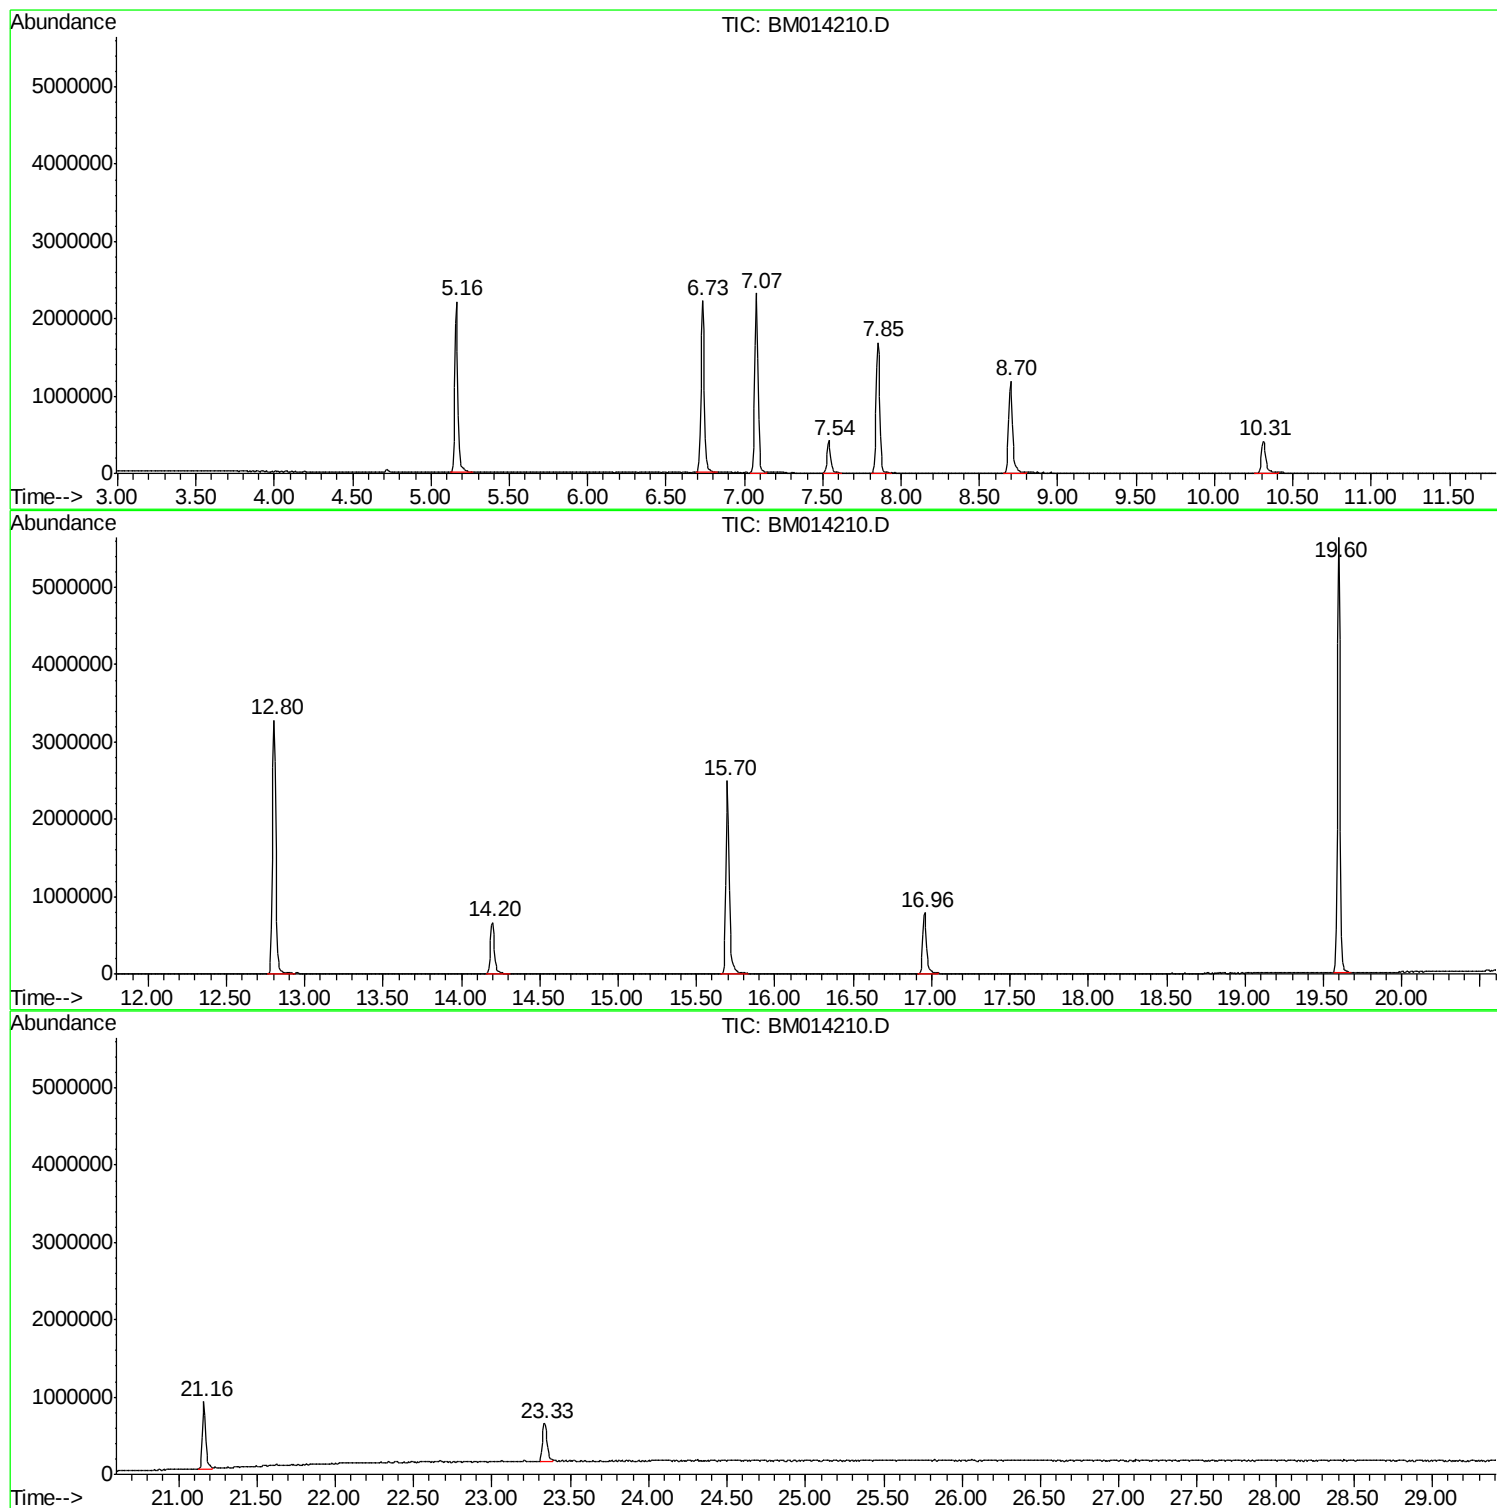

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020918\
Data File : BM014210.D
Acq On : 09 Feb 2018 10:34
Operator : SJ/JU
Sample : PB106402BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB106402BL










Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.07 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.07	105.49 ng	3562960	1,4-Dichlorobenzene-d4	7.54

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	16
2		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	14
3		3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	14
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	14
5		Benzene, 1,2,4-trifluoro-	132	C6H3F3	000367-23-7	10

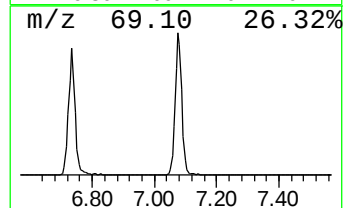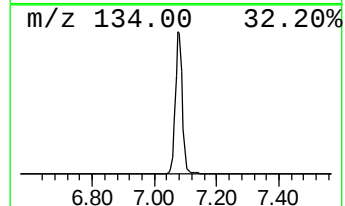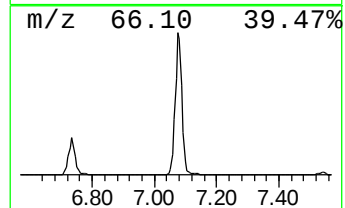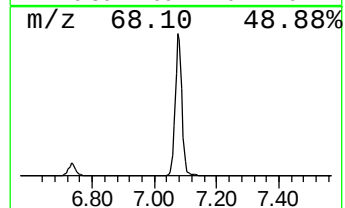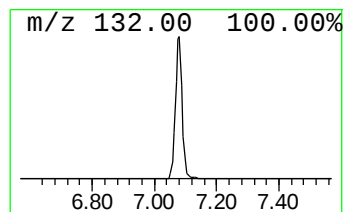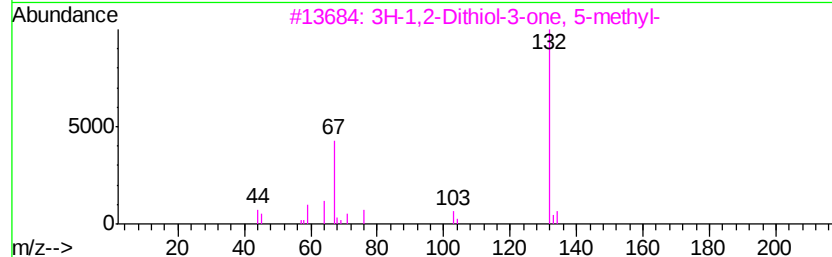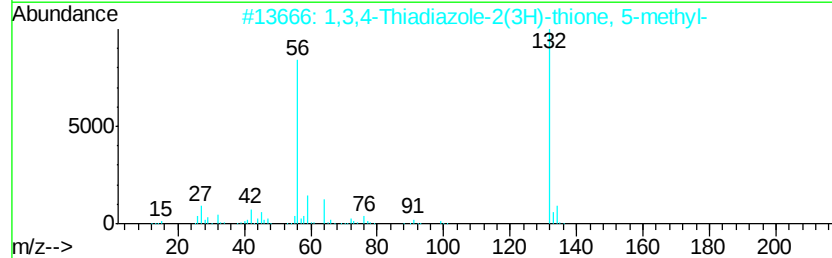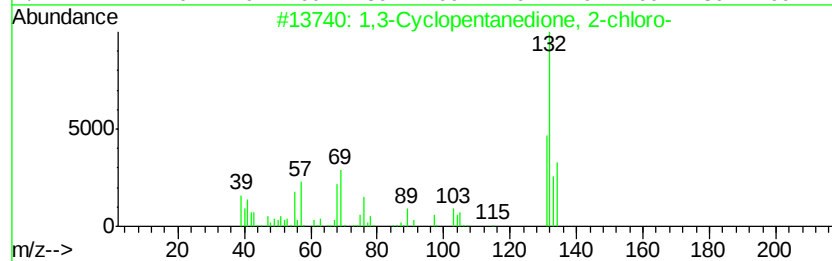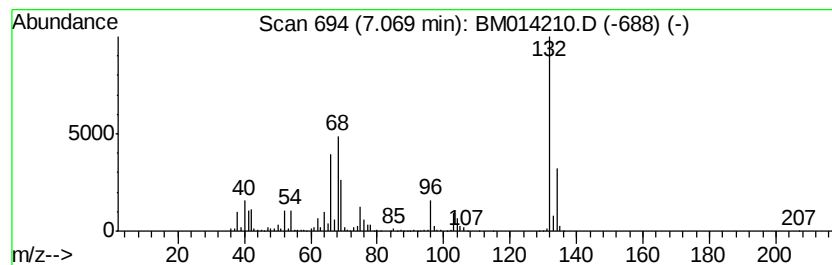

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020918\
Data File : BM014210.D
Acq On : 09 Feb 2018 10:34
Operator : SJ/JU
Sample : PB106402BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB106402BL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.07	7.07	105.5	ng	3562960	1	7.54	675509	20.0