

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020918\
Data File : BM014211.D
Acq On : 09 Feb 2018 11:46
Operator : SJ/JU
Sample : PB106384BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB106384BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM020718.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.163	364	370	385	rBV	2060317	2893313	45.87%	8.470%
2	6.734	630	637	654	rBV	2027662	3133378	49.67%	9.172%
3	7.081	688	696	707	rBV	2169577	3334449	52.86%	9.761%
4	7.539	768	774	784	rBV	392665	630210	9.99%	1.845%
5	7.851	820	827	837	rBV	1588418	2519508	39.94%	7.375%
6	8.698	964	971	987	rBV	1165101	1989112	31.53%	5.823%
7	10.310	1238	1245	1260	rBV	403083	768436	12.18%	2.249%
8	12.804	1662	1669	1680	rBV	2936727	4430673	70.24%	12.970%
9	14.198	1899	1906	1923	rBV2	610385	1056054	16.74%	3.091%
10	15.698	2155	2161	2174	rBV	2384387	3526289	55.90%	10.323%
11	16.956	2369	2375	2385	rBV2	735078	1228218	19.47%	3.595%
12	19.598	2818	2824	2835	rBV	5264682	6307974	100.00%	18.465%
13	21.162	3085	3090	3103	rBV2	835975	1264308	20.04%	3.701%
14	23.338	3453	3460	3475	rBV	506234	1079008	17.11%	3.159%


Sum of corrected areas: 34160930

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020918\
Data File : BM014211.D
Acq On : 09 Feb 2018 11:46
Operator : SJ/JU
Sample : PB106384BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB106384BL

Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

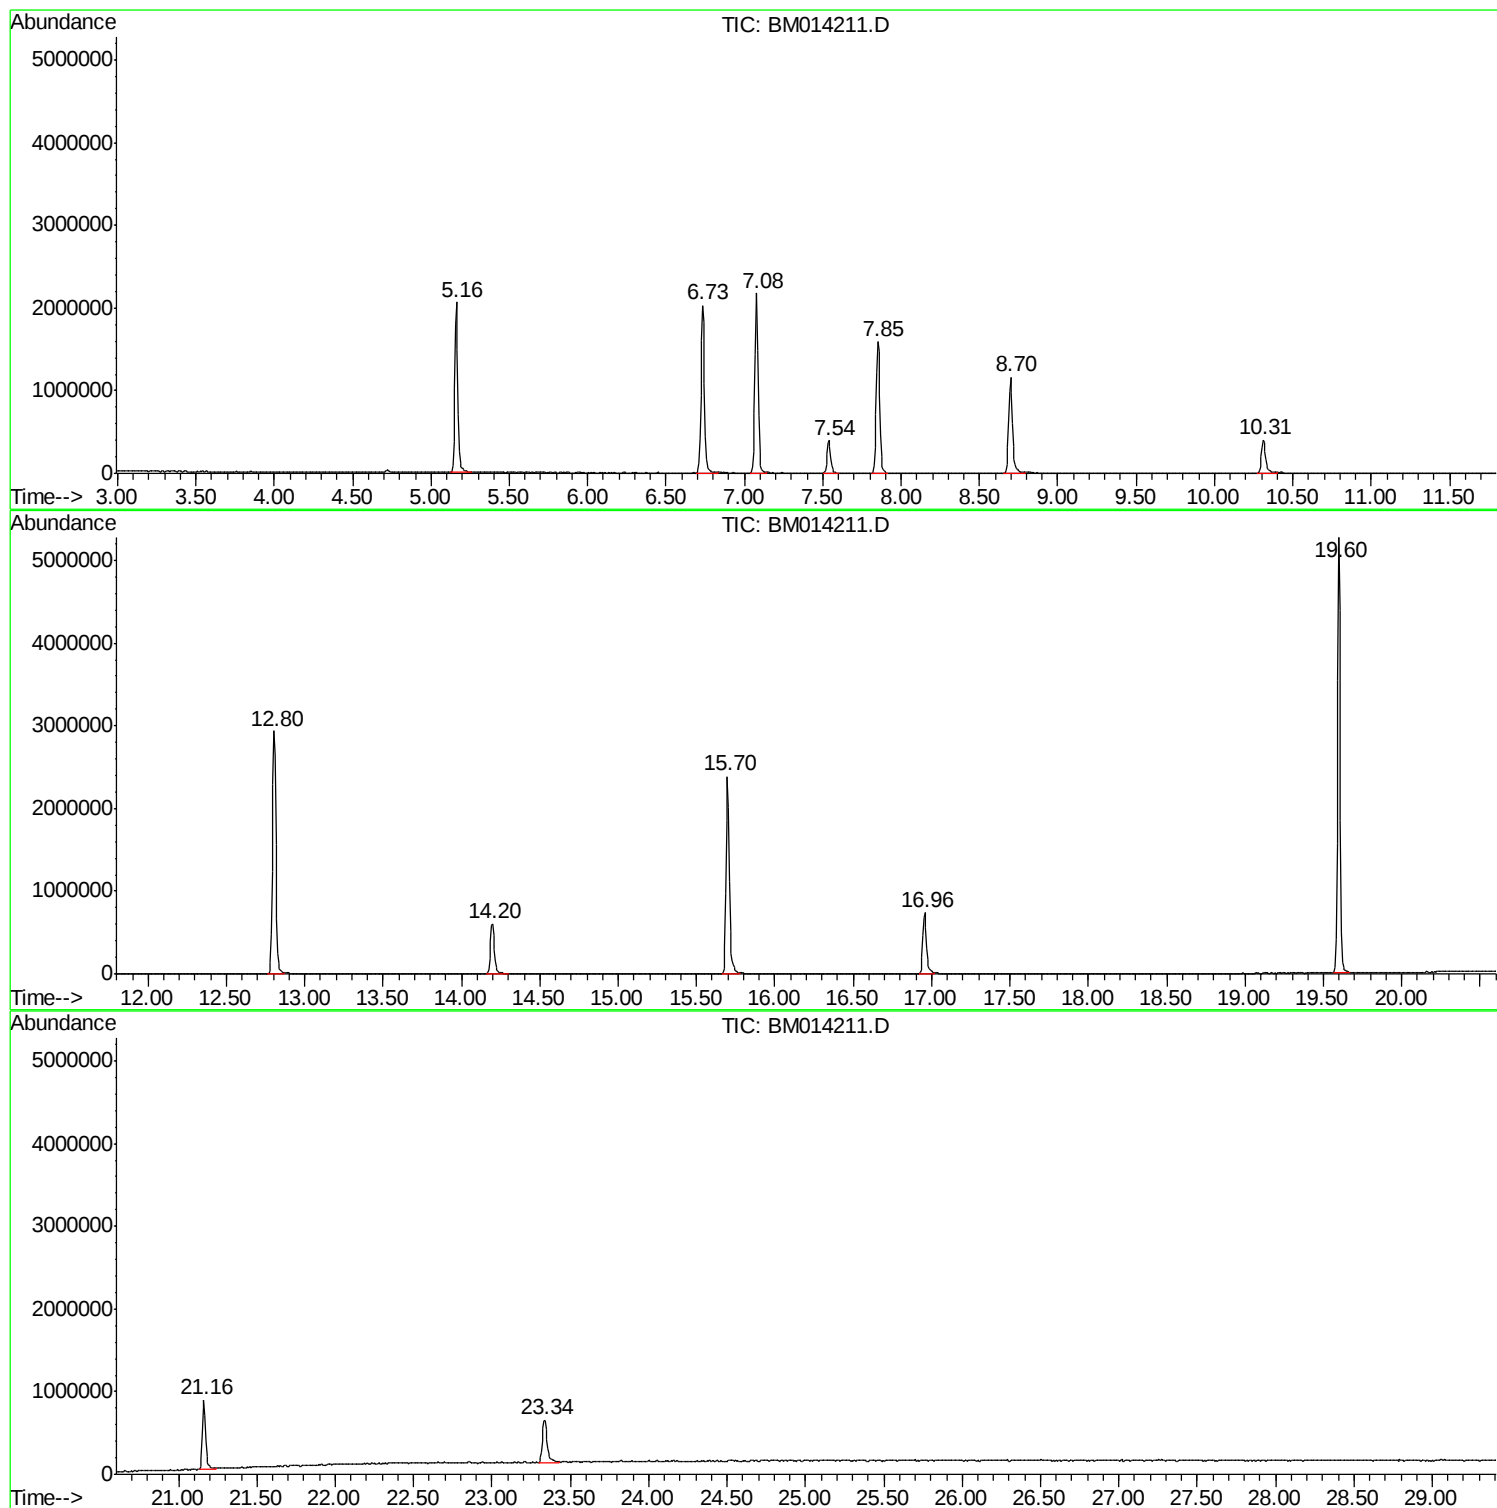

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020918\
Data File : BM014211.D
Acq On : 09 Feb 2018 11:46
Operator : SJ/JU
Sample : PB106384BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB106384BL










Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.08 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.08	105.82 ng	3334450	1,4-Dichlorobenzene-d4	7.54

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	16
2		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	14
3		3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	10
4		Pyrazolo(2,3-a)pyridine, 7-methyl-	132	C8H8N2	034760-58-2	10
5		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9

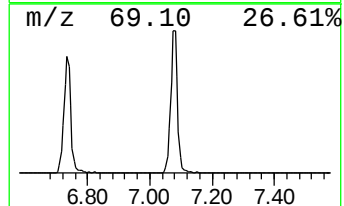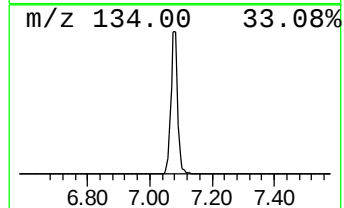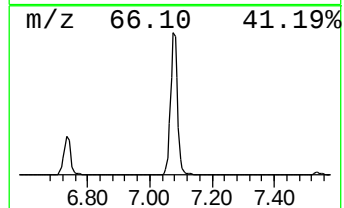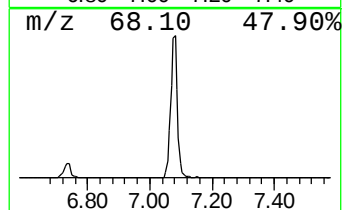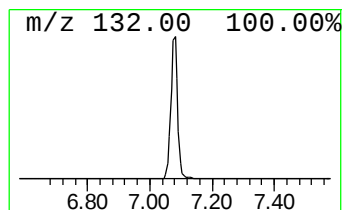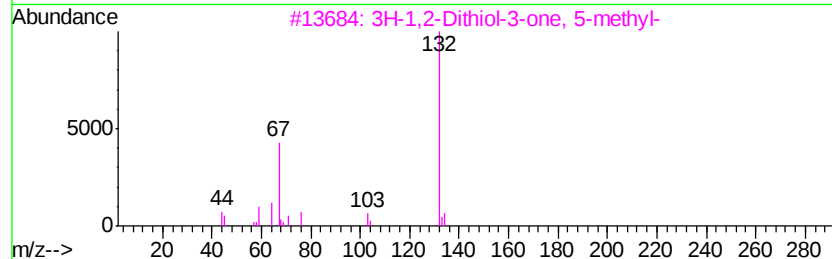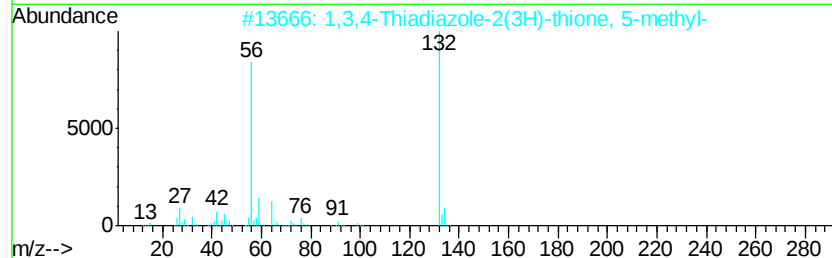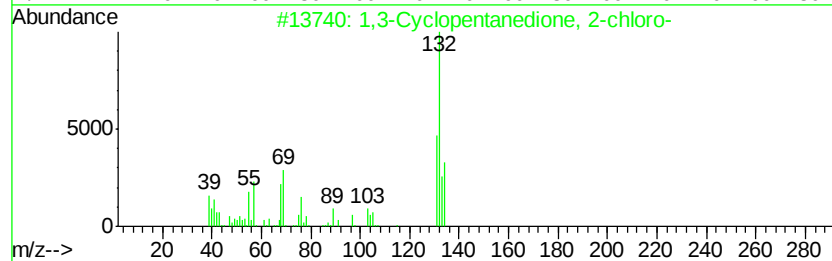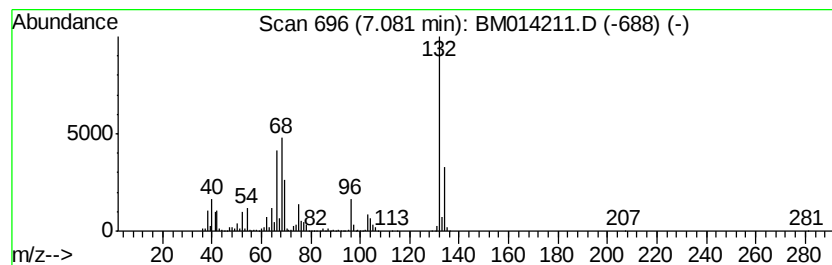

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020918\
Data File : BM014211.D
Acq On : 09 Feb 2018 11:46
Operator : SJ/JU
Sample : PB106384BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB106384BL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.08	7.08	105.8	ng	3334450	1	7.54	630210	20.0