

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020918\
 Data File : BM014216.D
 Acq On : 09 Feb 2018 16:10
 Operator : SJ/JU
 Sample : PB106423BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB106423BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM020718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.163	364	370	383	rBV	1568743	2251715	47.89%	8.051%
2	6.734	630	637	650	rBV	1565165	2423306	51.54%	8.665%
3	7.075	688	695	711	rBV	1655268	2592044	55.13%	9.268%
4	7.540	767	774	788	rBV	427405	683446	14.54%	2.444%
5	7.851	821	827	842	rVB	1227822	1999521	42.53%	7.149%
6	8.698	965	971	983	rBV	867312	1528160	32.50%	5.464%
7	10.310	1238	1245	1262	rBV	437590	846458	18.00%	3.027%
8	12.804	1662	1669	1684	rBV	2212008	3475058	73.91%	12.425%
9	14.198	1900	1906	1923	rBV2	685966	1161058	24.69%	4.151%
10	15.698	2154	2161	2177	rBV	1738043	2696929	57.36%	9.643%
11	16.951	2369	2374	2388	rBV2	791197	1310084	27.86%	4.684%
12	19.598	2818	2824	2836	rBV	3807246	4701929	100.00%	16.812%
13	21.162	3085	3090	3101	rBV	864410	1242989	26.44%	4.444%
14	23.339	3453	3460	3470	rBV	501620	1054797	22.43%	3.772%


Sum of corrected areas: 27967494

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020918\
Data File : BM014216.D
Acq On : 09 Feb 2018 16:10
Operator : SJ/JU
Sample : PB106423BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB106423BL

Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

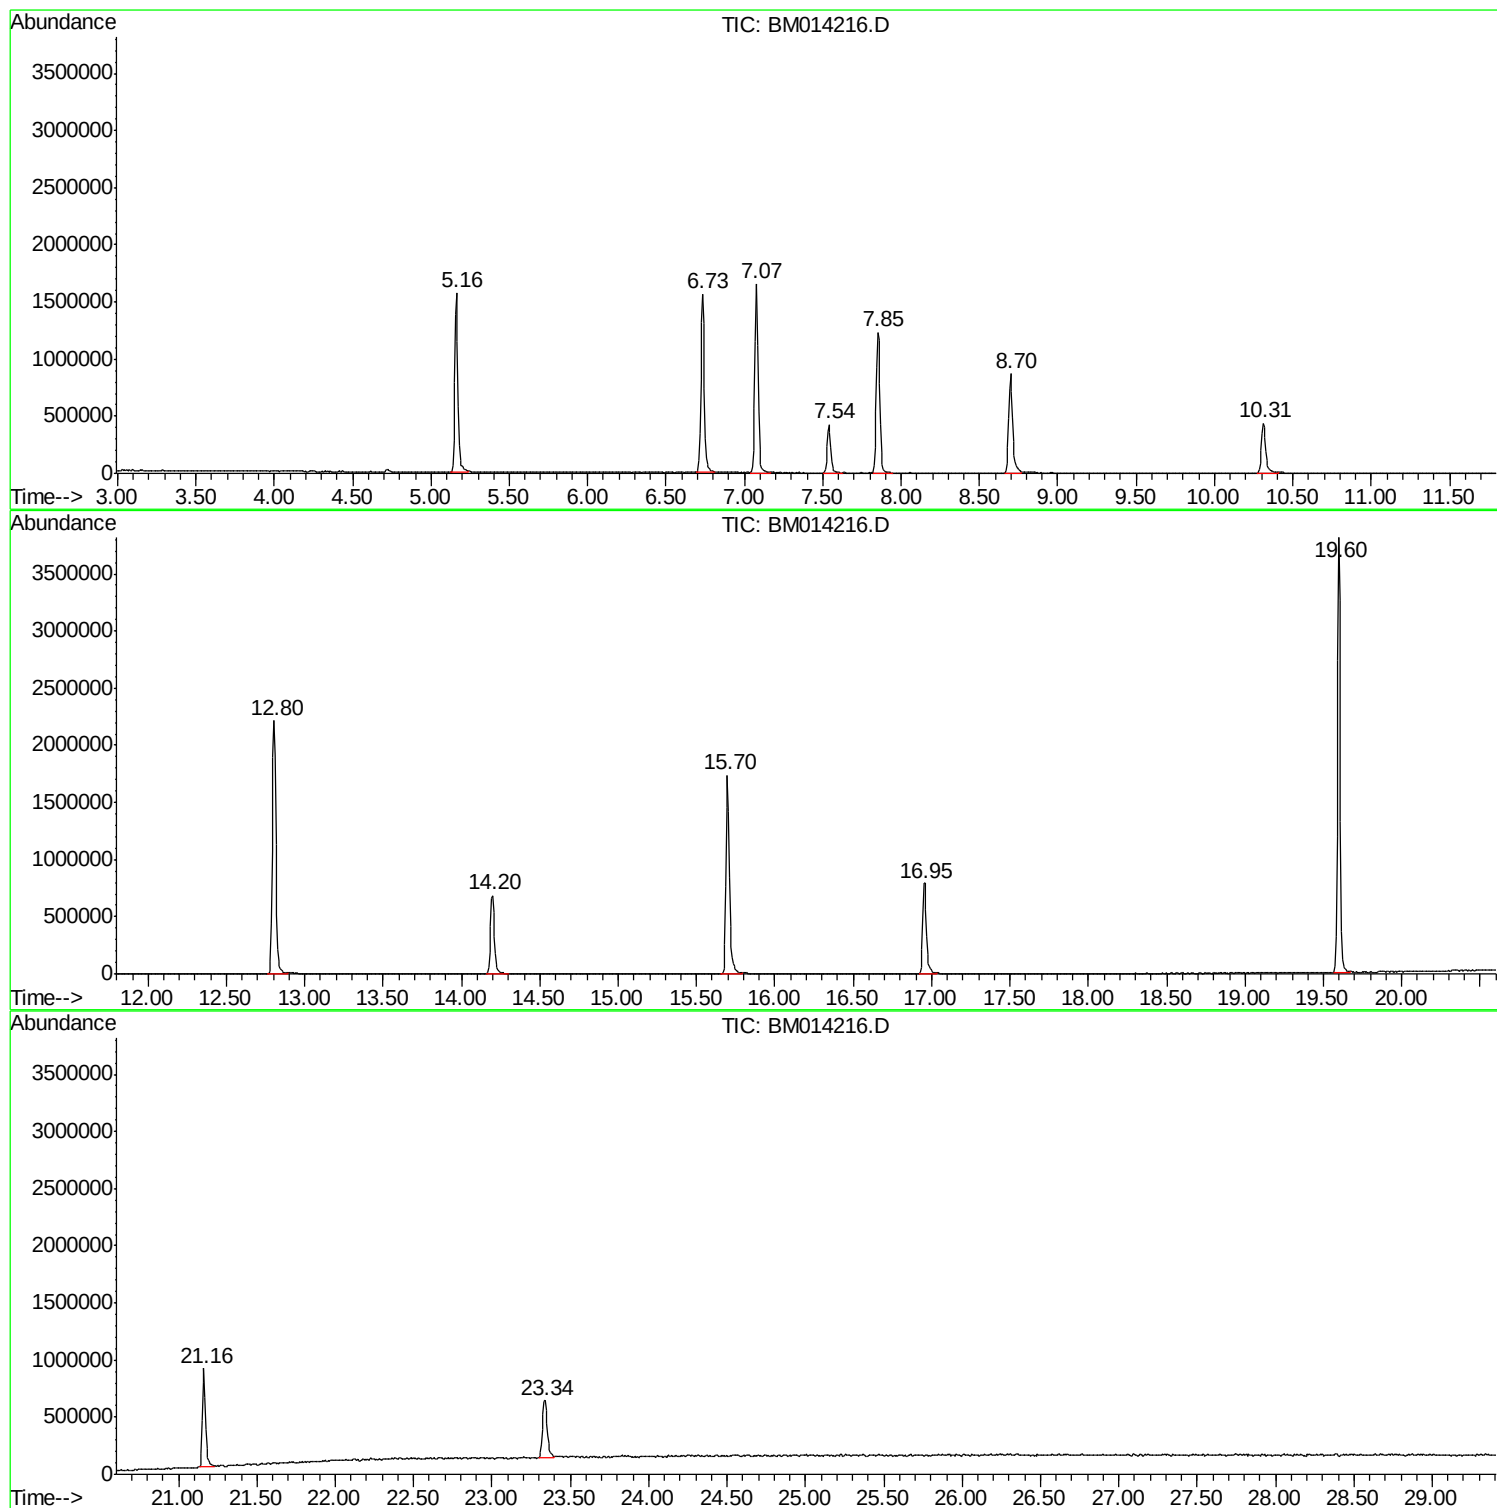

Data Path : Z:\HPCHEM1\BNA M\DATA\BM020918\
Data File : BM014216.D
Acq On : 09 Feb 2018 16:10
Operator : SJ/JU
Sample : PB106423BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB106423BL










Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.07 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.07	75.85 ng	2592040	1,4-Dichlorobenzene-d4	7.54

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	16
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	14
3		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	14
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	10
5		3H-1,2-Dithiol-3-one, 5-methyl-	132	C4H4OS2	003620-08-4	10

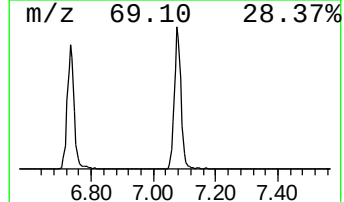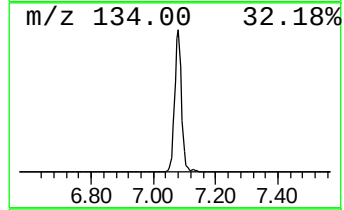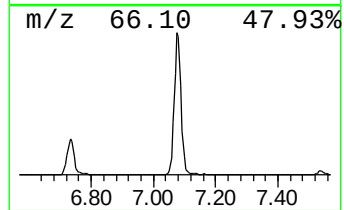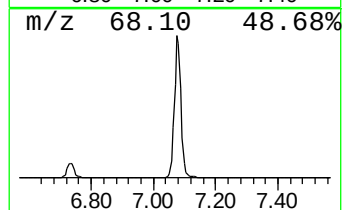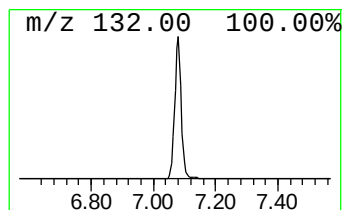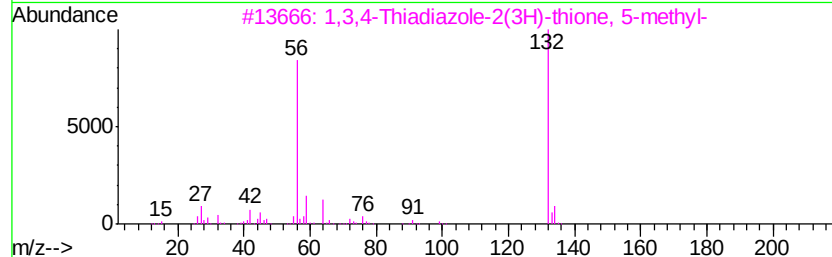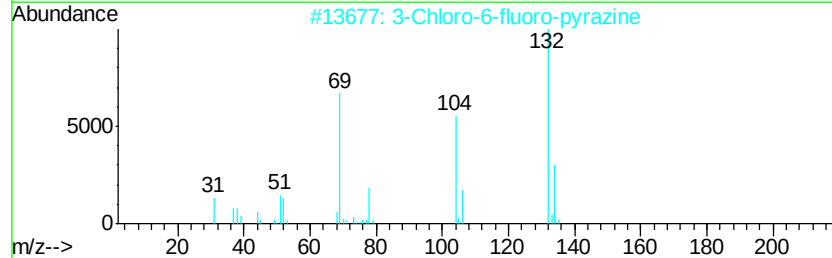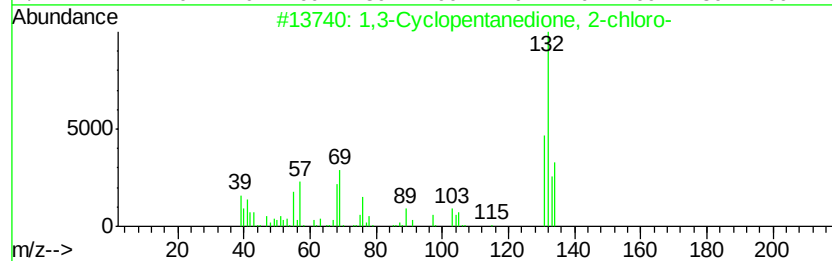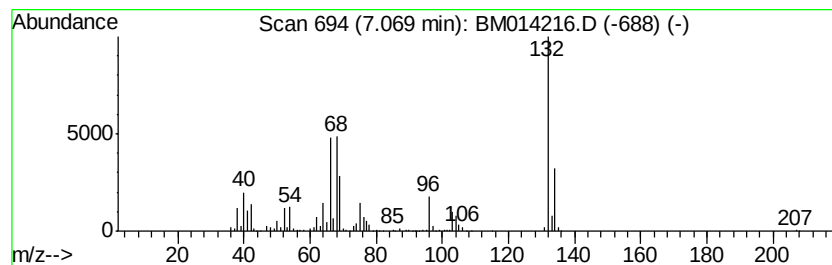

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM020918\
Data File : BM014216.D
Acq On : 09 Feb 2018 16:10
Operator : SJ/JU
Sample : PB106423BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB106423BL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM020718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.07	7.07	75.8	ng	2592040	1	7.54	683446	20.0