


Data Path : Z:\HPCHEM1\BNA M\Data\BM020918\
 Data File : BM014208.D
 Acq On : 09 Feb 2018 09:22
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM020718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 07 17:16:49 2018

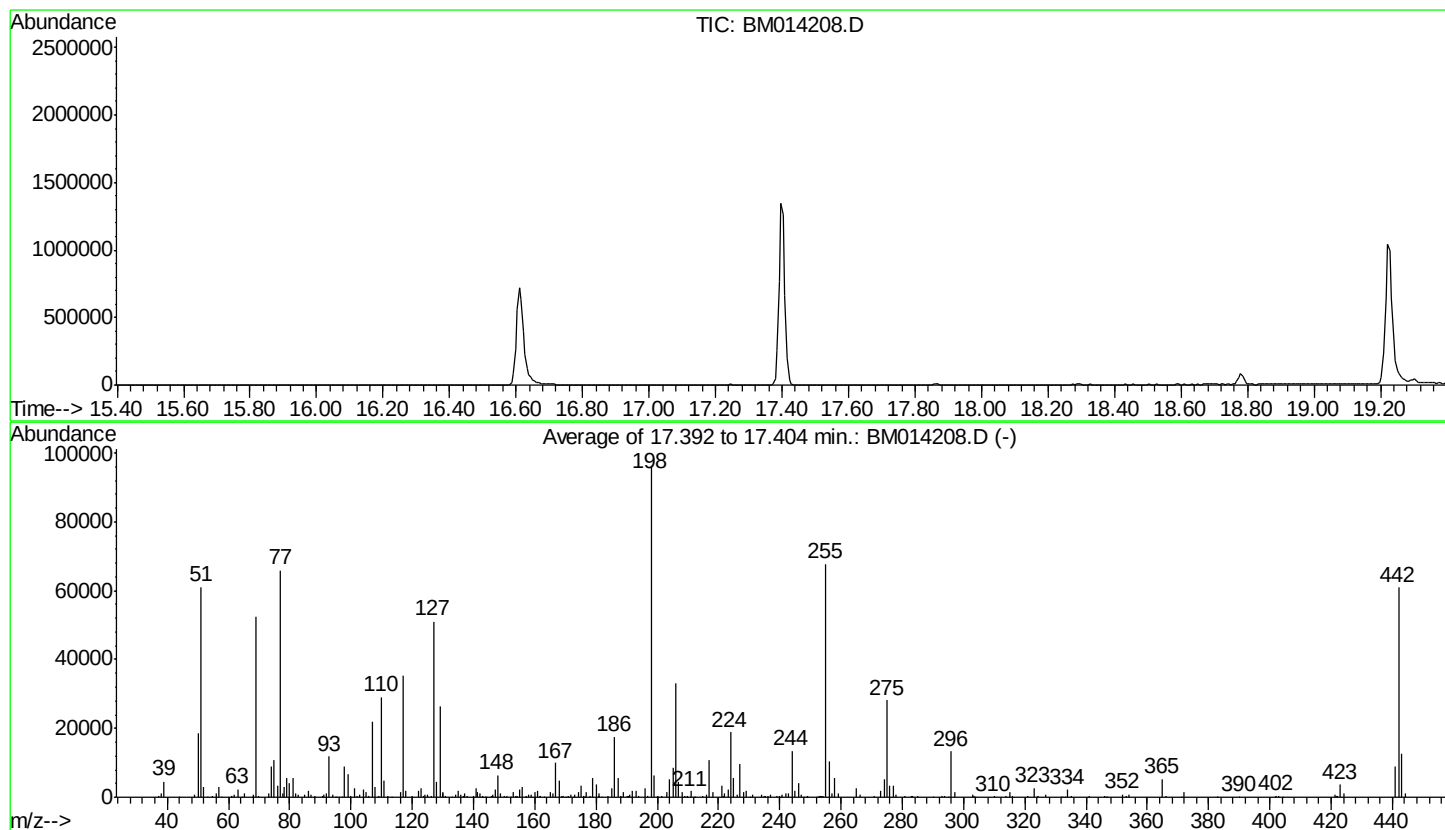

AutoFind: Scans 2449, 2450, 2451; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	63.4	61120	PASS
68	69	0.00	2	1.6	850	PASS
69	198	0.00	100	54.5	52546	PASS
70	69	0.00	2	0.6	335	PASS
127	198	10	80	53.0	51096	PASS
197	198	0.00	2	0.4	418	PASS
198	198	100	100	100.0	96354	PASS
199	198	5	9	6.6	6363	PASS
275	198	10	60	29.2	28136	PASS
365	198	1	100	5.5	5309	PASS
441	443	0.01	100	69.0	8814	PASS
442	198	50	100	63.2	60848	PASS
443	442	15	24	21.0	12779	PASS