
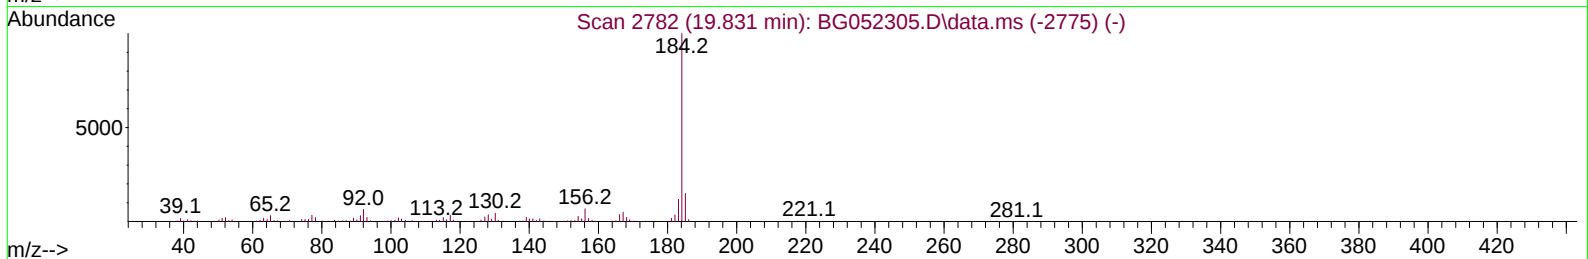
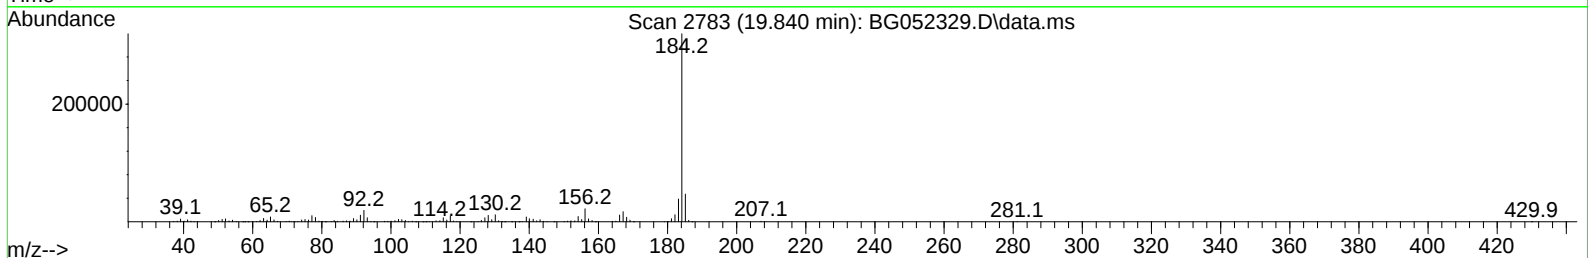


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020922\
 Data File : BG052329.D
 Acq On : 9 Feb 2022 10:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 11:42:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 08 01:21:20 2022
 Response via : Initial Calibration

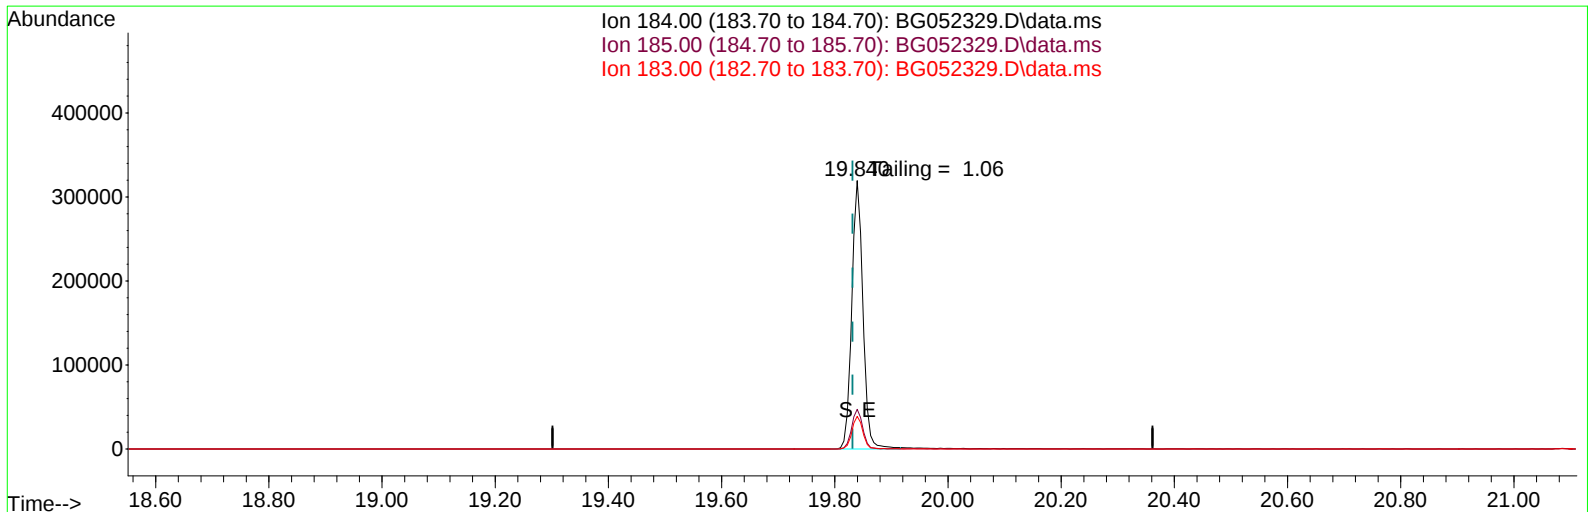

TIC: BG052329.D\data.ms

(77) Benzidine

19.840min (+ 0.009) 349965.80 ng m

response 433723

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.79
183.00	12.20	12.17
0.00	0.00	0.00