
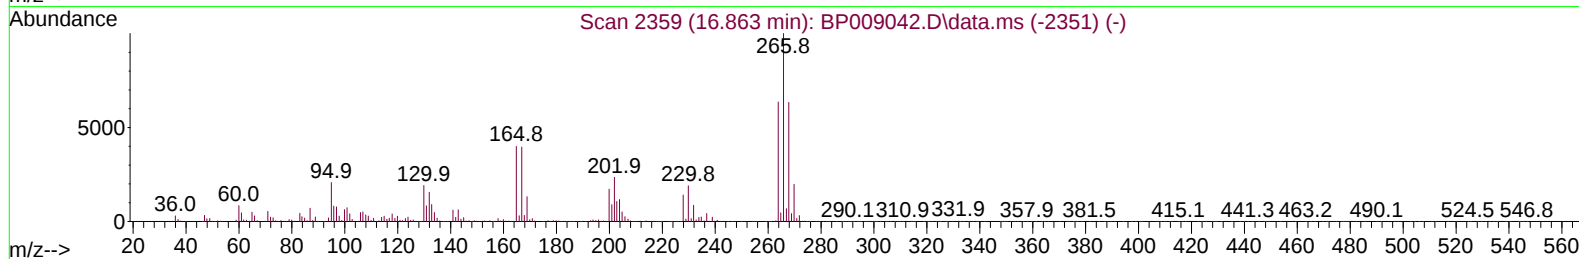
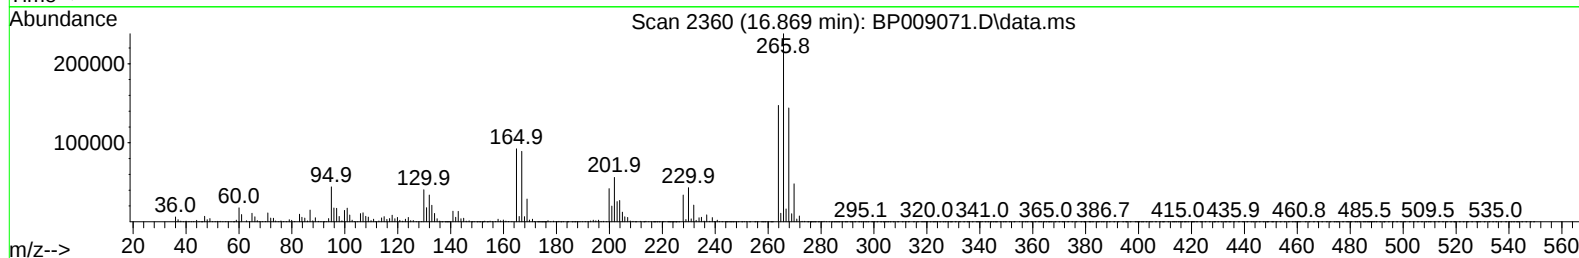


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020922\
Data File : BP009071.D
Acq On : 09 Feb 2022 09:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 12:05:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 07 15:13:17 2022
Response via : Initial Calibration

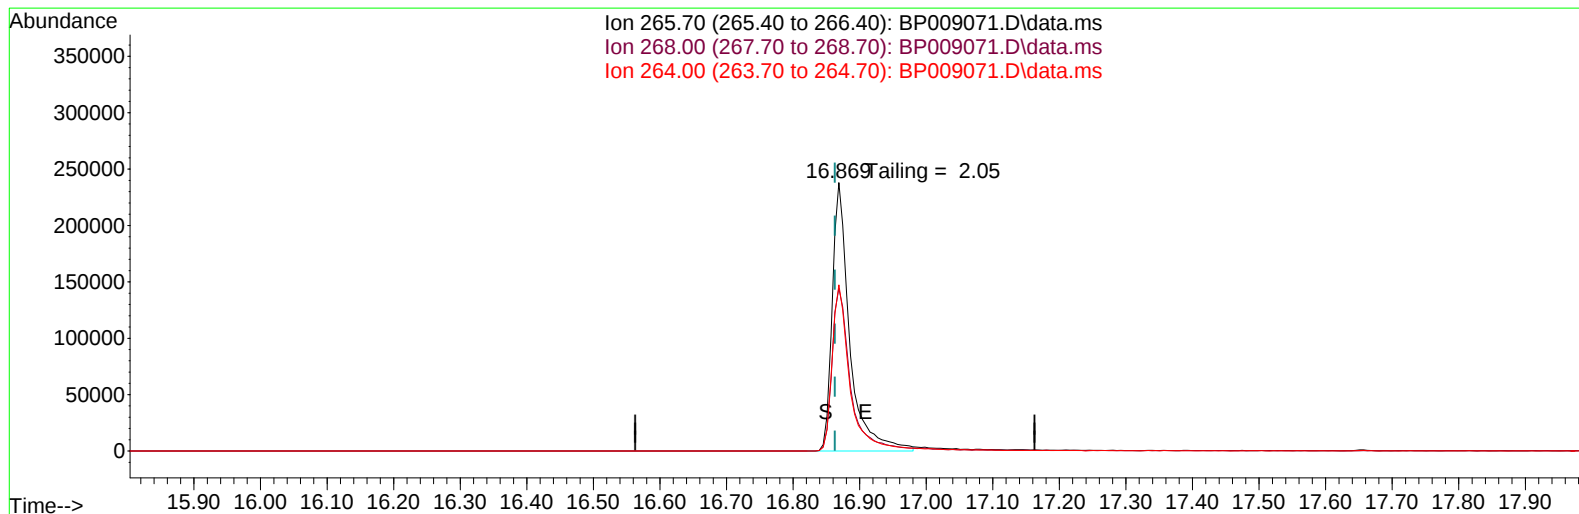

TIC: BP009071.D\data.ms

(70) Pentachlorophenol (C)

16.869min (+ 0.006) 5801337.89 ng

response 436167

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	60.55
264.00	62.90	61.90
0.00	0.00	0.00