

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020922\
 Data File : BM034032.D
 Acq On : 09 Feb 2022 17:44
 Operator : CG/JU
 Sample : PB142558BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB142558BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034032.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.444	96	98	101	rBV	2474267	3988042	51.57%	10.595%
2	7.066	167	170	172	rBV	1868923	3988472	51.57%	10.596%
3	7.900	204	207	209	rBV	496924	819489	10.60%	2.177%
4	9.071	256	259	261	rBV	975387	2576016	33.31%	6.843%
5	10.715	329	332	334	rBV	546408	1081408	13.98%	2.873%
6	13.170	438	441	443	rBV	4143672	6574704	85.02%	17.466%
7	14.545	499	502	504	rBV	726169	1385659	17.92%	3.681%
8	16.031	565	568	570	rBV2	1723479	4285079	55.41%	11.384%
9	17.270	621	623	626	rBV	1066383	1712030	22.14%	4.548%
10	19.883	737	739	742	rBV	3983577	7733569	100.00%	20.545%
11	21.437	806	808	811	rBV	1122903	1821903	23.56%	4.840%
12	23.825	912	914	917	rVB	815020	1675441	21.66%	4.451%




Sum of corrected areas: 37641812

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020922\
Data File : BM034032.D
Acq On : 09 Feb 2022 17:44
Operator : CG/JU
Sample : PB142558BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB142558BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

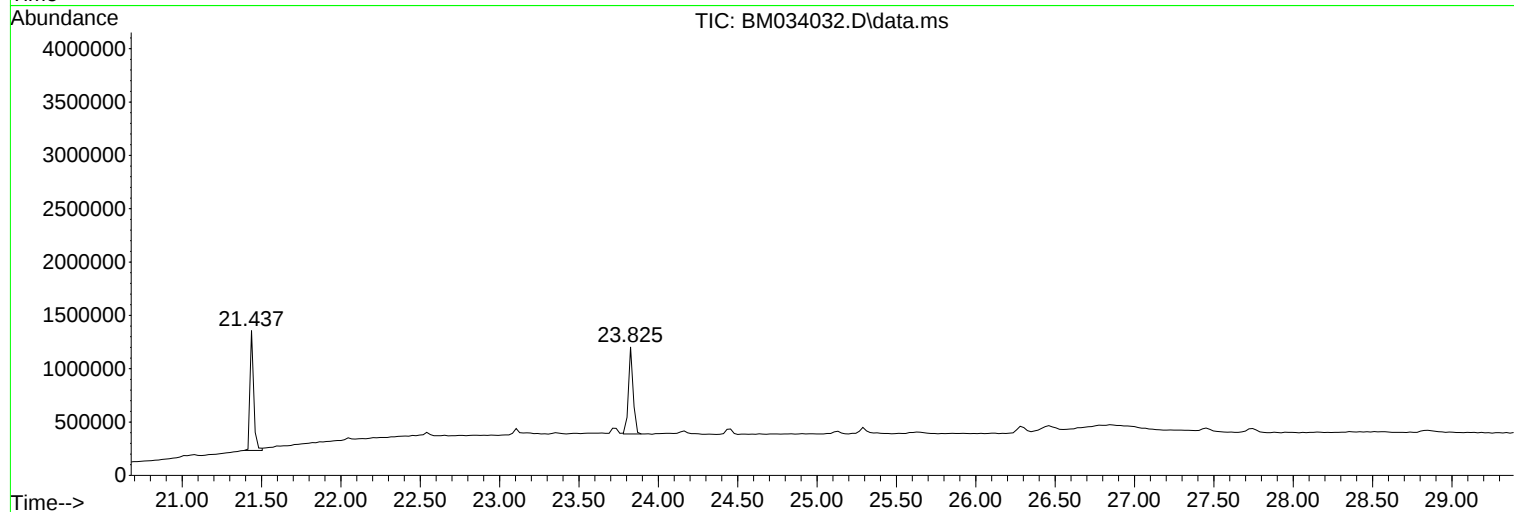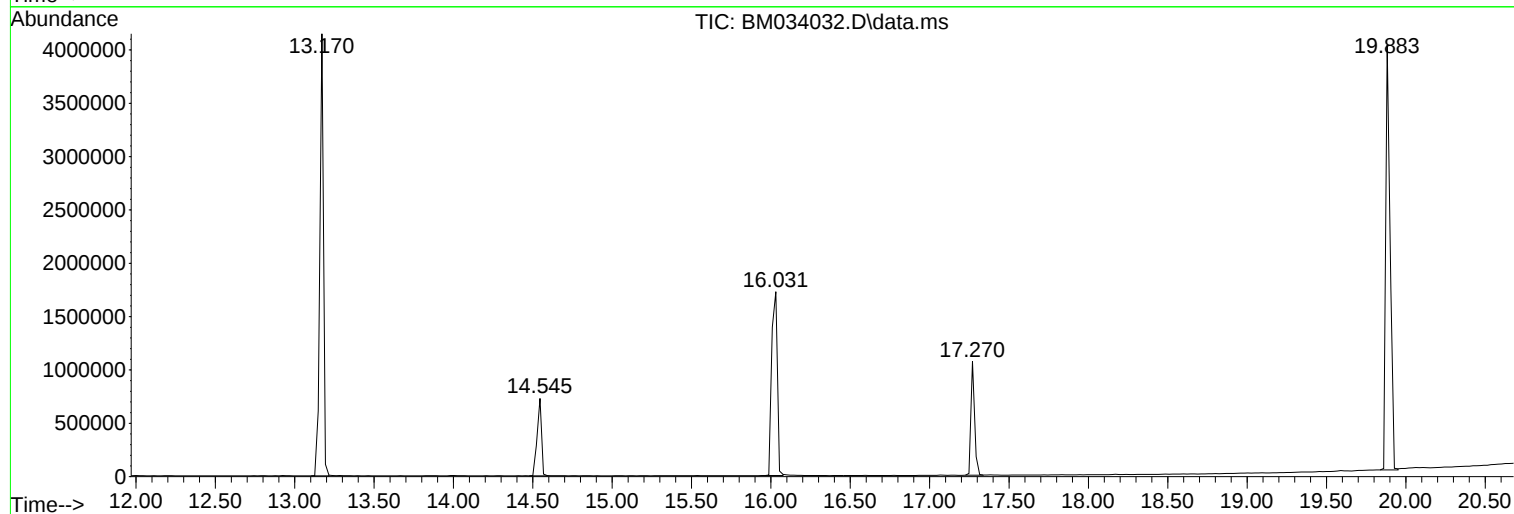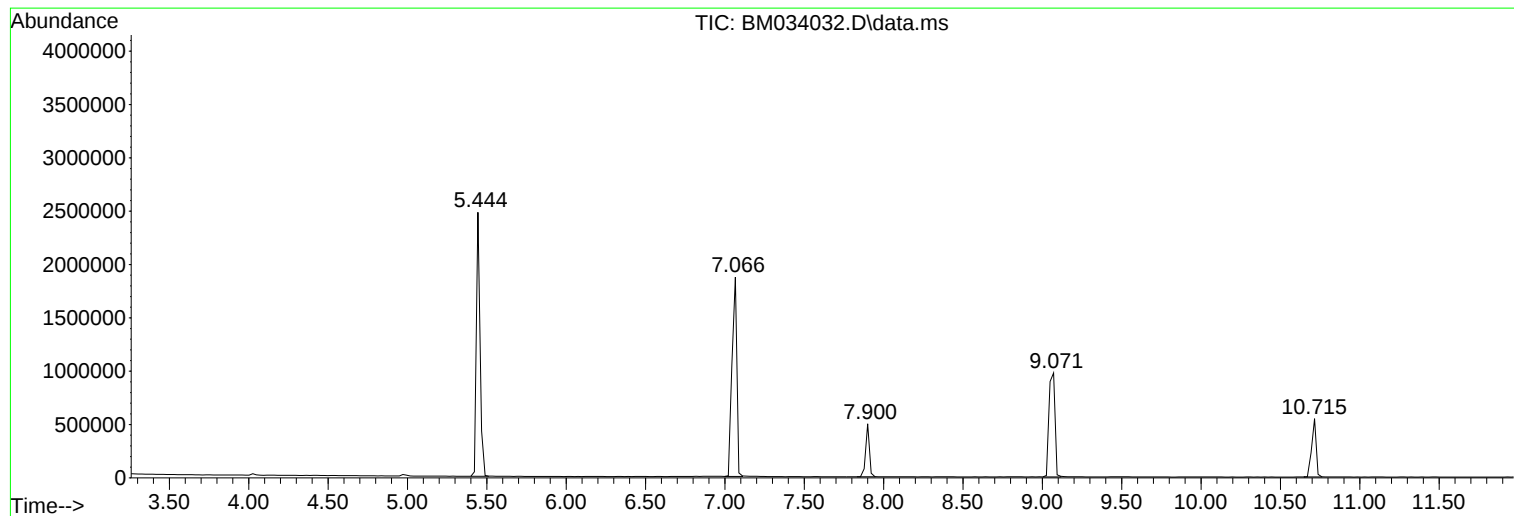

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020922\
Data File : BM034032.D
Acq On : 09 Feb 2022 17:44
Operator : CG/JU
Sample : PB142558BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB142558BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020922\
Data File : BM034032.D
Acq On : 09 Feb 2022 17:44
Operator : CG/JU
Sample : PB142558BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB142558BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------