
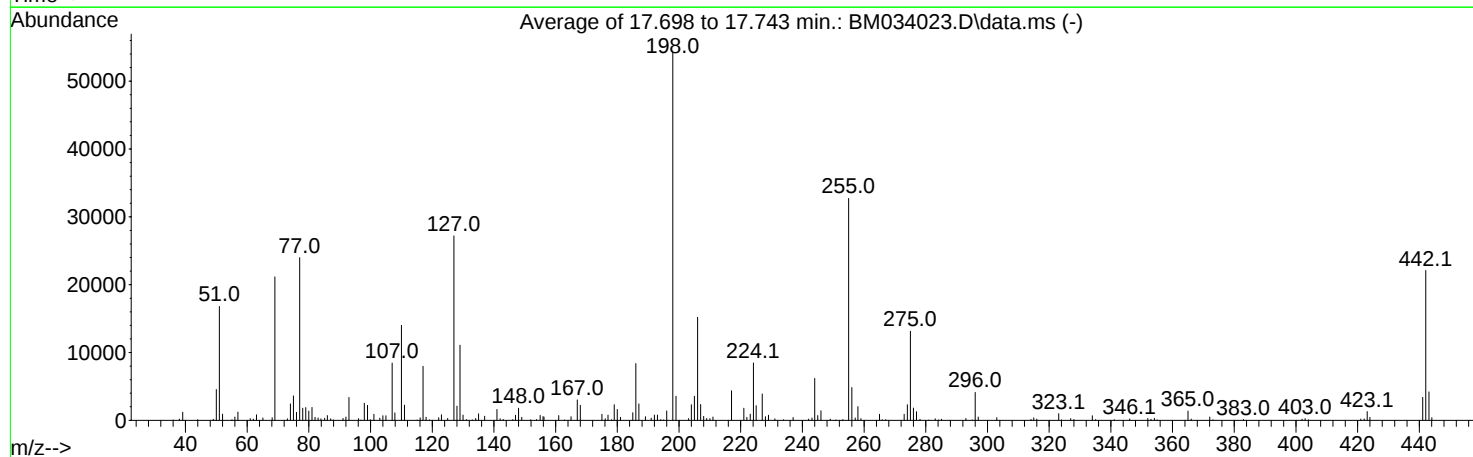


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020922\
 Data File : BM034023.D
 Acq On : 09 Feb 2022 11:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 09 17:52:36 2022

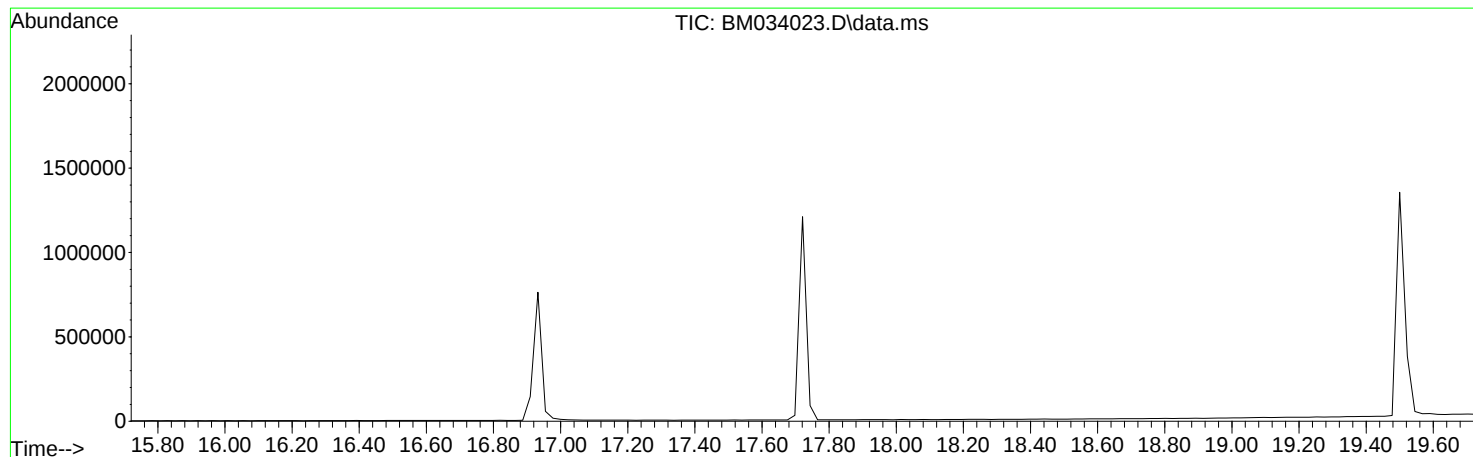




AutoFind: Scans 642, 643, 644; Background Corrected with Scan 639

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.0	16805	PASS
68	69	0.00	2	1.9	393	PASS
69	198	0.00	100	39.0	21150	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.2	27205	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	54222	PASS
199	198	5	9	6.6	3570	PASS
275	198	10	60	24.2	13134	PASS
365	198	1	100	2.5	1368	PASS
441	198	0.01	100	6.3	3401	PASS
442	442	50	100	100.0	22091	PASS
443	442	15	24	19.0	4194	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020922\
Data File : BM034023.D
Acq On : 09 Feb 2022 11:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 09 15:07:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 09 15:00:54 2022
Response via : Initial Calibration

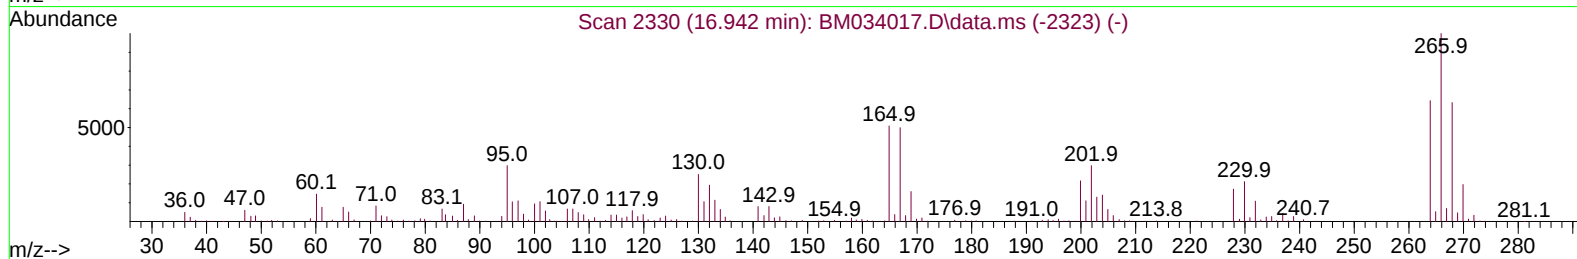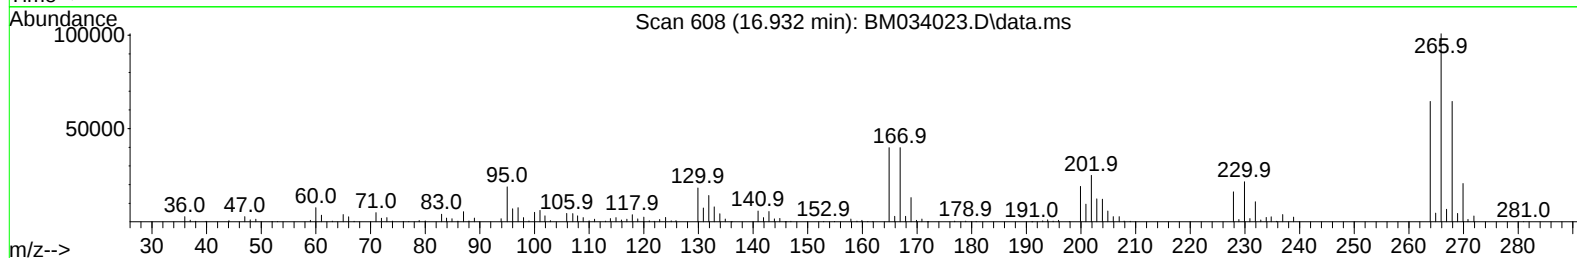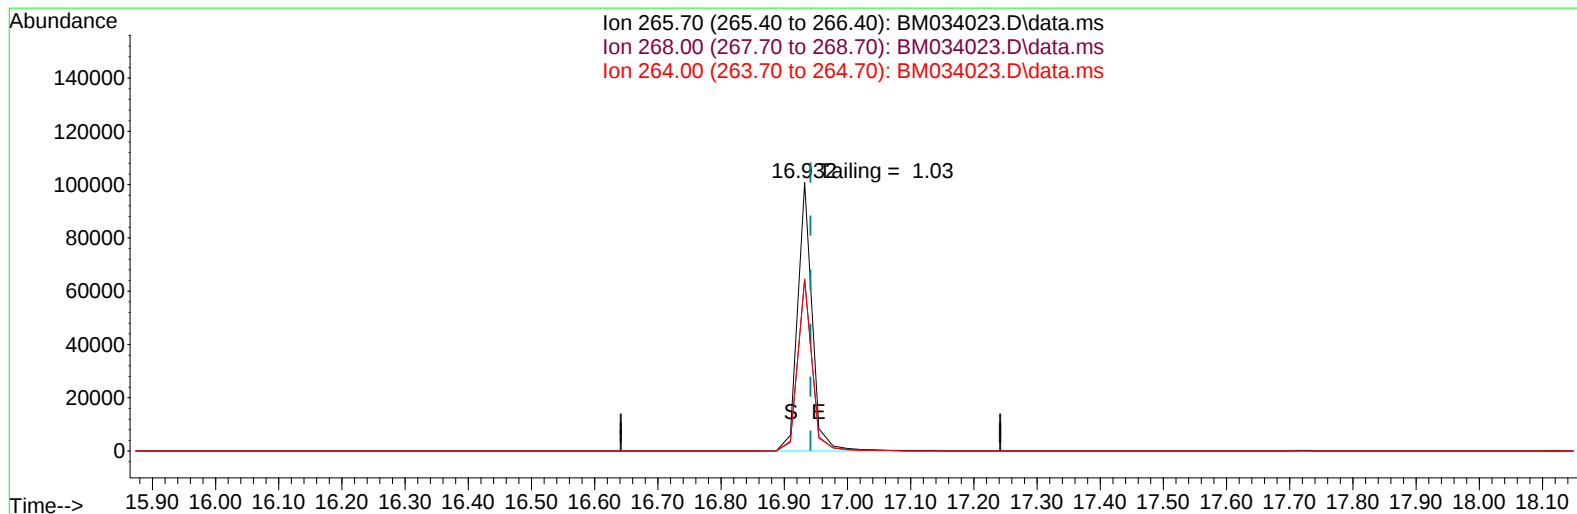

TIC: BM034023.D\data.ms

(70) Pentachlorophenol (C)

16.932min (-0.010) 0.00 ng




response 161860

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.02
264.00	61.40	64.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020922\
 Data File : BM034023.D
 Acq On : 09 Feb 2022 11:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Feb 09 15:07:07 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 09 15:00:54 2022
 Response via : Initial Calibration

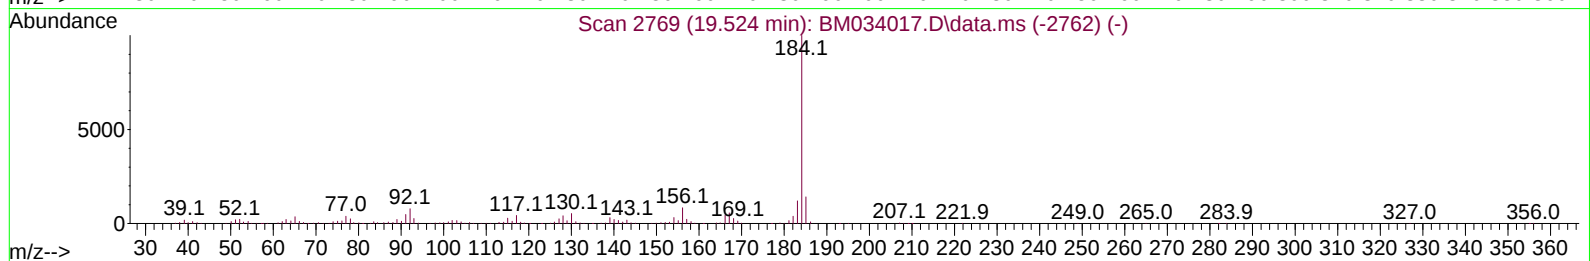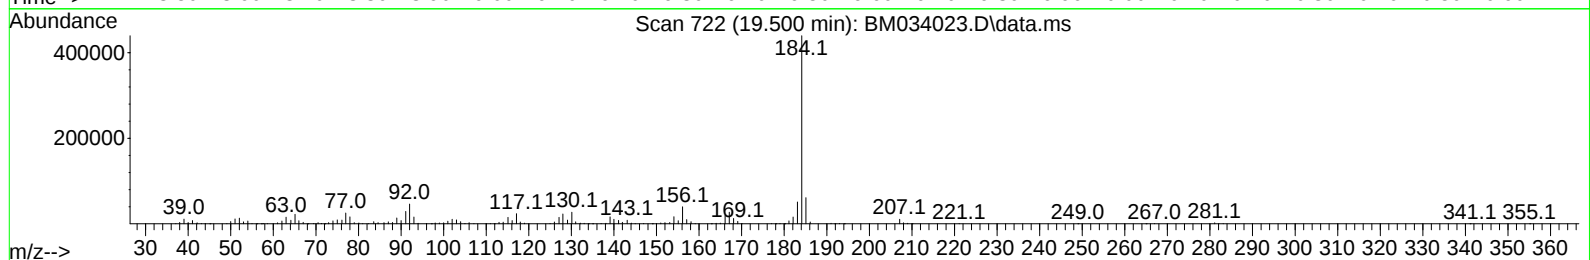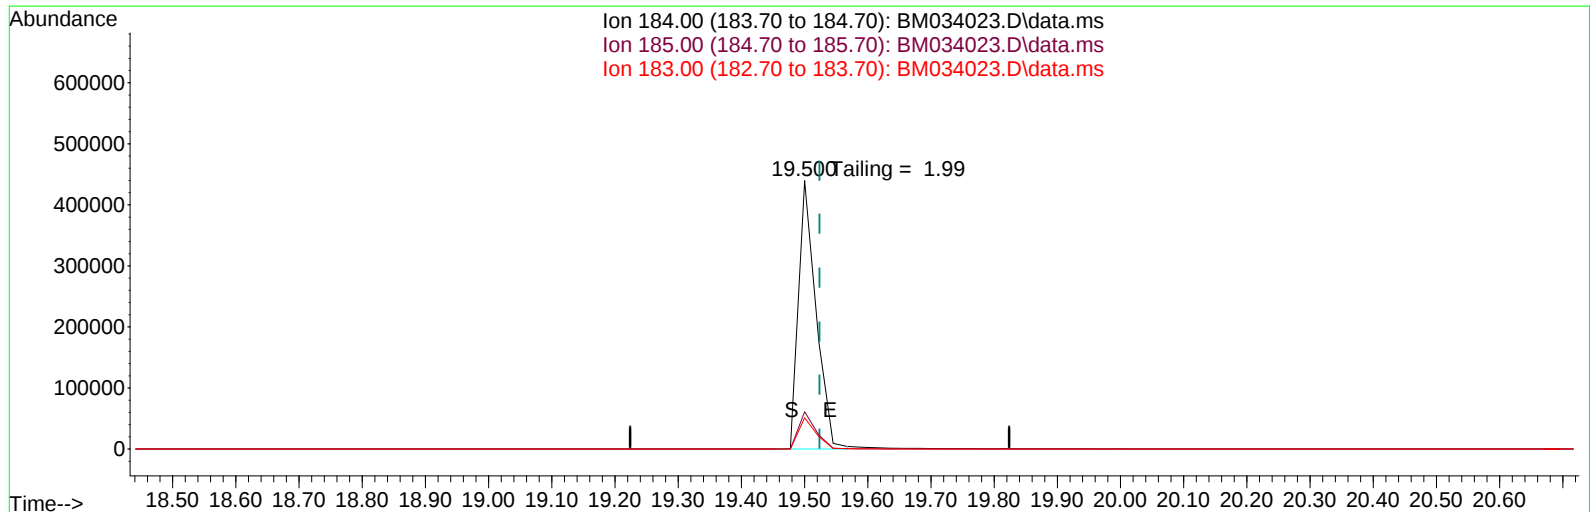

TIC: BM034023.D\data.ms

(77) Benzidine

19.500min (-0.024) 0.00 ng

response 864453

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.92
183.00	12.10	11.64
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/9/2022	BNA_M	<u>BM034023.D</u>
Compound Name	Response	Retention Time
DDT	535960	20.73
DDD	1224	20.31
DDE	0	19.9
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1224	537184	0.23

Instrument :
BNA_M
ClientSampleId :
DFTPP