


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020924\
Data File : BM044029.D
Acq On : 09 Feb 2024 08:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 09 02:42:01 2024

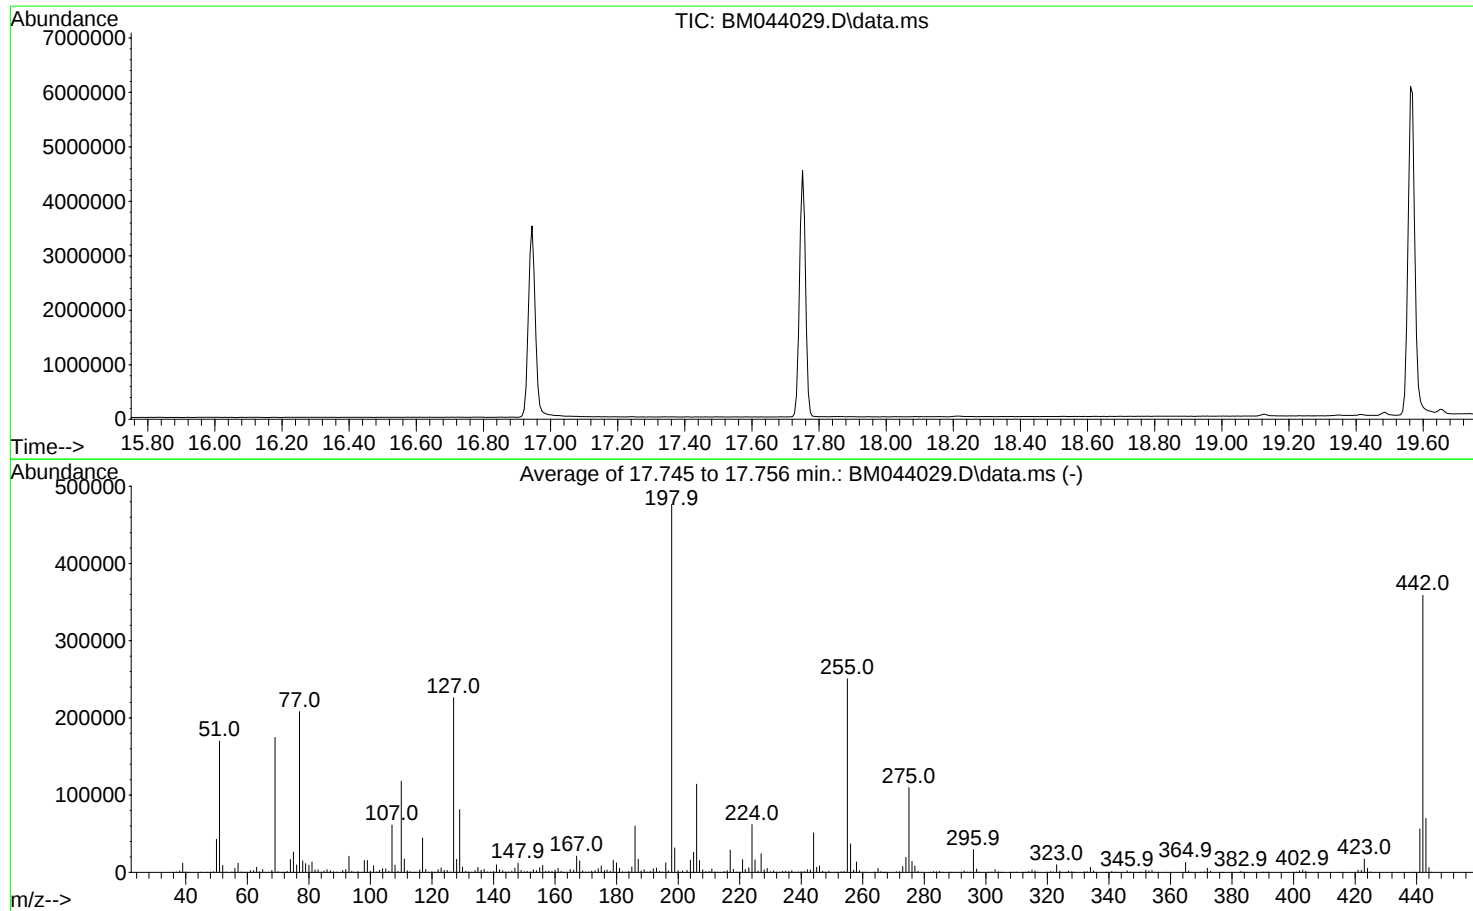




AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	170196	PASS
68	69	0.00	2	1.5	2598	PASS
69	198	0.00	100	36.7	174672	PASS
70	69	0.00	2	0.6	970	PASS
127	198	10	80	47.5	226069	PASS
197	198	0.00	2	0.4	1879	PASS
198	198	100	100	100.0	476416	PASS
199	198	5	9	6.7	31755	PASS
275	198	10	60	23.0	109776	PASS
365	198	1	100	2.7	12887	PASS
441	198	0.01	100	11.9	56477	PASS
442	442	50	100	100.0	358763	PASS
443	442	15	24	19.5	69877	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020924\
 Data File : BM044029.D
 Acq On : 09 Feb 2024 08:51
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Feb 09 10:38:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 09 02:42:01 2024
 Response via : Initial Calibration

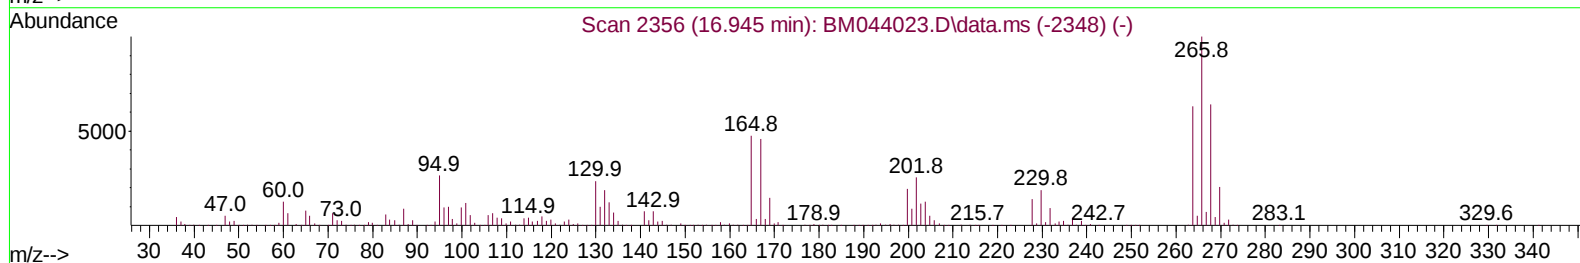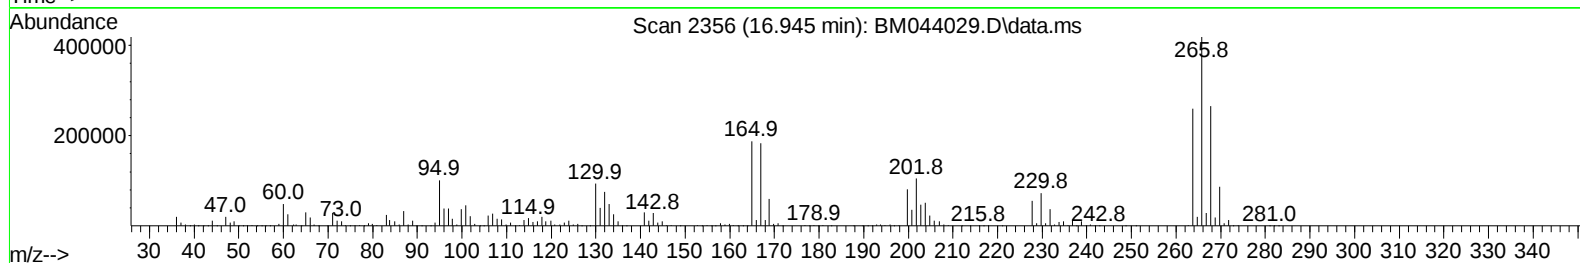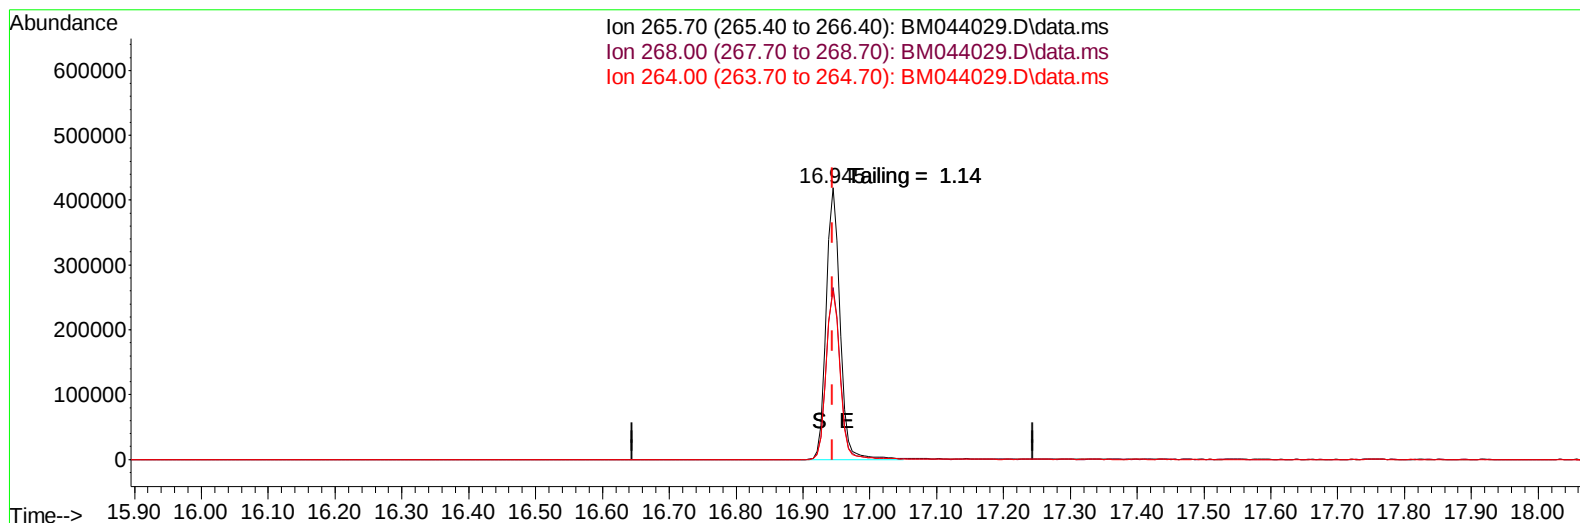

TIC: BM044029.D\data.ms

(70) Pentachlorophenol (C)

16.945min (-0.000) 0.00 ng




response 599756

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	63.33
264.00	63.10	62.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020924\
Data File : BM044029.D
Acq On : 09 Feb 2024 08:51
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 09 10:38:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 09 02:42:01 2024
Response via : Initial Calibration

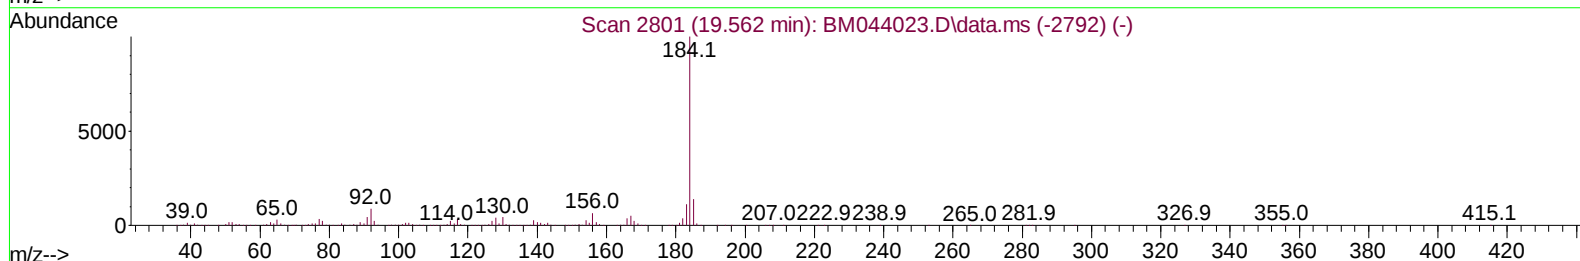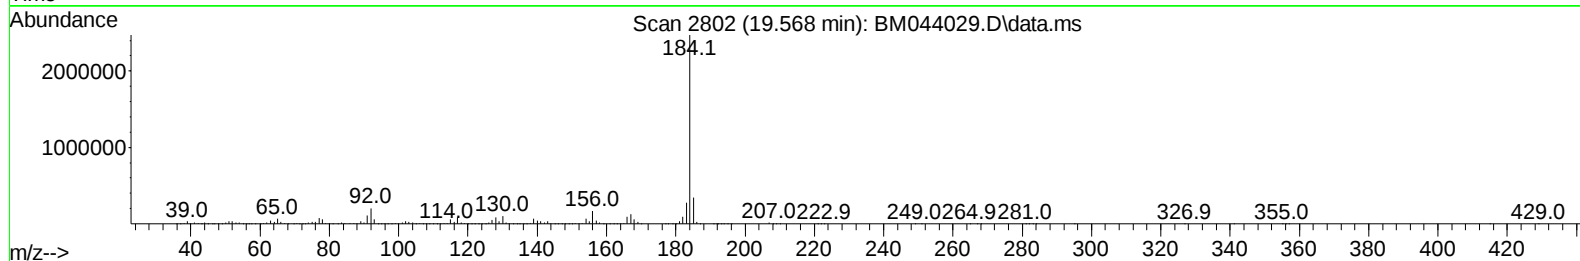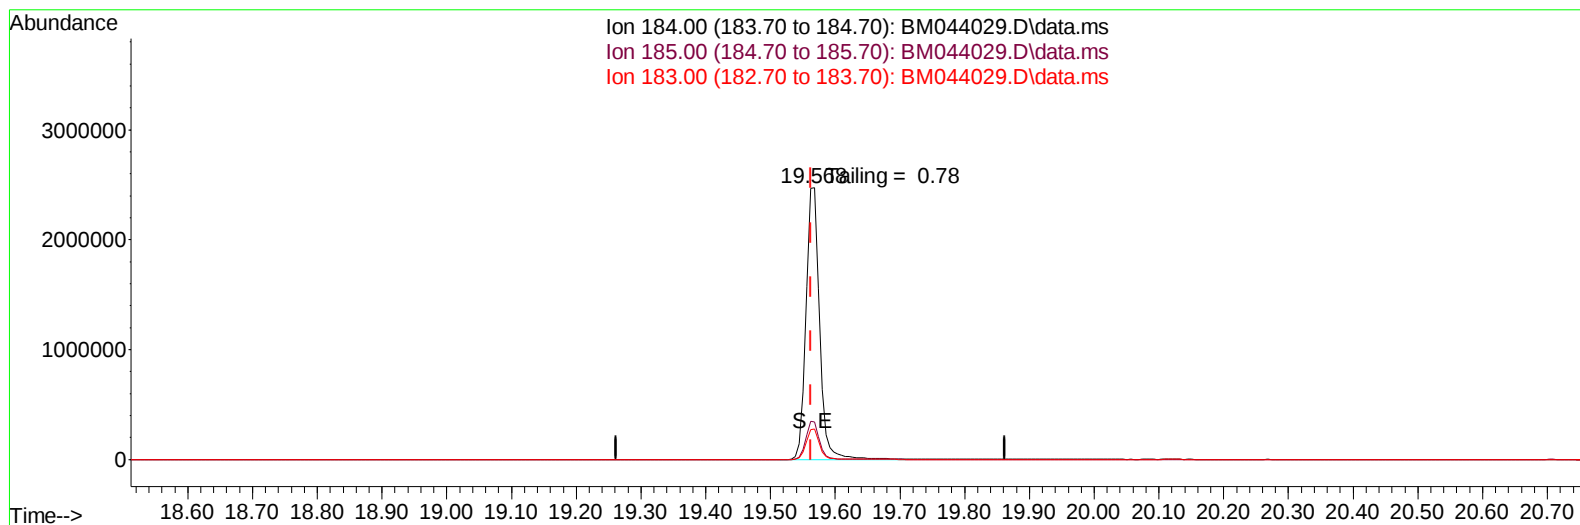

TIC: BM044029.D\data.ms

(77) Benzidine

19.568min (+ 0.006) 410930.13 ng

response 3601714

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	13.84
183.00	11.20	11.25
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/9/2024	BNA_M	<u>BM044029.D</u>
Compound Name	Response	Retention Time
DDT	1651148	20.803
DDD	23710	20.409
DDE	1805	19.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25515	1676663	1.52

Instrument :
BNA_M
ClientSampleId :
DFTPP