

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021021\
 Data File : BM028712.D
 Acq On : 10 Feb 2021 19:55
 Operator : CG/JU
 Sample : M1310-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Feb 10 23:36:38 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 10 14:28:04 2021
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	448	0.40	ng/ul	0.00
2) Naphthalene-d8	10.70	136	1819	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.55	164	989	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.28
16) Chrysene-d12	21.43	240	1624	0.40	ng/ul	0.00
20) Perylene-d12	23.66	264	1654	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.29	152	889	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.29	212	1562	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.66	202	293	0.050	ng/ul#	1
23) Benzo(a)pyrene	23.52	252	457	0.091	ng/ul#	27


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021021\
Data File : BM028712.D
Acq On : 10 Feb 2021 19:55
Operator : CG/JU
Sample : M1310-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Feb 10 23:36:38 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 10 14:28:04 2021
Response via : Initial Calibration

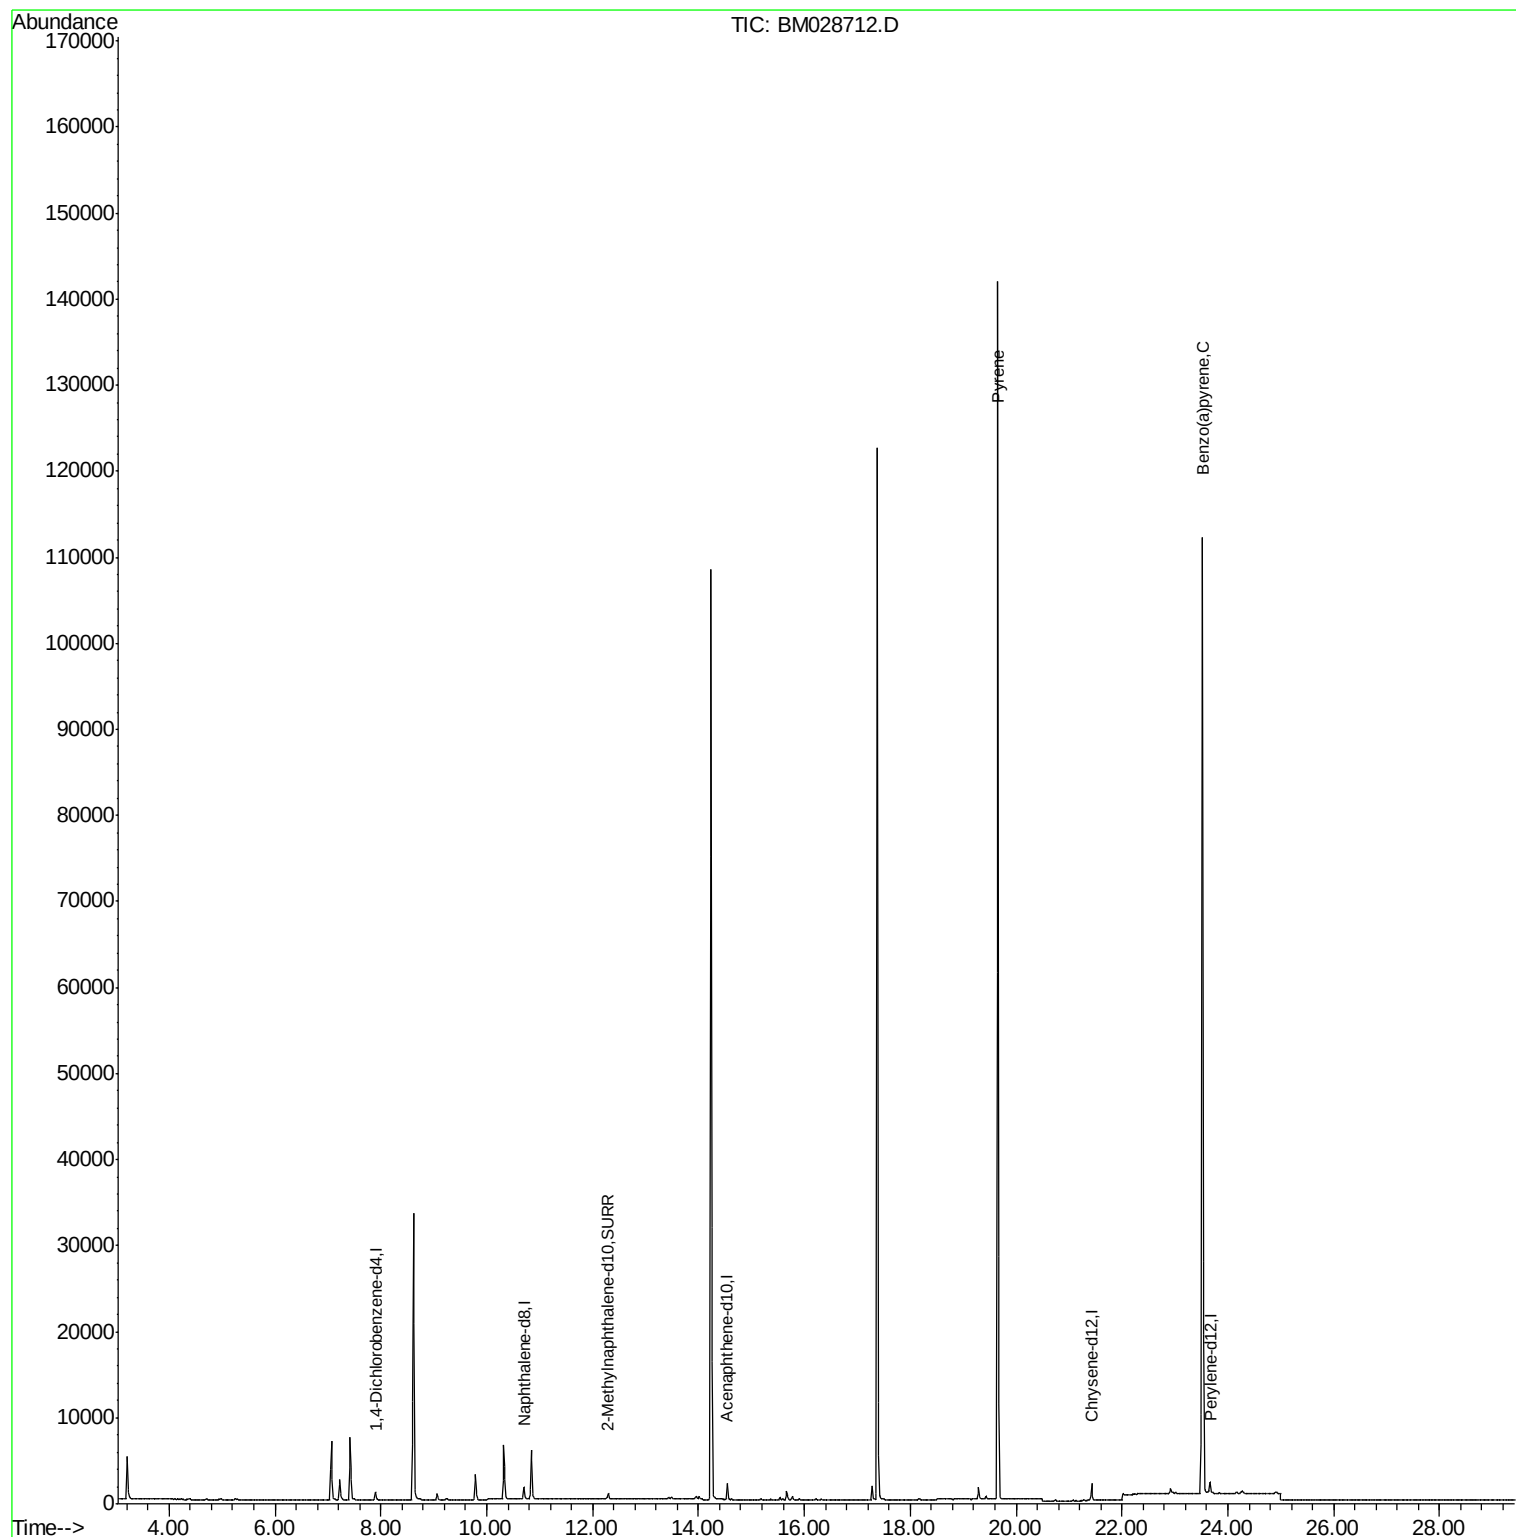


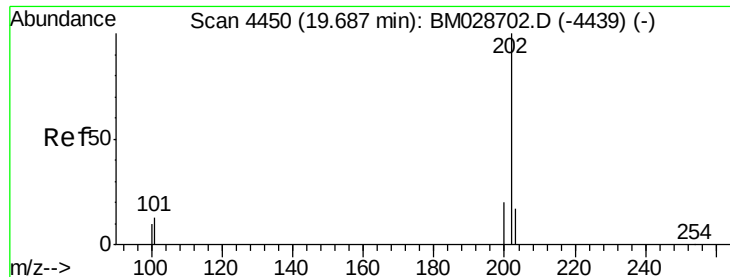




#17
 Pvrene
 Concen: 0.050 ng/ul
 RT: 19.66 min Scan# 4442
 Delta R.T. -0.03 min
 Lab File: BM028712.D
 Acq: 10 Feb 2021 19:55

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:202 Resp: 293
 Ion Ratio Lower Upper
 202 100
 101 157.9 12.7 19.1#
 100 924.6 10.2 15.4#

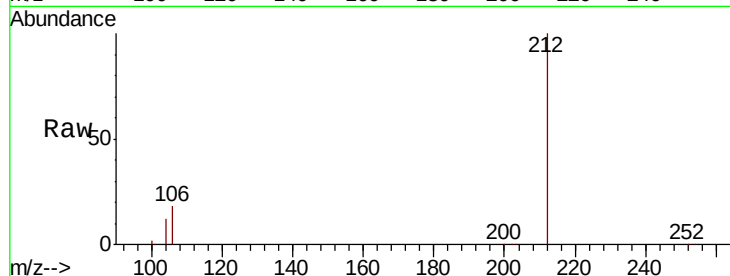


Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

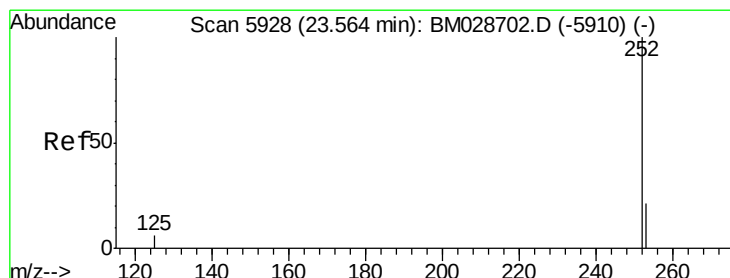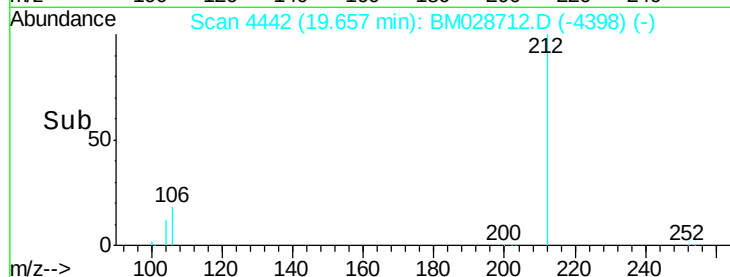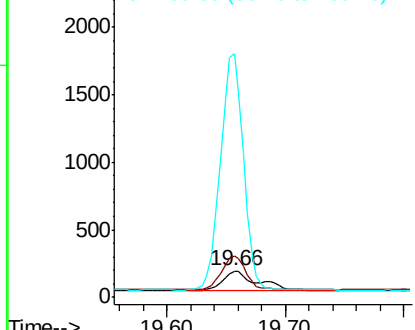

#23
 Benzo(a)pyrene
 Concen: 0.091 ng/ul
 RT: 23.52 min Scan# 5909
 Delta R.T. -0.05 min
 Lab File: BM028712.D
 Acq: 10 Feb 2021 19:55

Tgt Ion:252 Resp: 457
 Ion Ratio Lower Upper
 252 100
 253 64.9 28.7 43.1#
 125 91.5 27.9 41.9#

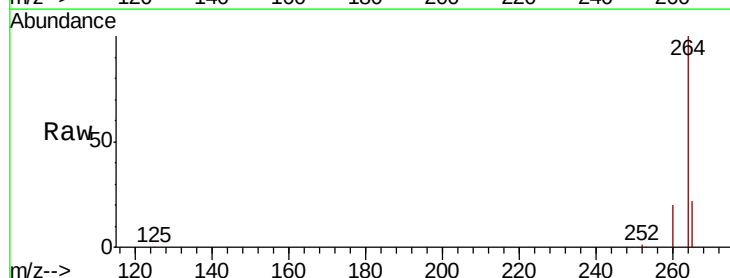

Abundance Ion 252.00 (251.70 to 252.70): E
 Ion 253.00 (252.70 to 253.70): E
 Ion 125.00 (124.70 to 125.70): E

