


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021021\
Data File : BM028703.D
Acq On : 10 Feb 2021 14:27
Operator : CG/JU
Sample : PB134505BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK05

Manual Integrations
APPROVED

mohammad
2/11/2021 9:46:54 AM

Quant Time: Feb 10 14:59:16 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 10 14:28:04 2021
Response via : Initial Calibration

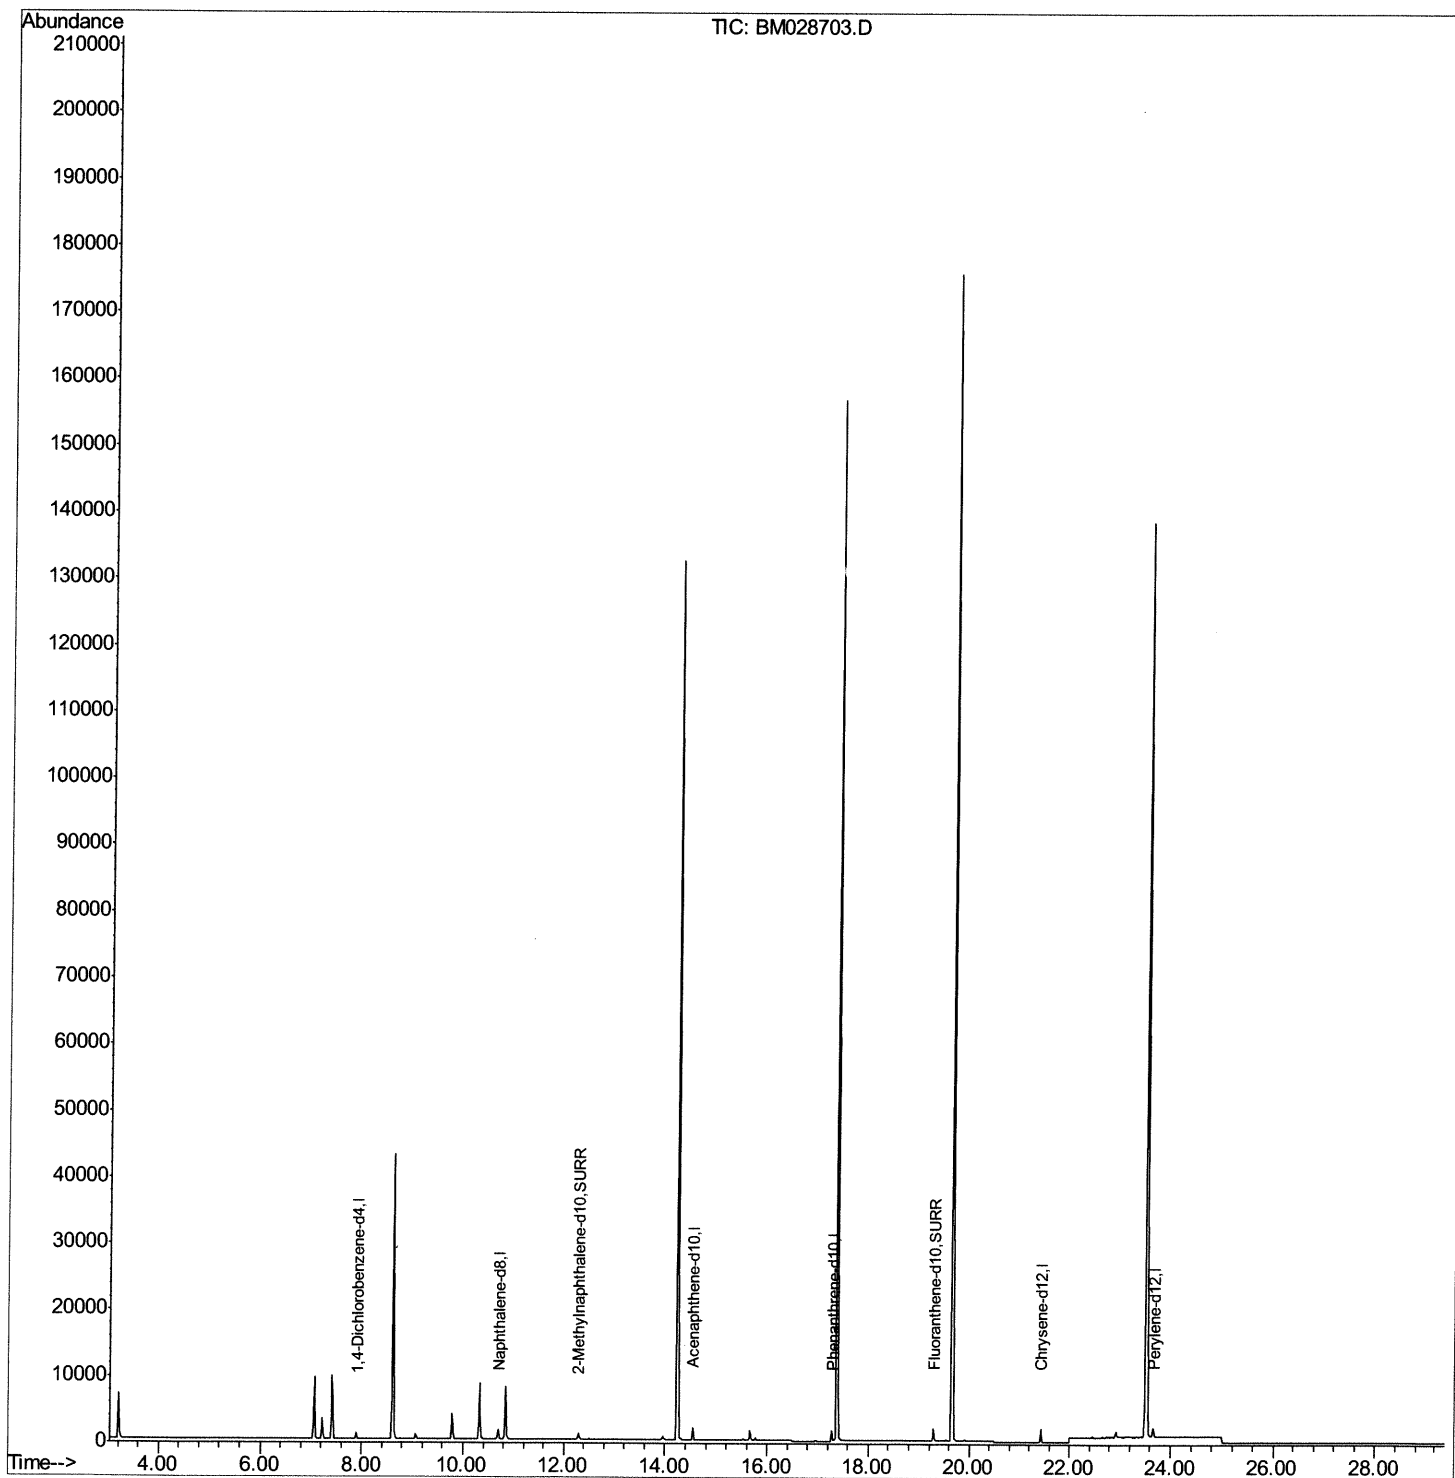

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021021\
Data File : BM028703.D
Acq On : 10 Feb 2021 14:27
Operator : CG/JU
Sample : PB134505BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK05

Manual Integrations
APPROVED

mohammad
2/11/2021 9:46:54 AM

Quant Time: Feb 10 14:58:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 10 14:28:04 2021
Response via : Initial Calibration

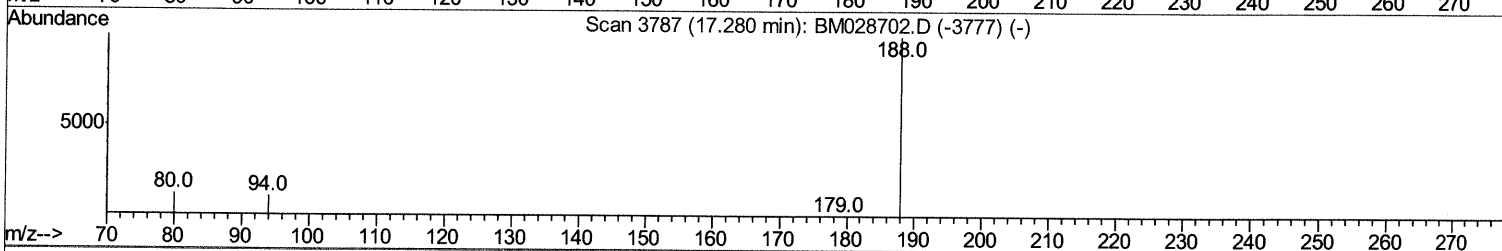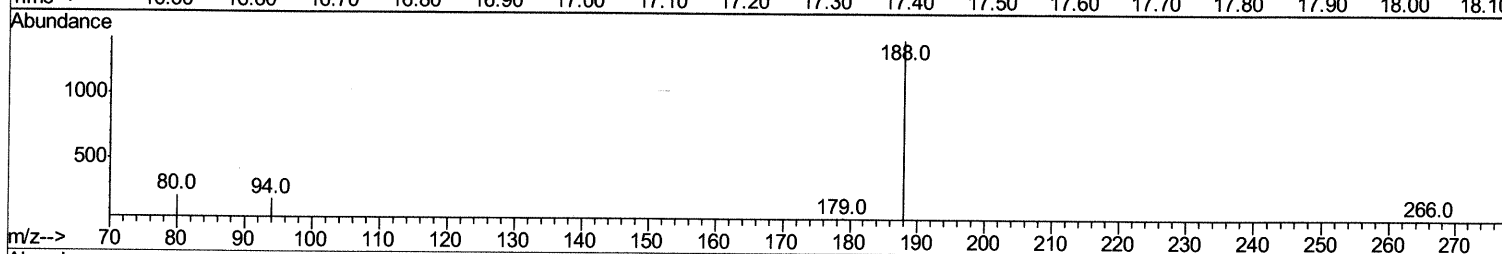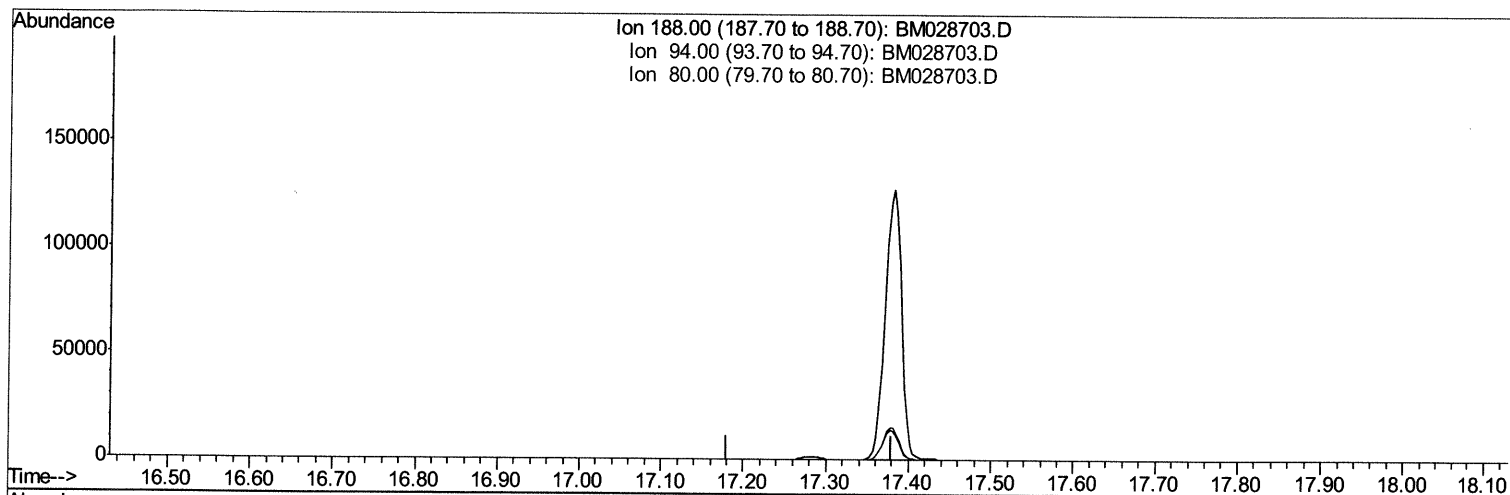

TIC: BM028703.D

(10) Phenanthrene-d10 (I)

17.280min (-17.280) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	13.50	0.00#
80.00	14.00	0.00#
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021021\
Data File : BM028703.D
Acq On : 10 Feb 2021 14:27
Operator : CG/JU
Sample : PB134505BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK05

Manual Integrations
APPROVED

mohammad
2/11/2021 9:46:54 AM

Quant Time: Feb 10 14:58:10 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 10 14:28:04 2021
Response via : Initial Calibration

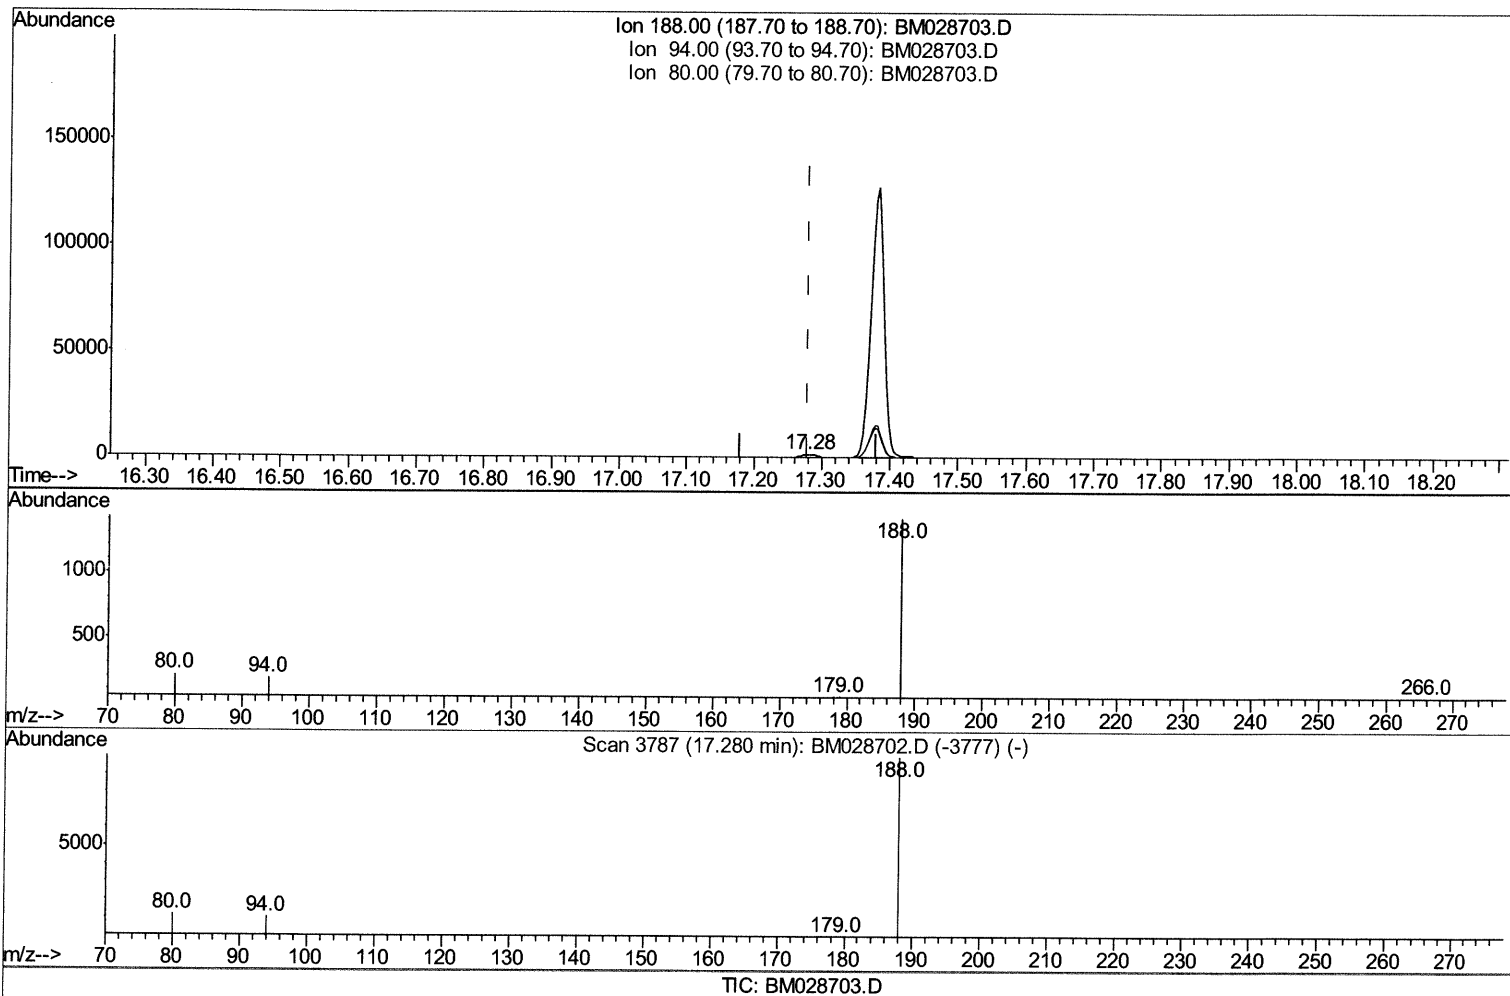

(10) Phenanthrene-d10 (I)

17.280min (-0.000) 0.40ng/ul m 02/12/21 JU

response 2084

Ion	Exp%	Act%
188.00	100	100
94.00	13.50	13.17
80.00	14.00	14.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021021\
Data File : BM028703.D
Acq On : 10 Feb 2021 14:27
Operator : CG/JU
Sample : PB134505BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK05

Manual Integrations
APPROVED

mohammad
2/11/2021 9:46:54 AM

Quant Time: Feb 10 14:59:16 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM020521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 10 14:28:04 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	500	0.40	ng/ul	0.00
2) Naphthalene-d8	10.70	136	1946	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.55	164	1058	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.28	188	2084m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.43	240	1767	0.40	ng/ul	0.00
20) Perylene-d12	23.66	264	1733	0.40	ng/ul	0.00

02/11/21 JU

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.29	152	1110	0.40	ng/ul	0.00
14) Fluoranthene-d10	19.29	212	1959	0.36	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed