


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM021021\
 Data File : BM028701.D
 Acq On : 10 Feb 2021 13:14
 Operator : CG/JU
 Sample : DFTPP26
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP26

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM020521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 10 14:28:04 2021

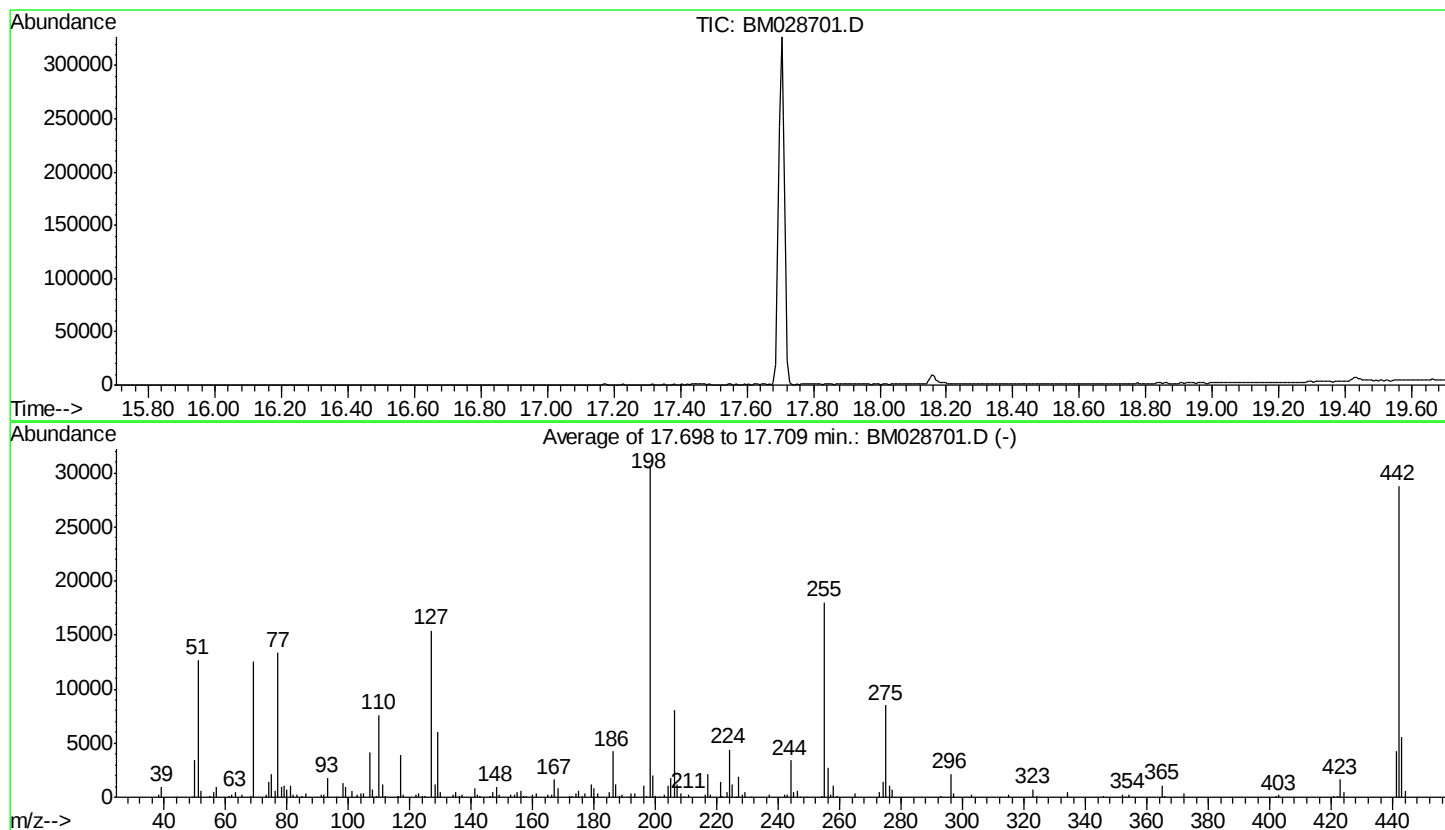

AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	12712	PASS
68	69	0.00	2	1.4	175	PASS
69	198	0.00	100	40.9	12526	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.3	15425	PASS
197	198	0.00	2	0.2	72	PASS
198	198	100	100	100.0	30653	PASS
199	198	5	9	6.8	2073	PASS
275	198	10	60	27.7	8477	PASS
365	198	1	100	3.5	1076	PASS
441	198	0.01	100	14.0	4283	PASS
442	198	50	100	94.0	28802	PASS
443	442	15	24	19.3	5568	PASS

Scan 2495 (17.662 min): BM028701.D
DFTPP26

m/z	Abundance
44.00	243.0
207.00	257.0

Instrument :
BNA_M
ClientSampleId :
DFTPP26

m/z	Abundance
38.00	201.0
39.10	1062.0
43.90	255.0
49.00	160.0
50.00	3541.0
51.00	13113.0
52.00	648.0
55.00	180.0
56.00	416.0
57.00	906.0
61.00	159.0
61.90	182.0
63.00	465.0
65.00	264.0
69.00	12654.0
72.90	273.0
74.00	1379.0
75.00	2060.0
76.00	672.0
77.10	13114.0
78.00	947.0
79.00	1062.0
80.00	786.0
81.00	980.0
81.90	244.0
83.00	243.0
85.00	204.0
86.00	340.0
91.00	209.0
91.90	273.0
93.00	1789.0
98.00	1316.0
99.00	936.0
101.00	595.0
102.90	226.0
104.00	298.0
105.00	380.0
107.00	4171.0
108.00	793.0
109.10	159.0
110.00	7475.0
111.00	1103.0
111.90	166.0
115.90	261.0
117.00	3709.0
117.90	317.0
122.00	255.0
122.90	382.0
123.90	216.0
125.00	230.0
127.00	14719.0
128.00	1156.0
129.00	5397.0
130.00	523.0
133.90	173.0
135.00	473.0
136.00	189.0
136.90	209.0
141.00	764.0
141.90	198.0
142.90	202.0
145.90	202.0
147.00	448.0
148.00	888.0
148.90	183.0
152.90	262.0
153.90	204.0
155.00	437.0
156.00	599.0
157.00	162.0
157.90	154.0
159.90	177.0
161.00	375.0
164.90	258.0
166.00	209.0
167.00	1603.0
168.00	803.0
173.00	187.0
173.90	321.0
175.00	553.0
177.00	285.0
178.90	1064.0
180.00	722.0
180.90	346.0
185.00	513.0
186.00	3851.0
187.00	1192.0
188.90	269.0
192.00	272.0
193.00	365.0
196.00	989.0
197.10	216.0

Instrument :
BNA_M
ClientSampleId :
DFTPP26

198.00	27328.0
199.00	1880.0
200.00	224.0
201.30	160.0
203.00	214.0
204.00	1001.0
205.00	1644.0
206.00	7037.0
207.10	1237.0
208.00	276.0
210.90	249.0
215.90	161.0
217.00	1848.0
218.00	251.0
221.00	1044.0
223.00	396.0
224.00	3788.0
225.00	991.0
227.00	1569.0
228.00	245.0
229.00	396.0
237.00	239.0
242.00	201.0
242.90	188.0
244.00	2931.0
244.90	380.0
246.00	484.0
254.10	201.0
255.00	15525.0
256.00	2345.0
257.00	226.0
257.90	849.0
258.90	199.0
264.90	290.0
273.00	425.0
274.00	1199.0
275.00	6871.0
276.00	914.0
277.00	574.0
296.00	1673.0
297.00	291.0
303.00	211.0
315.00	233.0
323.00	557.0
334.00	410.0
352.00	165.0
354.10	174.0
365.00	876.0
366.00	154.0
372.00	289.0
423.00	1111.0
424.00	356.0
441.00	2946.0
442.00	19432.0
443.00	3721.0
443.90	367.0

Instrument :
BNA_M
ClientSampleId :
DFTPP26

m/z	Abundance
38.00	206.0
39.00	1182.0
43.90	263.0
50.00	3861.0
51.10	15187.0
52.00	716.0
55.90	550.0
57.00	1044.0
61.00	174.0
62.00	242.0
63.00	605.0
65.00	301.0
68.10	312.0
69.00	14818.0
73.00	297.0
74.00	1586.0
75.00	2390.0
76.10	669.0
77.00	15880.0
78.10	1087.0
79.00	1245.0
80.00	833.0
81.00	1291.0
82.00	351.0
83.00	231.0
85.00	182.0
86.00	356.0
91.00	266.0
92.00	255.0
93.00	2096.0
95.90	155.0
98.00	1580.0
99.00	1103.0
100.90	637.0
103.00	201.0
104.00	495.0
105.00	430.0
107.00	4931.0
107.90	803.0
109.20	161.0
110.00	9195.0
111.00	1436.0
111.90	197.0
116.10	289.0
117.00	4639.0
118.00	340.0
121.90	384.0
123.00	473.0
123.90	195.0
125.00	252.0
127.00	17984.0
128.00	1490.0
129.00	7512.0
130.00	638.0
133.90	255.0
135.00	554.0
136.00	236.0
137.00	375.0
141.00	965.0
141.90	356.0
142.90	180.0
145.90	201.0
147.00	467.0
148.00	1211.0
149.00	268.0
152.90	364.0
154.00	298.0
155.00	510.0
156.00	708.0
156.90	178.0
158.00	168.0
160.00	319.0
160.90	412.0
164.90	342.0
165.90	228.0
167.00	1919.0
168.00	944.0
171.90	177.0
172.90	249.0
174.00	424.0
175.00	732.0
175.90	200.0
177.00	361.0
179.00	1334.0
180.00	1016.0
181.00	397.0
185.00	633.0
186.00	5048.0
187.00	1423.0
188.00	193.0
188.90	383.0
190.90	153.0

Instrument :
BNA_M
ClientSampleId :
DFTPP26

192.00	503.0
193.00	516.0
196.00	1072.0
198.00	36536.0
199.00	2511.0
200.00	194.0
202.90	209.0
204.00	1276.0
205.00	2072.0
206.00	10047.0
207.00	1631.0
208.00	331.0
208.90	151.0
210.90	396.0
215.90	207.0
217.00	2563.0
217.90	351.0
221.00	1854.0
221.70	365.0
223.00	541.0
224.00	5352.0
225.00	1424.0
226.00	165.0
227.00	2256.0
228.00	246.0
229.00	479.0
231.00	176.0
237.00	204.0
242.00	279.0
243.00	345.0
244.00	4090.0
245.00	624.0
246.00	750.0
246.90	155.0
248.90	182.0
254.00	215.0
255.00	21208.0
256.00	3113.0
257.00	305.0
258.00	1281.0
265.00	466.0
273.00	559.0
274.00	1647.0
275.00	9974.0
276.00	1224.0
277.00	832.0
293.00	166.0
296.00	2697.0
297.00	369.0
303.00	308.0
315.00	329.0
323.00	839.0
324.00	191.0
334.00	592.0
345.90	245.0
352.00	298.0
353.00	181.0
354.10	289.0
365.00	1229.0
365.90	155.0
372.00	535.0
402.00	204.0
403.00	279.0
420.90	217.0
421.90	238.0
423.00	1904.0
424.00	562.0
441.00	4955.0
442.00	33608.0
443.00	6648.0
444.00	659.0

Instrument :
BNA_M
ClientSampleId :
DFTPP26

m/z	Abundance
37.90	153.0
39.00	760.0
44.00	287.0
50.00	2759.0
51.00	9838.0
52.00	542.0
55.00	153.0
56.00	310.0
57.00	785.0
61.90	153.0
63.00	359.0
65.10	199.0
68.00	213.0
69.00	10108.0
73.10	283.0
74.00	1144.0
75.00	1780.0
76.10	519.0
77.10	10961.0
78.00	785.0
79.00	785.0
80.00	685.0
81.00	837.0
81.90	183.0
83.00	205.0
86.00	237.0
91.00	172.0
92.00	193.0
93.00	1480.0
98.00	1088.0
98.90	784.0
101.00	419.0
103.00	214.0
104.00	332.0
105.00	233.0
107.00	3433.0
108.00	605.0
109.10	150.0
110.00	6192.0
111.00	1035.0
116.00	222.0
117.00	3256.0
118.00	203.0
122.00	230.0
123.00	354.0
127.00	13572.0
128.00	1007.0
129.00	5064.0
130.00	399.0
134.00	250.0
134.90	424.0
136.90	222.0
141.00	821.0
141.90	228.0
147.00	378.0
148.00	770.0
148.90	167.0
153.00	250.0
153.90	169.0
155.00	378.0
156.00	518.0
158.00	155.0
159.90	160.0
161.00	363.0
165.00	251.0
166.00	174.0
167.00	1430.0
168.00	652.0
172.00	194.0
173.80	227.0
175.00	482.0
176.90	276.0
178.90	999.0
180.00	797.0
181.00	284.0
185.00	413.0
186.00	3834.0
187.00	1063.0
188.90	236.0
192.00	344.0
193.00	370.0
196.00	986.0
198.00	28096.0
199.00	1830.0
203.00	151.0
204.00	994.0
205.00	1722.0
206.00	7194.0
207.00	1301.0
208.00	342.0
210.90	241.0
216.00	247.0

Instrument :
BNA_M
ClientSampleId :
DFTPP26

217.00	1977.0
217.90	270.0
221.00	1473.0
223.00	499.0
224.00	4117.0
225.00	1206.0
227.00	1746.0
228.00	268.0
228.90	386.0
236.90	158.0
242.00	196.0
242.90	250.0
244.00	3254.0
245.00	415.0
245.90	639.0
255.00	17352.0
256.00	2699.0
256.90	178.0
258.00	922.0
259.00	153.0
265.00	396.0
273.00	554.0
274.00	1452.0
275.00	8588.0
276.00	1153.0
277.00	689.0
292.90	150.0
296.00	2189.0
296.90	314.0
303.00	247.0
314.90	212.0
323.00	775.0
334.00	514.0
345.90	158.0
352.00	236.0
354.00	265.0
365.00	1124.0
372.00	329.0
402.00	198.0
402.90	319.0
421.00	200.0
421.90	193.0
423.00	1812.0
424.00	521.0
441.00	4949.0
442.00	33368.0
443.00	6335.0
444.00	599.0

Instrument :
BNA_M
ClientSampleId :
DFTPP26