
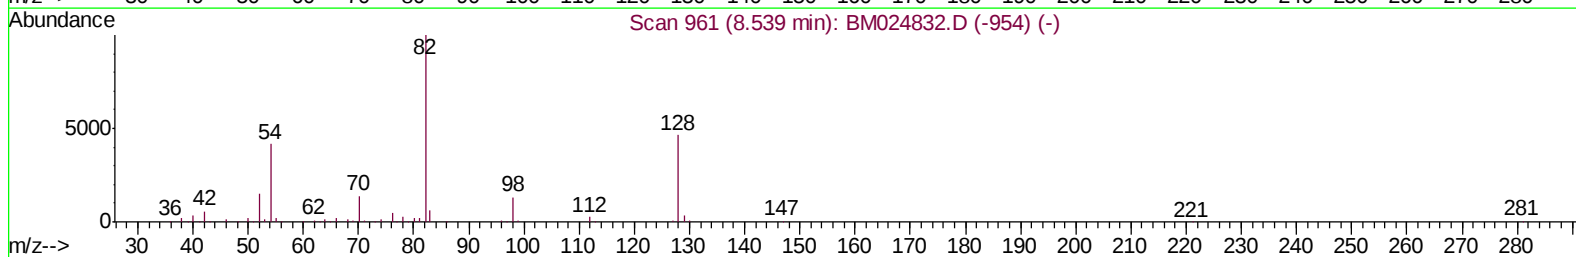
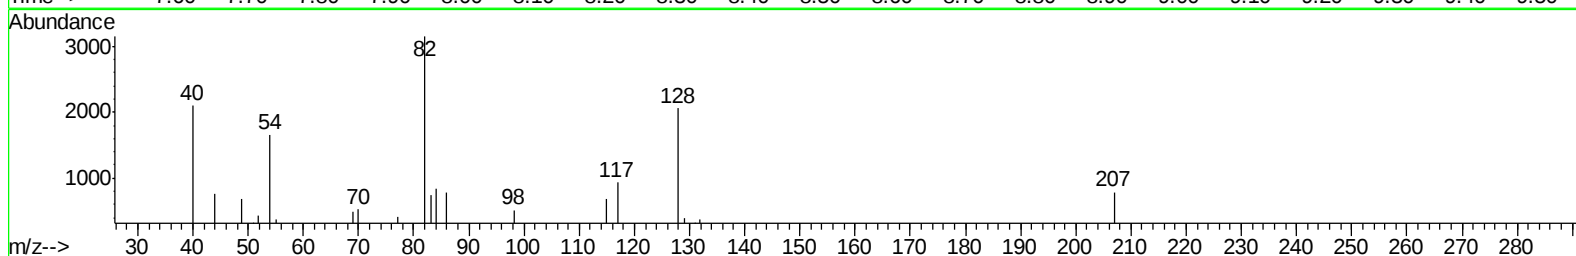


Data File : BM024836.D
Acq On : 11 Feb 2020 16:13
Operator : CG/JU
Sample : L1424-22DL 50X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Feb 12 04:12:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 12 04:09:26 2020
Response via : Initial Calibration

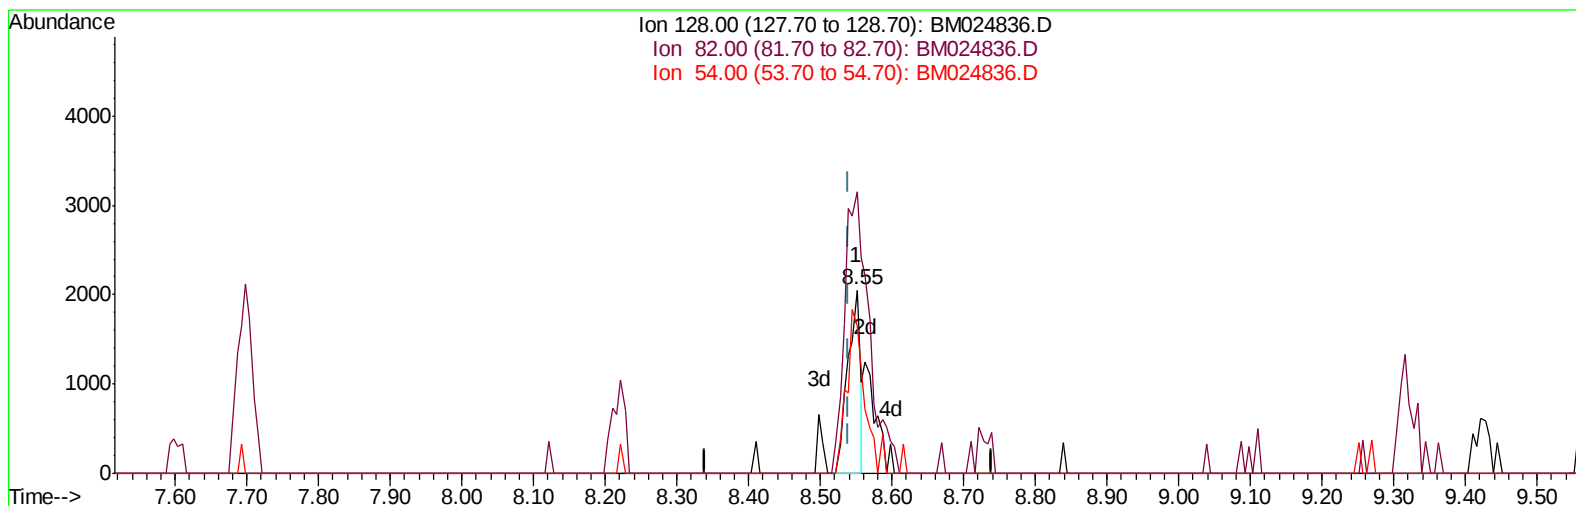

TIC: BM024836.D

(19) Nitrobenzene-d5 (S)

8.551min (+0.012) 0.39ng/ul

response 2509

Ion	Exp%	Act%
128.00	100	100
82.00	216.00	153.46#
54.00	87.00	80.57
0.00	0.00	0.00