
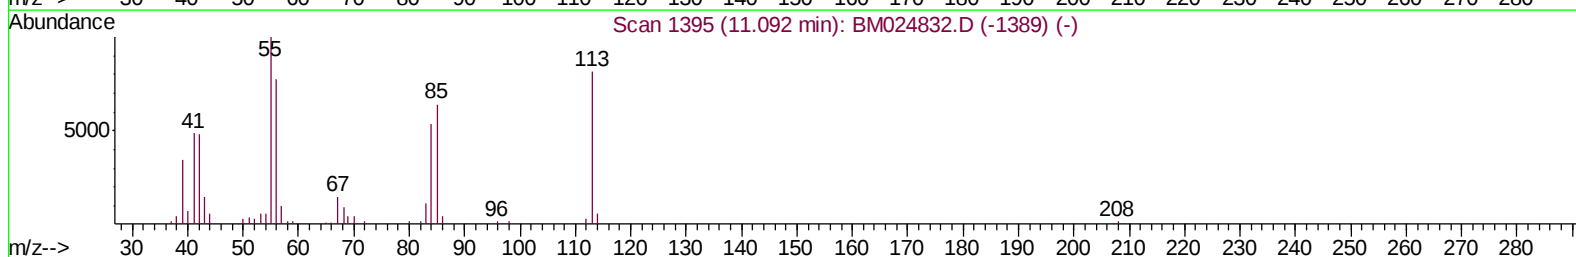
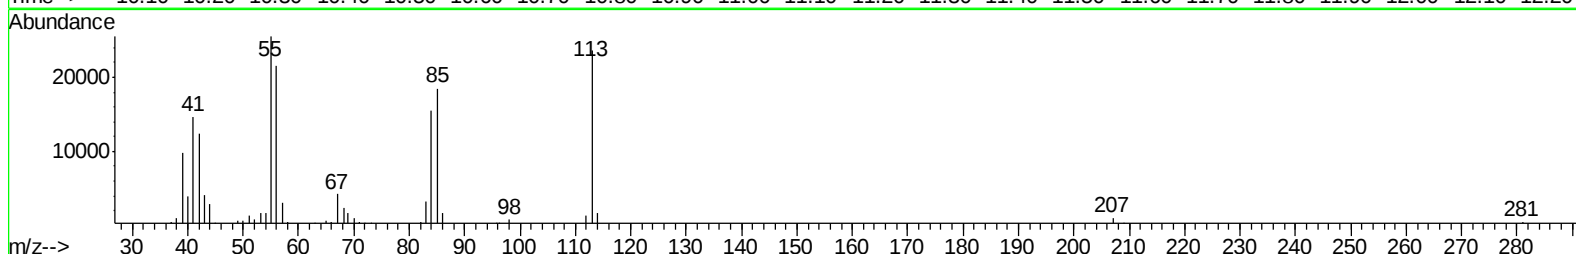


Data File : BM024837.D
Acq On : 11 Feb 2020 16:49
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Feb 12 04:12:17 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 12 04:09:26 2020
Response via : Initial Calibration

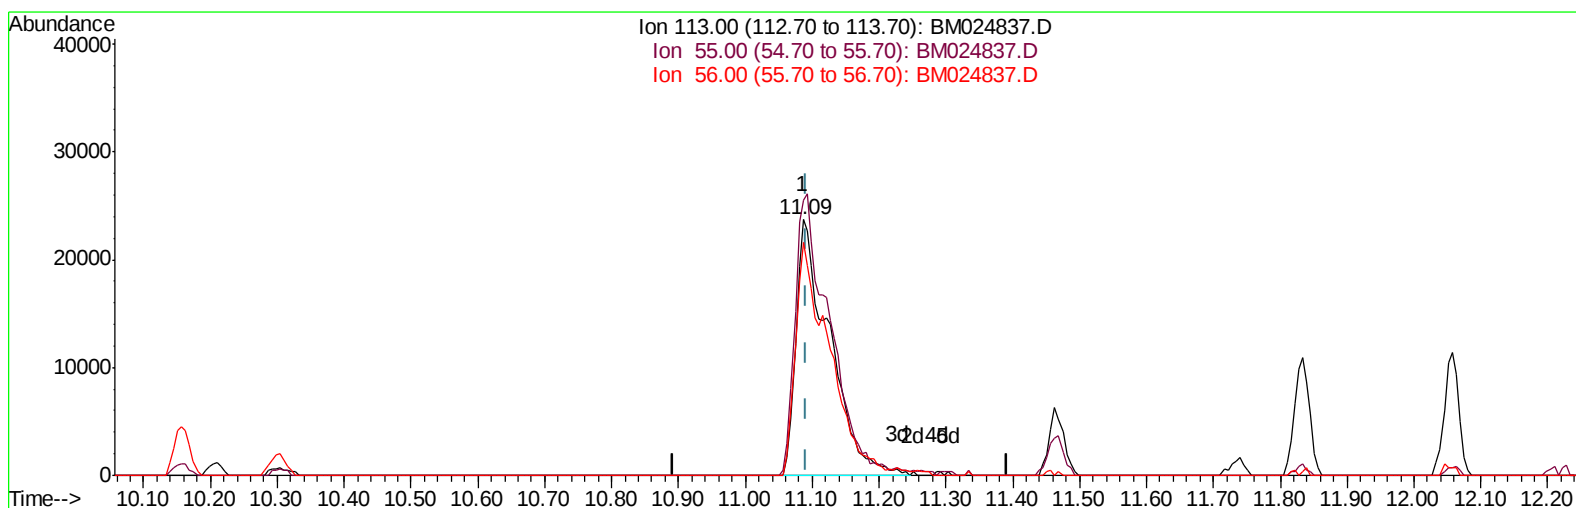

TIC: BM024837.D

(32) Caprolactam

11.086min (-0.006) 20.18ng/ul m

response 82176

Ion	Exp%	Act%
113.00	100	100
55.00	107.70	107.80
56.00	89.90	91.32
0.00	0.00	0.00