
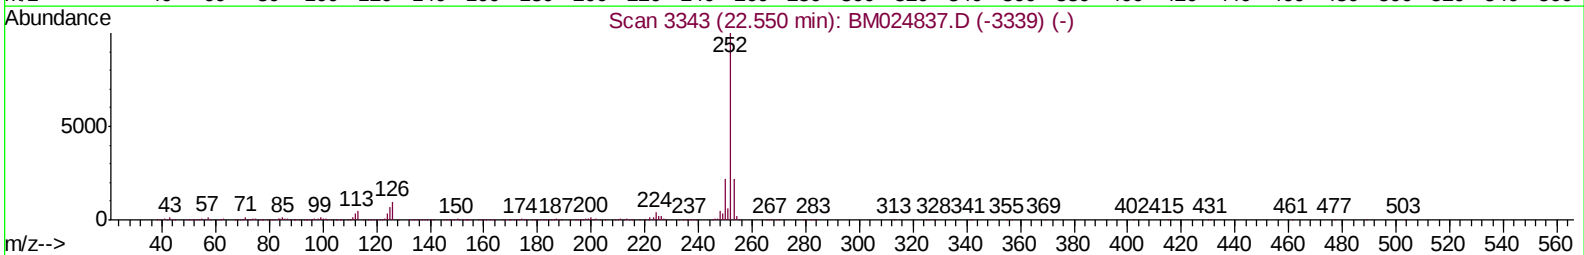
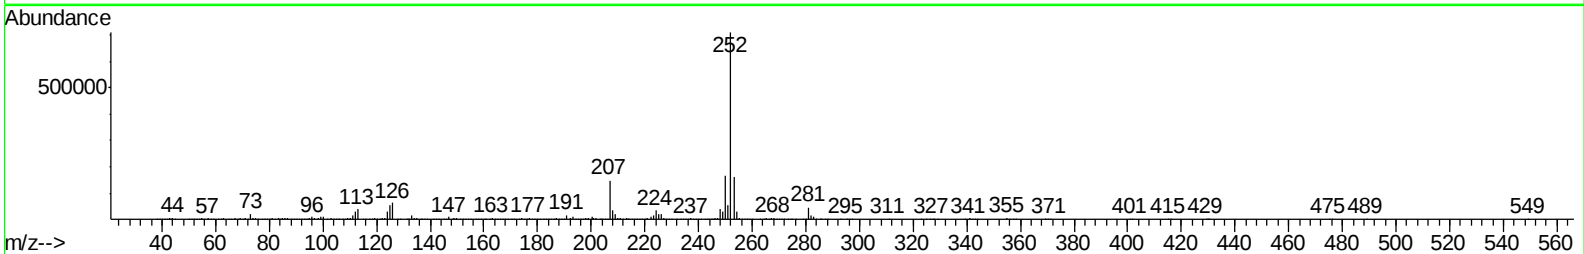


Data File : BM024839.D
Acq On : 11 Feb 2020 18:02
Operator : CG/JU
Sample : L1405-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Feb 12 04:42:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 12 04:40:07 2020
Response via : Initial Calibration

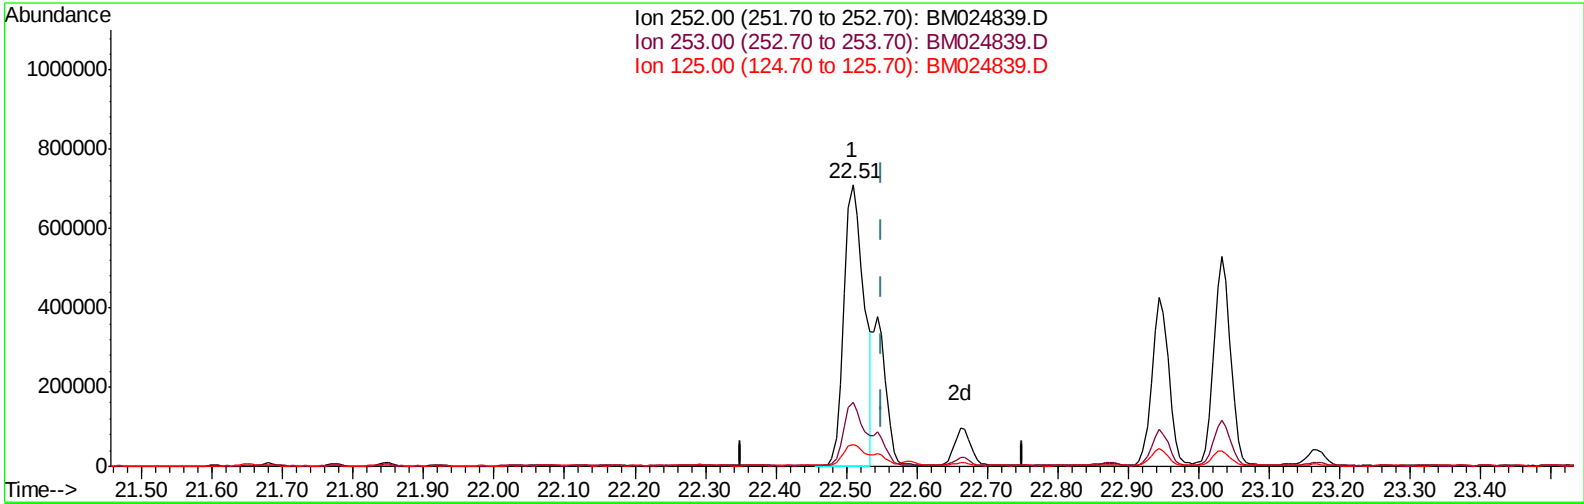

TIC: BM024839.D

(89) Benzo(k)fluoranthene

22.509min (-0.041) 15.68ng/ul

response 1394603

Ion	Exp%	Act%
252.00	100	100
253.00	21.70	22.52
125.00	6.40	7.82#
0.00	0.00	0.00